

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011911.D
 Acq On : 04 Oct 2022 14:26
 Operator : CG/JU
 Sample : N4859-23
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	28	rVB	4502737	5526275	77.13%	8.639%
2	3.299	49	53	61	rVB	55826	70715	0.99%	0.111%
3	3.728	125	126	144	rBV	122062	206755	2.89%	0.323%
4	3.952	159	164	170	rVB	27980	39887	0.56%	0.062%
5	4.046	176	180	187	rVB	20746	33434	0.47%	0.052%
6	5.511	423	429	437	rBV	27273	51181	0.71%	0.080%
7	6.363	569	574	580	rBV3	6095	10284	0.14%	0.016%
8	7.046	682	690	708	rBV	244551	431748	6.03%	0.675%
9	7.216	711	719	732	rBV	757236	1250474	17.45%	1.955%
10	7.410	745	752	763	rBV	706586	1177107	16.43%	1.840%
11	7.528	769	772	780	rVB2	11224	17833	0.25%	0.028%
12	7.887	825	833	842	rBV	773225	1283959	17.92%	2.007%
13	7.993	848	851	856	rVB4	6734	11067	0.15%	0.017%
14	8.263	889	897	902	rVB	11857	20585	0.29%	0.032%
15	8.593	946	953	968	rBV	660823	1154955	16.12%	1.806%
16	8.881	997	1002	1006	rBV2	7249	12803	0.18%	0.020%
17	8.963	1011	1016	1024	rBV	29124	54156	0.76%	0.085%
18	9.052	1024	1031	1044	rBV	804352	1354625	18.91%	2.118%
19	9.246	1057	1064	1072	rVB	21028	40690	0.57%	0.064%
20	9.363	1077	1084	1091	rVV5	10237	29435	0.41%	0.046%
21	9.434	1091	1096	1106	rVV	37884	71334	1.00%	0.112%
22	9.516	1106	1110	1115	rVV2	5963	9810	0.14%	0.015%
23	9.575	1115	1120	1126	rVB3	6596	9846	0.14%	0.015%
24	9.693	1133	1140	1144	rBV4	5517	10223	0.14%	0.016%
25	9.775	1147	1154	1169	rVV	590129	996855	13.91%	1.558%
26	9.881	1169	1172	1177	rVV6	8799	16457	0.23%	0.026%
27	9.940	1177	1182	1184	rVV6	5701	9940	0.14%	0.016%
28	9.969	1184	1187	1194	rVB3	9014	14297	0.20%	0.022%
29	10.099	1203	1209	1218	rVB3	18650	36898	0.51%	0.058%
30	10.187	1218	1224	1229	rBV4	10670	20148	0.28%	0.031%
31	10.316	1238	1246	1264	rBV	915031	1646439	22.98%	2.574%
32	10.552	1280	1286	1290	rBV5	8195	15256	0.21%	0.024%
33	10.693	1299	1310	1317	rBV	1069249	1811547	25.28%	2.832%
34	10.746	1317	1319	1326	rVB2	39447	59925	0.84%	0.094%
35	10.834	1326	1334	1348	rBV	670749	1354346	18.90%	2.117%
36	10.940	1348	1352	1357	rVV	46279	83396	1.16%	0.130%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011911.D
 Acq On : 04 Oct 2022 14:26
 Operator : CG/JU
 Sample : N4859-23
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	10.987	1357	1360	1368	rVB3	26148	46225	0.65%	0.072%
38	11.063	1368	1373	1376	rBV3	8169	12876	0.18%	0.020%
39	11.110	1376	1381	1387	rVV	39326	69976	0.98%	0.109%
40	11.169	1387	1391	1396	rVB2	10800	16176	0.23%	0.025%
41	11.281	1408	1410	1416	rVB3	8939	11072	0.15%	0.017%
42	11.463	1436	1441	1445	rBV5	11347	21382	0.30%	0.033%
43	11.516	1445	1450	1460	rVB4	15137	31734	0.44%	0.050%
44	11.604	1460	1465	1469	rBV6	7559	12873	0.18%	0.020%
45	11.810	1492	1500	1509	rVV2	70976	138897	1.94%	0.217%
46	11.887	1509	1513	1523	rVB4	12802	28462	0.40%	0.044%
47	12.022	1532	1536	1542	rVB5	9149	17935	0.25%	0.028%
48	12.175	1558	1562	1569	rBV4	5942	13167	0.18%	0.021%
49	12.251	1569	1575	1579	rBV	37212	71492	1.00%	0.112%
50	12.410	1597	1602	1607	rBV3	14616	21373	0.30%	0.033%
51	12.475	1607	1613	1617	rVV6	6599	14878	0.21%	0.023%
52	12.575	1617	1630	1639	rVV2	87465	191972	2.68%	0.300%
53	12.681	1639	1648	1657	rVB2	9269	27749	0.39%	0.043%
54	13.063	1706	1713	1716	rBV8	4897	11109	0.16%	0.017%
55	13.363	1759	1764	1769	rVV3	23826	44442	0.62%	0.069%
56	13.428	1769	1775	1784	rVB2	21965	40042	0.56%	0.063%
57	13.504	1784	1788	1790	rBV5	6499	9255	0.13%	0.014%
58	13.540	1790	1794	1797	rVV3	10823	14902	0.21%	0.023%
59	13.587	1797	1802	1810	rVB2	36533	61153	0.85%	0.096%
60	13.704	1813	1822	1830	rBV2	23253	54709	0.76%	0.086%
61	13.851	1840	1847	1854	rBV6	22353	52786	0.74%	0.083%
62	13.940	1855	1862	1874	rBV	1853852	2703898	37.74%	4.227%
63	14.087	1882	1887	1890	rBV	57702	86747	1.21%	0.136%
64	14.122	1890	1893	1898	rVB	45782	62256	0.87%	0.097%
65	14.222	1904	1910	1926	rBV	2163918	3300105	46.06%	5.159%
66	14.534	1956	1963	1968	rBV	1520774	2193344	30.61%	3.429%
67	14.592	1968	1973	1984	rVB	708674	1069681	14.93%	1.672%
68	14.740	1993	1998	2011	rBV	84548	198581	2.77%	0.310%
69	14.840	2011	2015	2020	rVB	31817	48432	0.68%	0.076%
70	14.934	2026	2031	2038	rVB	57697	95497	1.33%	0.149%
71	15.145	2062	2067	2073	rVB7	13852	27034	0.38%	0.042%
72	15.369	2101	2105	2110	rBV2	15338	26636	0.37%	0.042%
73	15.528	2125	2132	2137	rBV	3025253	4377183	61.09%	6.843%
74	15.569	2137	2139	2146	rVB2	112736	173819	2.43%	0.272%
75	15.645	2146	2152	2159	rBV	785634	1117762	15.60%	1.747%
76	15.710	2160	2163	2166	rVB	13198	13698	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011911.D
 Acq On : 04 Oct 2022 14:26
 Operator : CG/JU
 Sample : N4859-23
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

77	15.875	2188	2191	2203	rVB4	30734	54884	0.77%	0.086%
78	15.987	2205	2210	2213	rBV4	11375	18811	0.26%	0.029%
79	16.022	2213	2216	2225	rVB2	29944	51243	0.72%	0.080%
80	16.104	2225	2230	2231	rBV2	8641	15189	0.21%	0.024%
81	16.222	2244	2250	2251	rBV5	6365	10233	0.14%	0.016%
82	16.263	2253	2257	2263	rVB2	30621	46828	0.65%	0.073%
83	16.381	2273	2277	2283	rVB5	10857	16477	0.23%	0.026%
84	16.745	2334	2339	2342	rBV2	12786	18065	0.25%	0.028%
85	17.104	2397	2400	2404	rBV	9051	9678	0.14%	0.015%
86	17.169	2408	2411	2417	rBV7	7983	13425	0.19%	0.021%
87	17.245	2421	2424	2425	rBV2	10862	11135	0.16%	0.017%
88	17.286	2425	2431	2437	rVV	1789459	2591012	36.16%	4.051%
89	17.328	2437	2438	2442	rVB	42803	38240	0.53%	0.060%
90	17.386	2442	2448	2459	rBV	3556479	5051119	70.50%	7.896%
91	17.692	2493	2500	2504	rBV2	14633	32348	0.45%	0.051%
92	18.169	2577	2581	2585	rBV4	61627	87138	1.22%	0.136%
93	18.345	2606	2611	2616	rBV4	25850	47073	0.66%	0.074%
94	19.198	2753	2756	2761	rVB2	46254	62151	0.87%	0.097%
95	19.269	2764	2768	2770	rBV	54599	69027	0.96%	0.108%
96	19.404	2788	2791	2795	rBV4	43366	52197	0.73%	0.082%
97	19.622	2822	2828	2842	rBV	4815881	6515409	90.93%	10.186%
98	21.374	3121	3126	3136	rBV	2589368	3275256	45.71%	5.120%
99	23.651	3506	3513	3527	rVB2	3568997	7165130	100.00%	11.201%
100	23.810	3534	3540	3549	rVB2	1621270	3239362	45.21%	5.064%




Sum of corrected areas: 63967425

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011911.D
Acq On : 04 Oct 2022 14:26
Operator : CG/JU
Sample : N4859-23
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

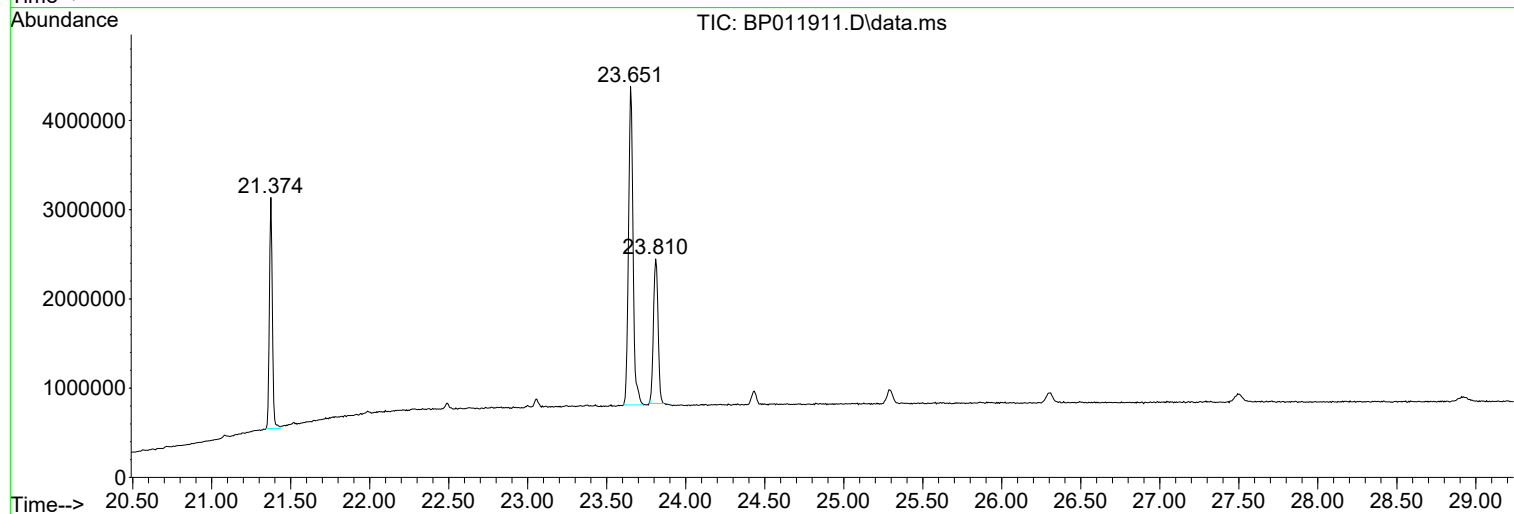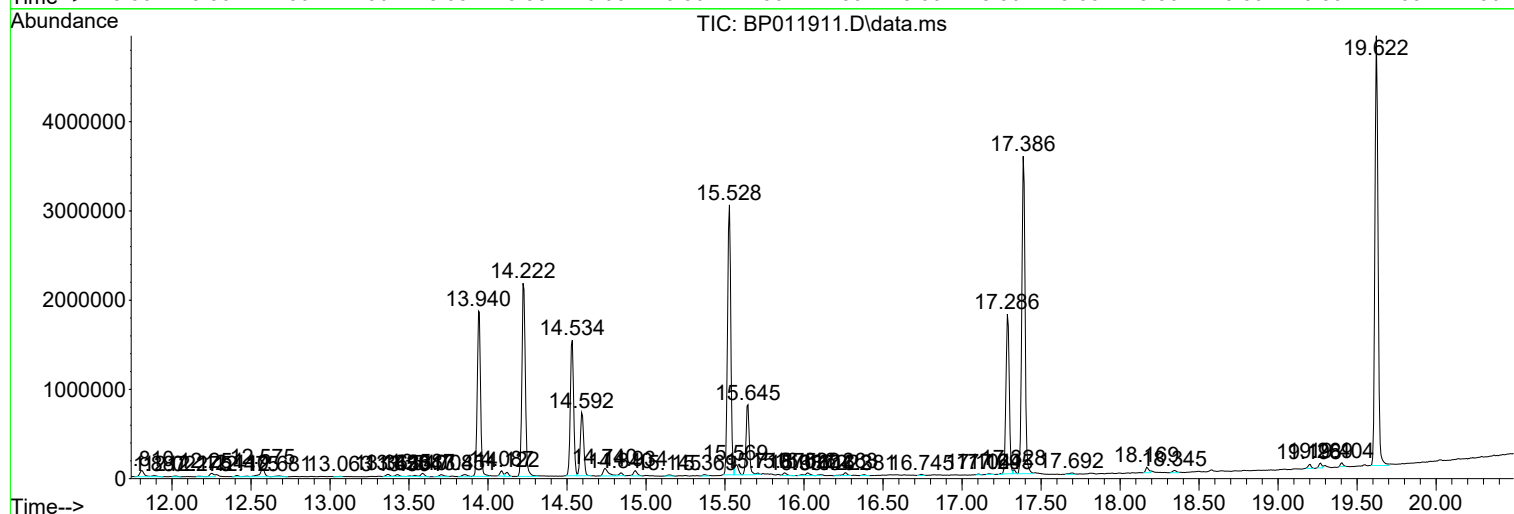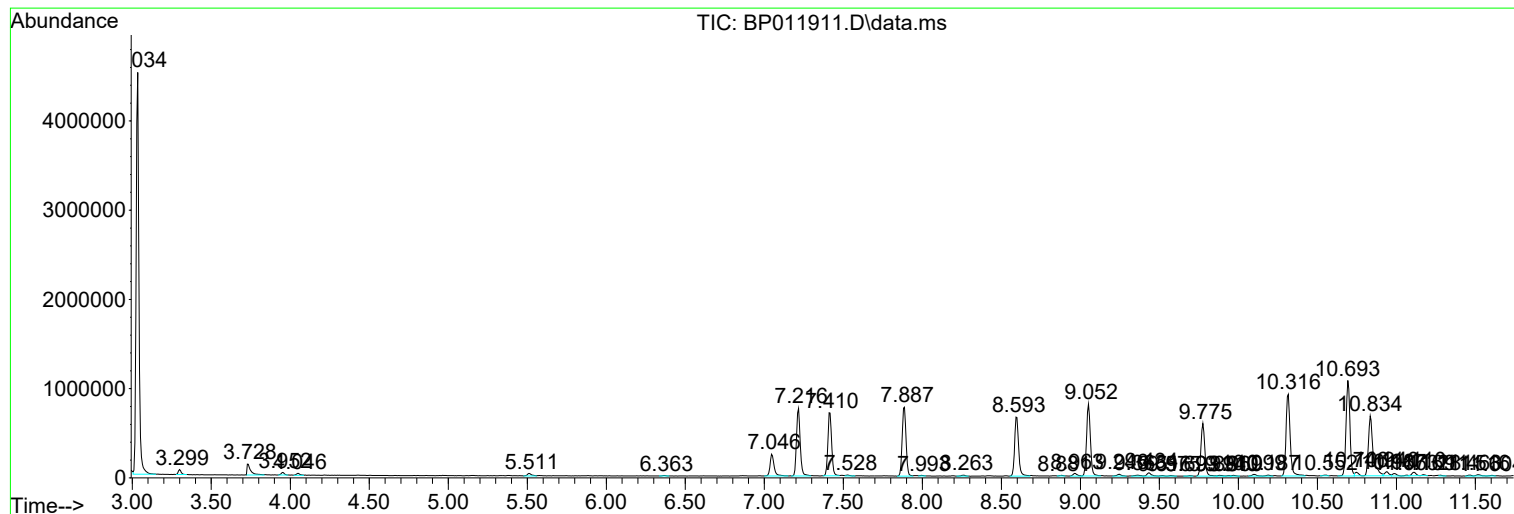

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011911.D
Acq On : 04 Oct 2022 14:26
Operator : CG/JU
Sample : N4859-23
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10054










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	86.08 ng/ul	5526280	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

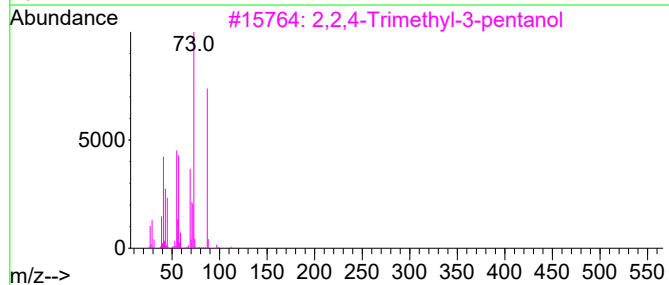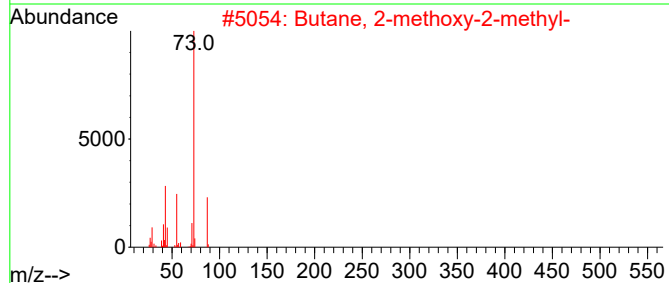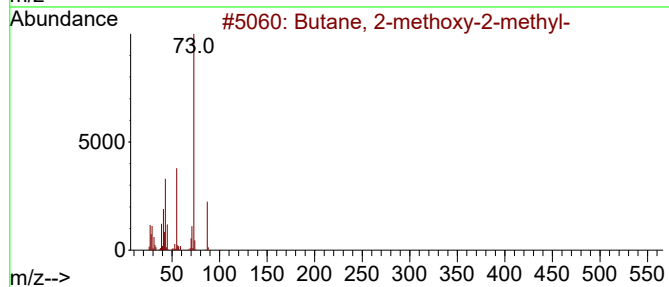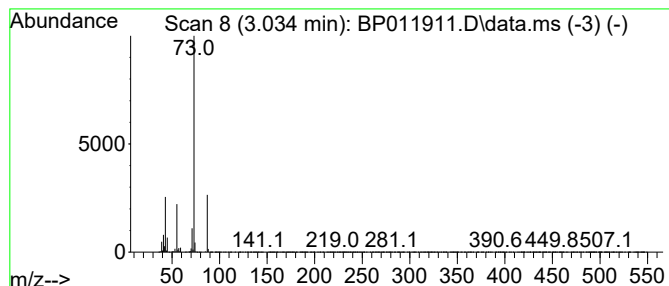

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011911.D
Acq On : 04 Oct 2022 14:26
Operator : CG/JU
Sample : N4859-23
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	86.1	ng/ul	5526280	1	7.887	1283960	20.0