

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100419\
 Data File : BP000510.D
 Acq On : 04 Oct 2019 16:24
 Operator : JU
 Sample : PB123656BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB123656BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	557	562	565	rBV	4072647	3833849	67.95%	9.571%
2	6.405	729	734	737	rBV	3724985	3762516	66.69%	9.393%
3	6.540	752	757	760	rBV	4430746	3911881	69.33%	9.766%
4	6.764	792	795	799	rBV	1198364	991852	17.58%	2.476%
5	6.922	818	822	825	rBV	4334962	3536194	62.67%	8.828%
6	7.328	886	891	893	rBV	2683193	2557458	45.33%	6.385%
7	8.046	1010	1013	1017	rBV	1623726	1359906	24.10%	3.395%
8	9.128	1193	1197	1200	rBV	6323202	5642172	100.00%	14.086%
9	9.810	1309	1313	1316	rBV	2184552	1716475	30.42%	4.285%
10	10.605	1444	1448	1472	rBV	3086379	2762855	48.97%	6.898%
11	11.305	1563	1567	1571	rBV	1419199	1263891	22.40%	3.155%
12	12.916	1836	1841	1844	rBV	5776971	5240548	92.88%	13.083%
13	13.975	2017	2021	2034	rVB	1555629	1447970	25.66%	3.615%
14	15.122	2211	2216	2225	rBV	85175	104285	1.85%	0.260%
15	15.457	2267	2273	2278	rBV	1232682	1496635	26.53%	3.736%
16	15.504	2278	2281	2291	rVB	126955	170970	3.03%	0.427%
17	15.945	2351	2356	2366	rBV	96533	158424	2.81%	0.396%
18	16.463	2437	2444	2455	rBV	45024	97215	1.72%	0.243%


Sum of corrected areas: 40055096

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100419\
Data File : BP000510.D
Acq On : 04 Oct 2019 16:24
Operator : JU
Sample : PB123656BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123656BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

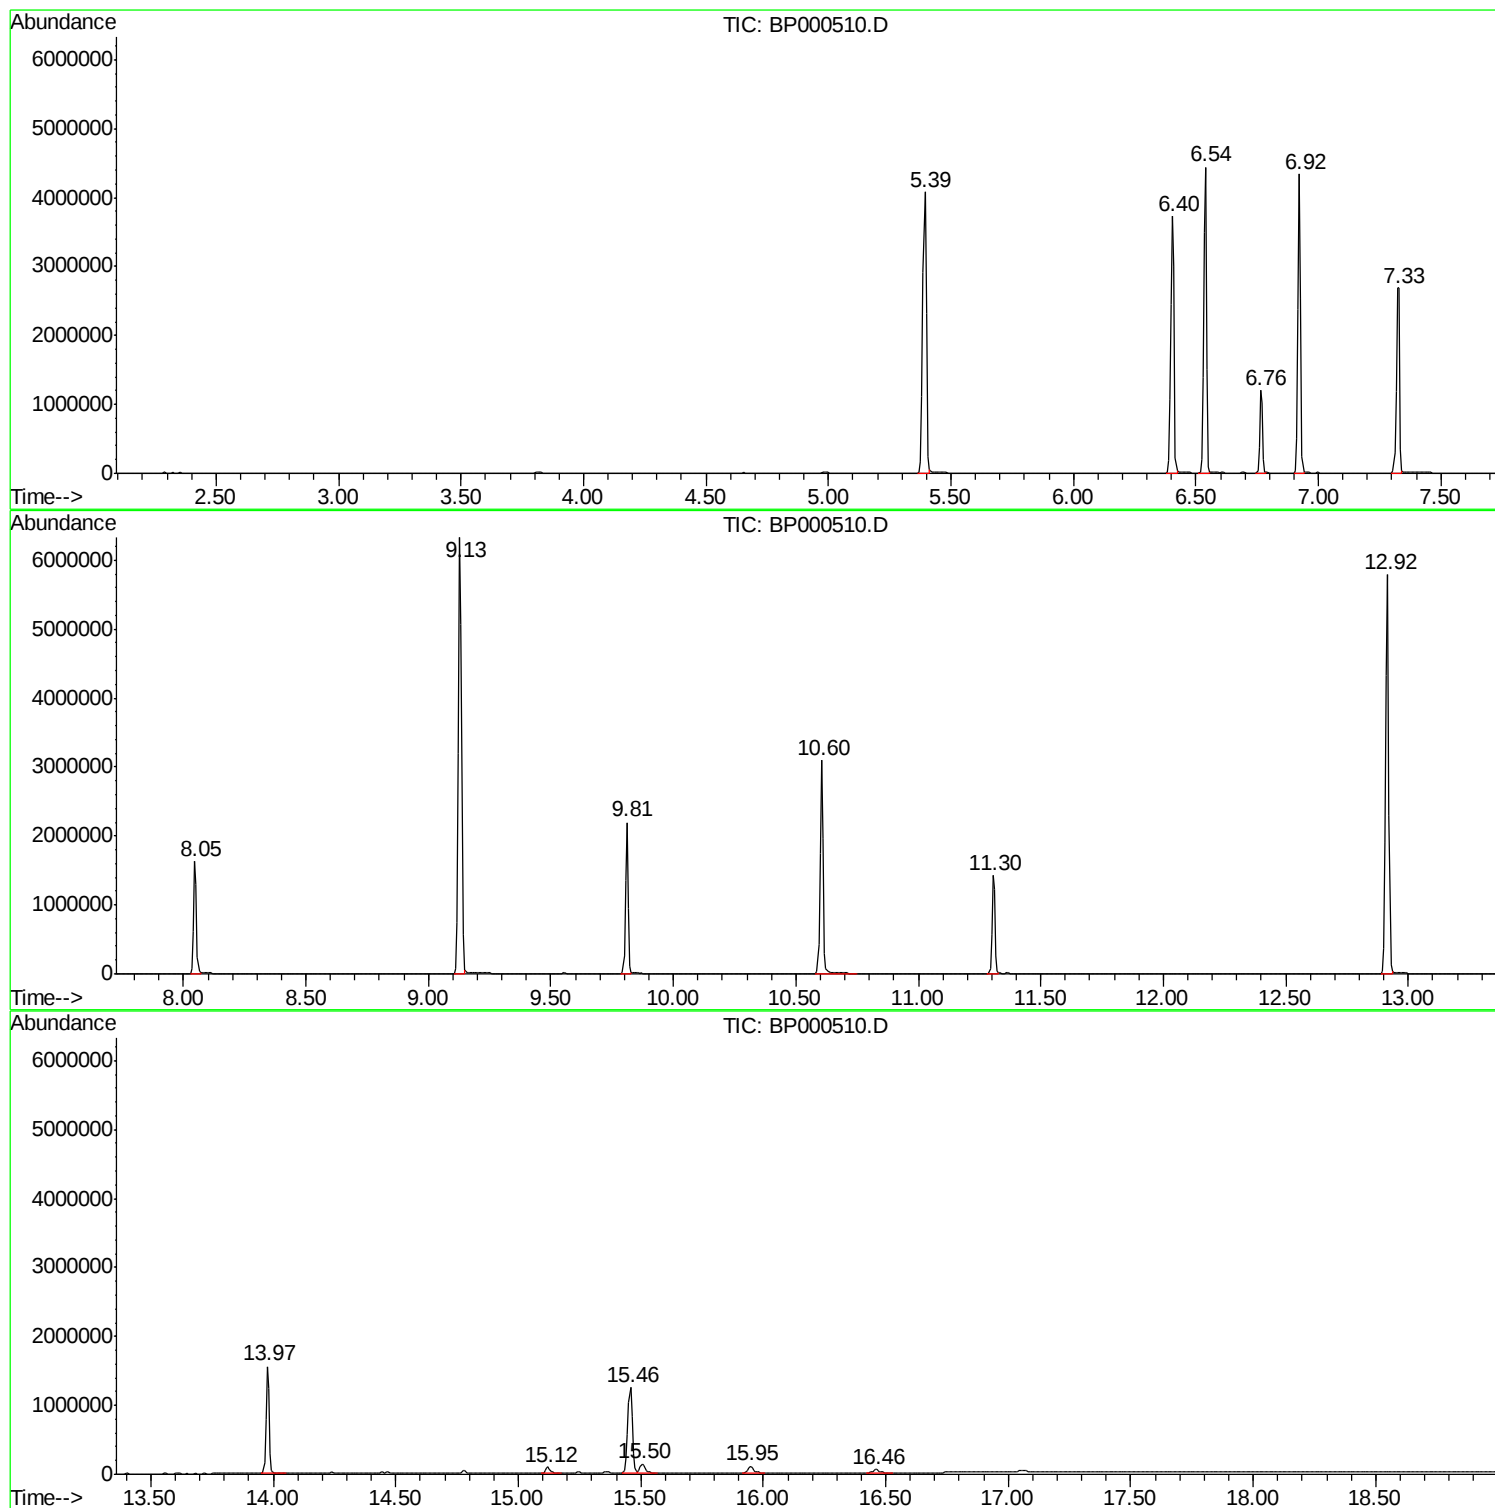

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100419\
Data_File : BP000510.D
Acq_On : 04 Oct 2019 16:244
Operator : JUJ
Sample : PB123656BLL
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
PB123656BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
