


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100419\
 Data File : BP000507.D
 Acq On : 04 Oct 2019 14:48
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 01 18:03:42 2019

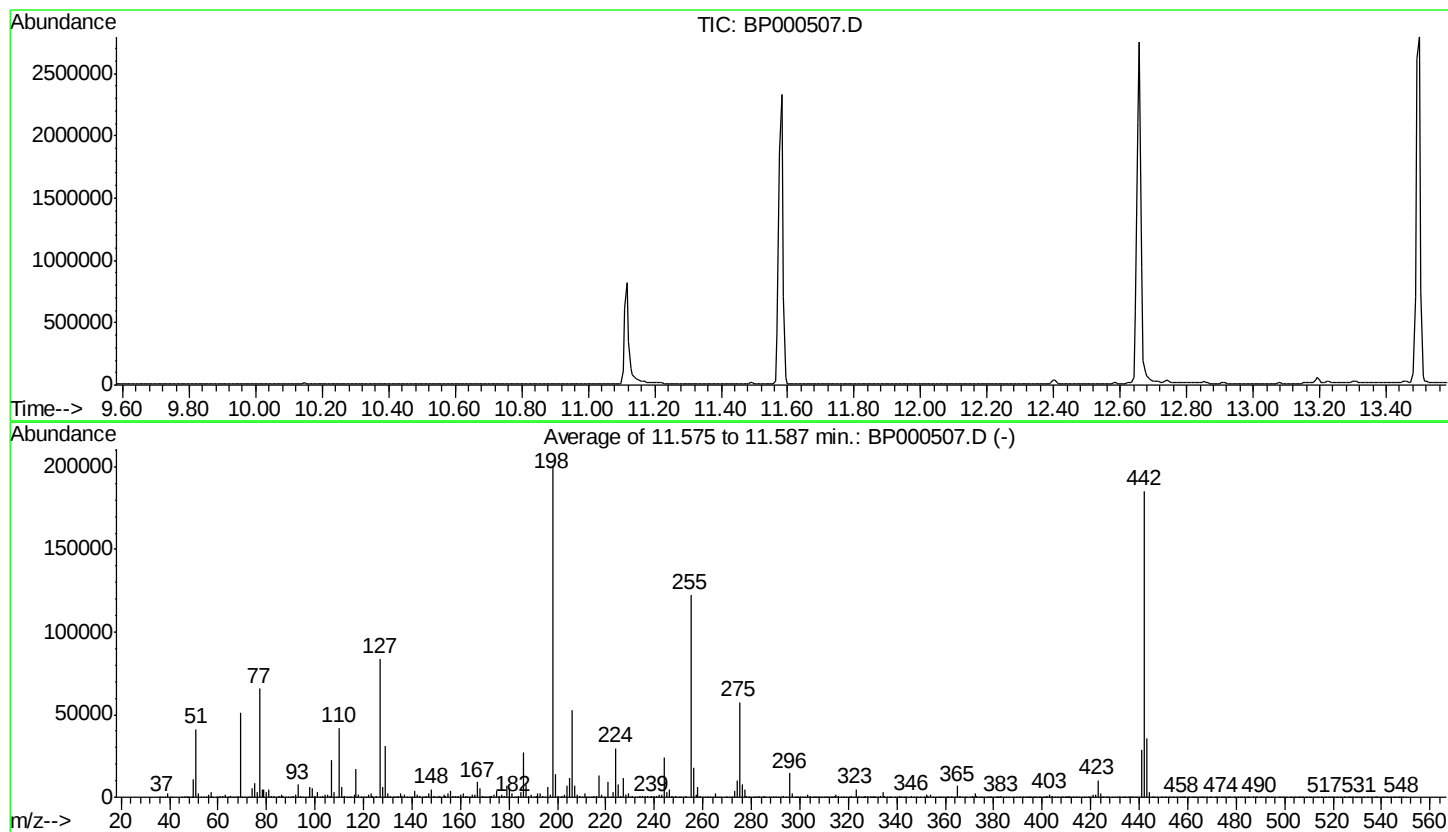

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.5	41199	PASS
68	69	0.00	2	1.9	967	PASS
69	198	0.00	100	25.4	51082	PASS
70	69	0.00	2	0.5	278	PASS
127	198	10	80	41.8	83909	PASS
197	198	0.00	2	0.6	1197	PASS
198	198	100	100	100.0	200725	PASS
199	198	5	9	6.9	13759	PASS
275	198	10	60	28.7	57670	PASS
365	198	1	100	3.5	6970	PASS
441	198	0.01	100	14.3	28784	PASS
442	198	50	100	92.3	185280	PASS
443	442	15	24	19.2	35581	PASS