

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017542.D
 Acq On : 04 Oct 2023 20:32
 Operator : MA/JU
 Sample : 04679-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PMW-4(20230927)MS

Quant Time: Oct 05 00:40:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 04 16:33:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	103869	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	424633	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	261477	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	598322	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	636925	20.000	ng/ul	0.00
88) Perylene-d12	24.133	264	720048	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	12686	4.883	ng/uL	0.00
4) Pyridine-d5	3.728	84	122847	18.065	ng/ul	0.00
7) Phenol-d5	7.099	99	100550	11.506	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	259301	48.625	ng/ul	0.00
11) 2-Chlorophenol-d4	7.464	132	266521	38.732	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	209599	29.959	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	163111	49.930	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	182830	49.621	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.393	165	318928	46.690	ng/ul	0.00
31) 4-Chloroaniline-d4	10.952	131	359491	36.944	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	1124517	55.134	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	1198710	53.299	ng/ul	0.00
54) 4-Nitrophenol-d4	14.881	143	31181	8.730	ng/ul	0.00
60) Fluorene-d10	15.640	176	946008	54.683	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.775	200	174071	46.667	ng/ul	0.00
73) Anthracene-d10	17.522	188	1559443	56.306	ng/ul	0.00
81) Pyrene-d10	19.775	212	2072364	58.555	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.969	264	2081851	57.291	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	11.805	113	6049	2.939	ng/ul	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017542.D
Acq On : 04 Oct 2023 20:32
Operator : MA/JU
Sample : 04679-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PMW-4(20230927)MS

Quant Time: Oct 05 00:40:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 04 16:33:47 2023
Response via : Initial Calibration

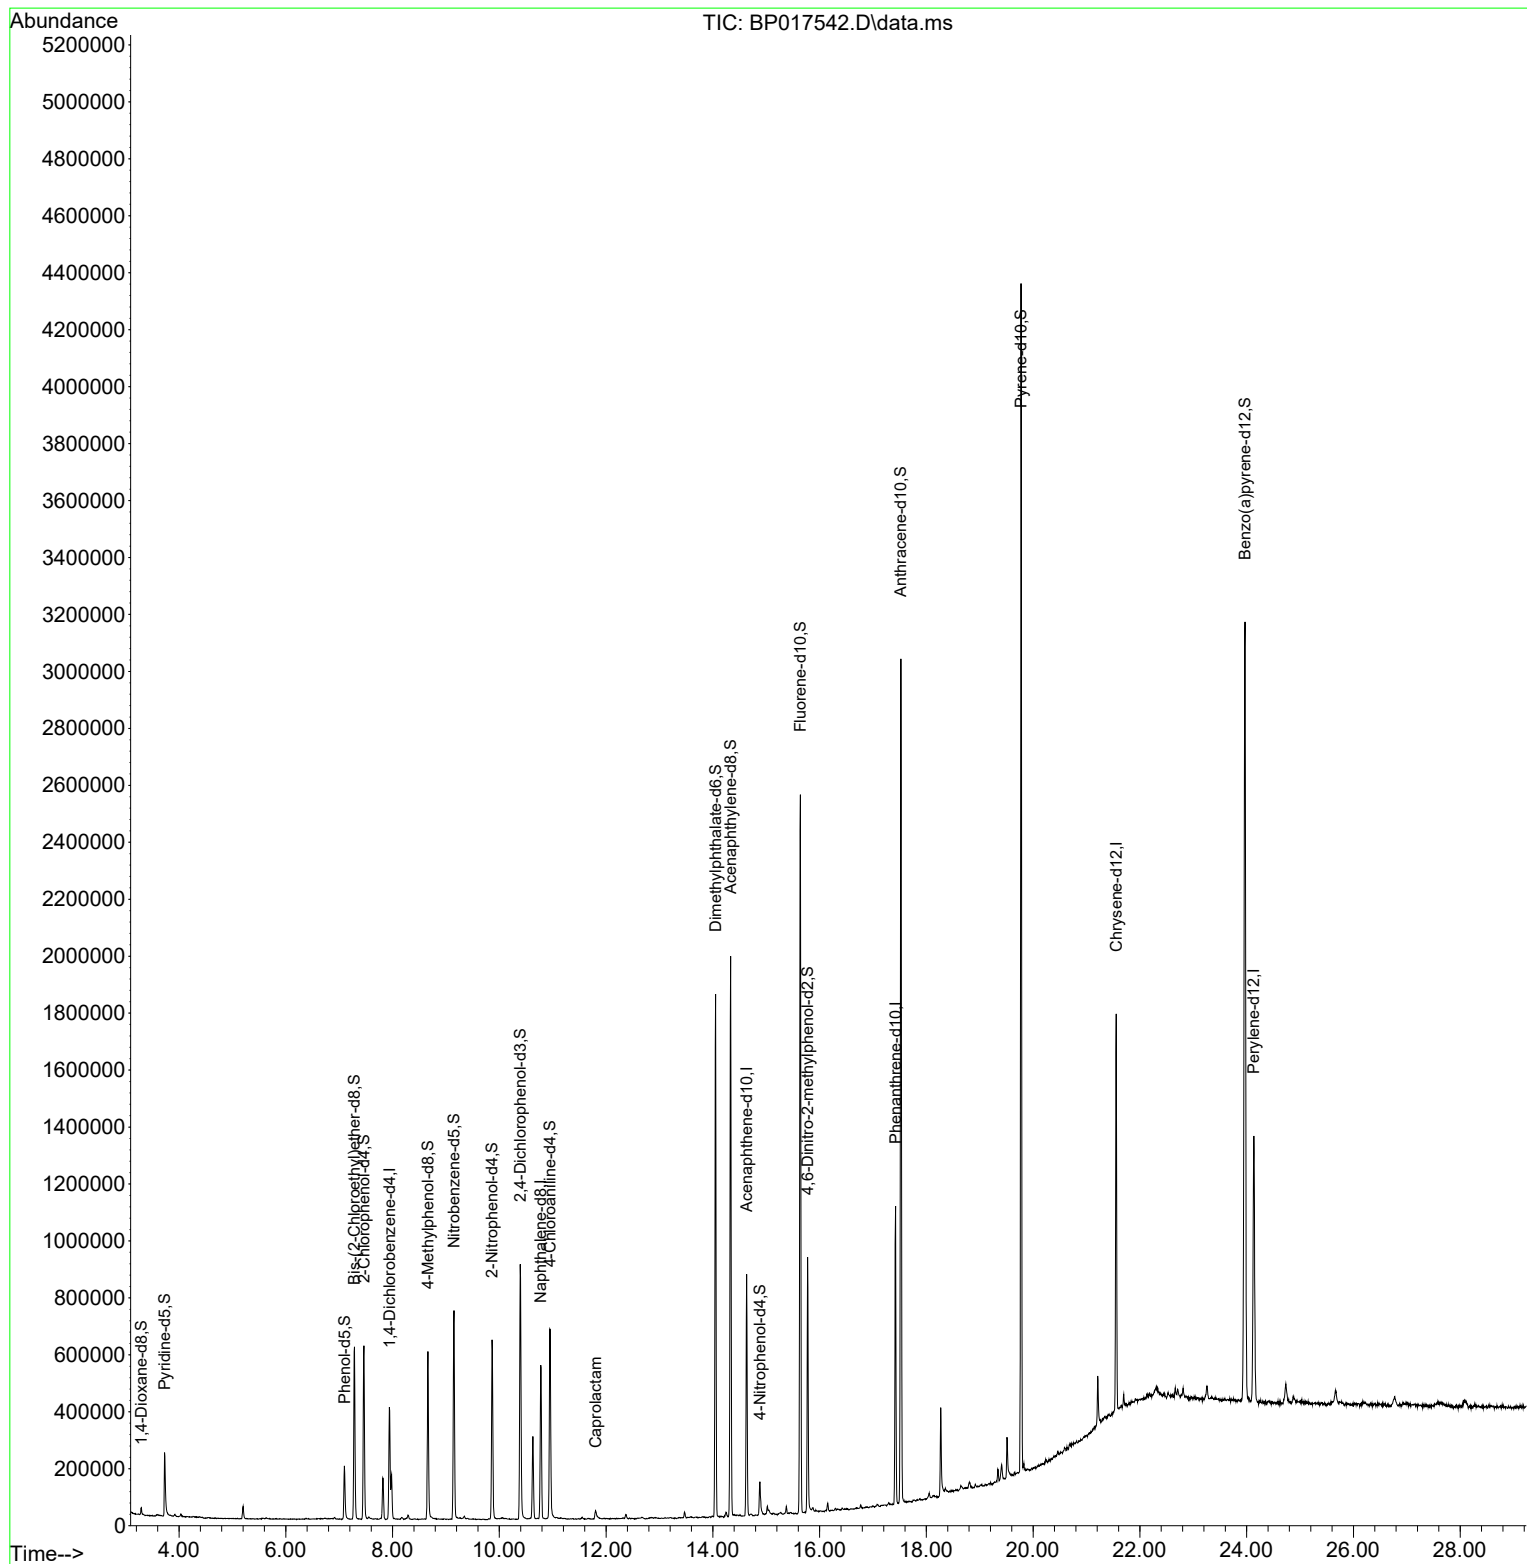

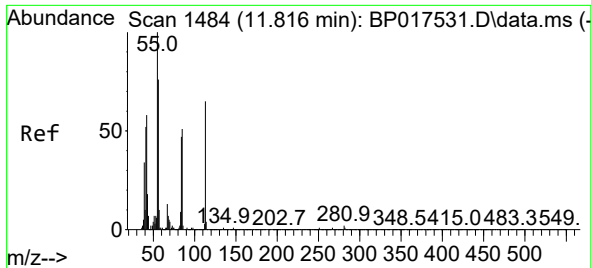

#34
Caprolactam
Concen: 2.939 ng/ul
RT: 11.805 min Scan# 14
Delta R.T. -0.012 min
Lab File: BP017542.D
Acq: 04 Oct 2023 20:32

Instrument :
BNA_P
ClientSampleId :
PMW-4(20230927)MS

Tgt Ion:113 Resp: 6049
Ion Ratio Lower Upper
113 100
55 181.1 124.6 187.0
56 129.3 94.7 142.1

