

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017557.D
 Acq On : 05 Oct 2023 10:11
 Operator : MA/JU
 Sample : 04679-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PMW-8D(20230928)

Quant Time: Oct 06 01:58:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 04 16:33:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	97724	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	406520	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.646	164	260437	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.434	188	611474	20.000	ng/u1	0.00
79) Chrysene-d12	21.569	240	642725	20.000	ng/u1	0.00
88) Perylene-d12	24.157	264	727987	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	12217	4.998	ng/uL	0.00
4) Pyridine-d5	3.734	84	73925	11.554	ng/u1	0.00
7) Phenol-d5	7.105	99	70177	8.535	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	216190	43.090	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	215129	33.229	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	138246	21.003	ng/u1	0.00
21) Nitrobenzene-d5	9.158	128	136319	43.588	ng/u1	0.00
24) 2-Nitrophenol-d4	9.875	143	147256	41.746	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.405	165	256404	39.209	ng/u1	0.00
31) 4-Chloroaniline-d4	10.958	131	317544	34.087	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	986045	48.538	ng/u1	0.00
49) Acenaphthylene-d8	14.340	160	1016771	45.390	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	31676	8.904	ng/u1	0.02
60) Fluorene-d10	15.646	176	847756	49.199	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	169300	44.411	ng/u1	0.00
73) Anthracene-d10	17.534	188	1672797	59.100	ng/u1	0.00
81) Pyrene-d10	19.786	212	2173568	60.860	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.992	264	2278314	62.014	ng/u1	0.02
Target Compounds						
2) 1,4-Dioxane	3.329	88	57699	22.963	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017557.D
Acq On : 05 Oct 2023 10:11
Operator : MA/JU
Sample : 04679-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PMW-8D(20230928)

Quant Time: Oct 06 01:58:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 04 16:33:47 2023
Response via : Initial Calibration

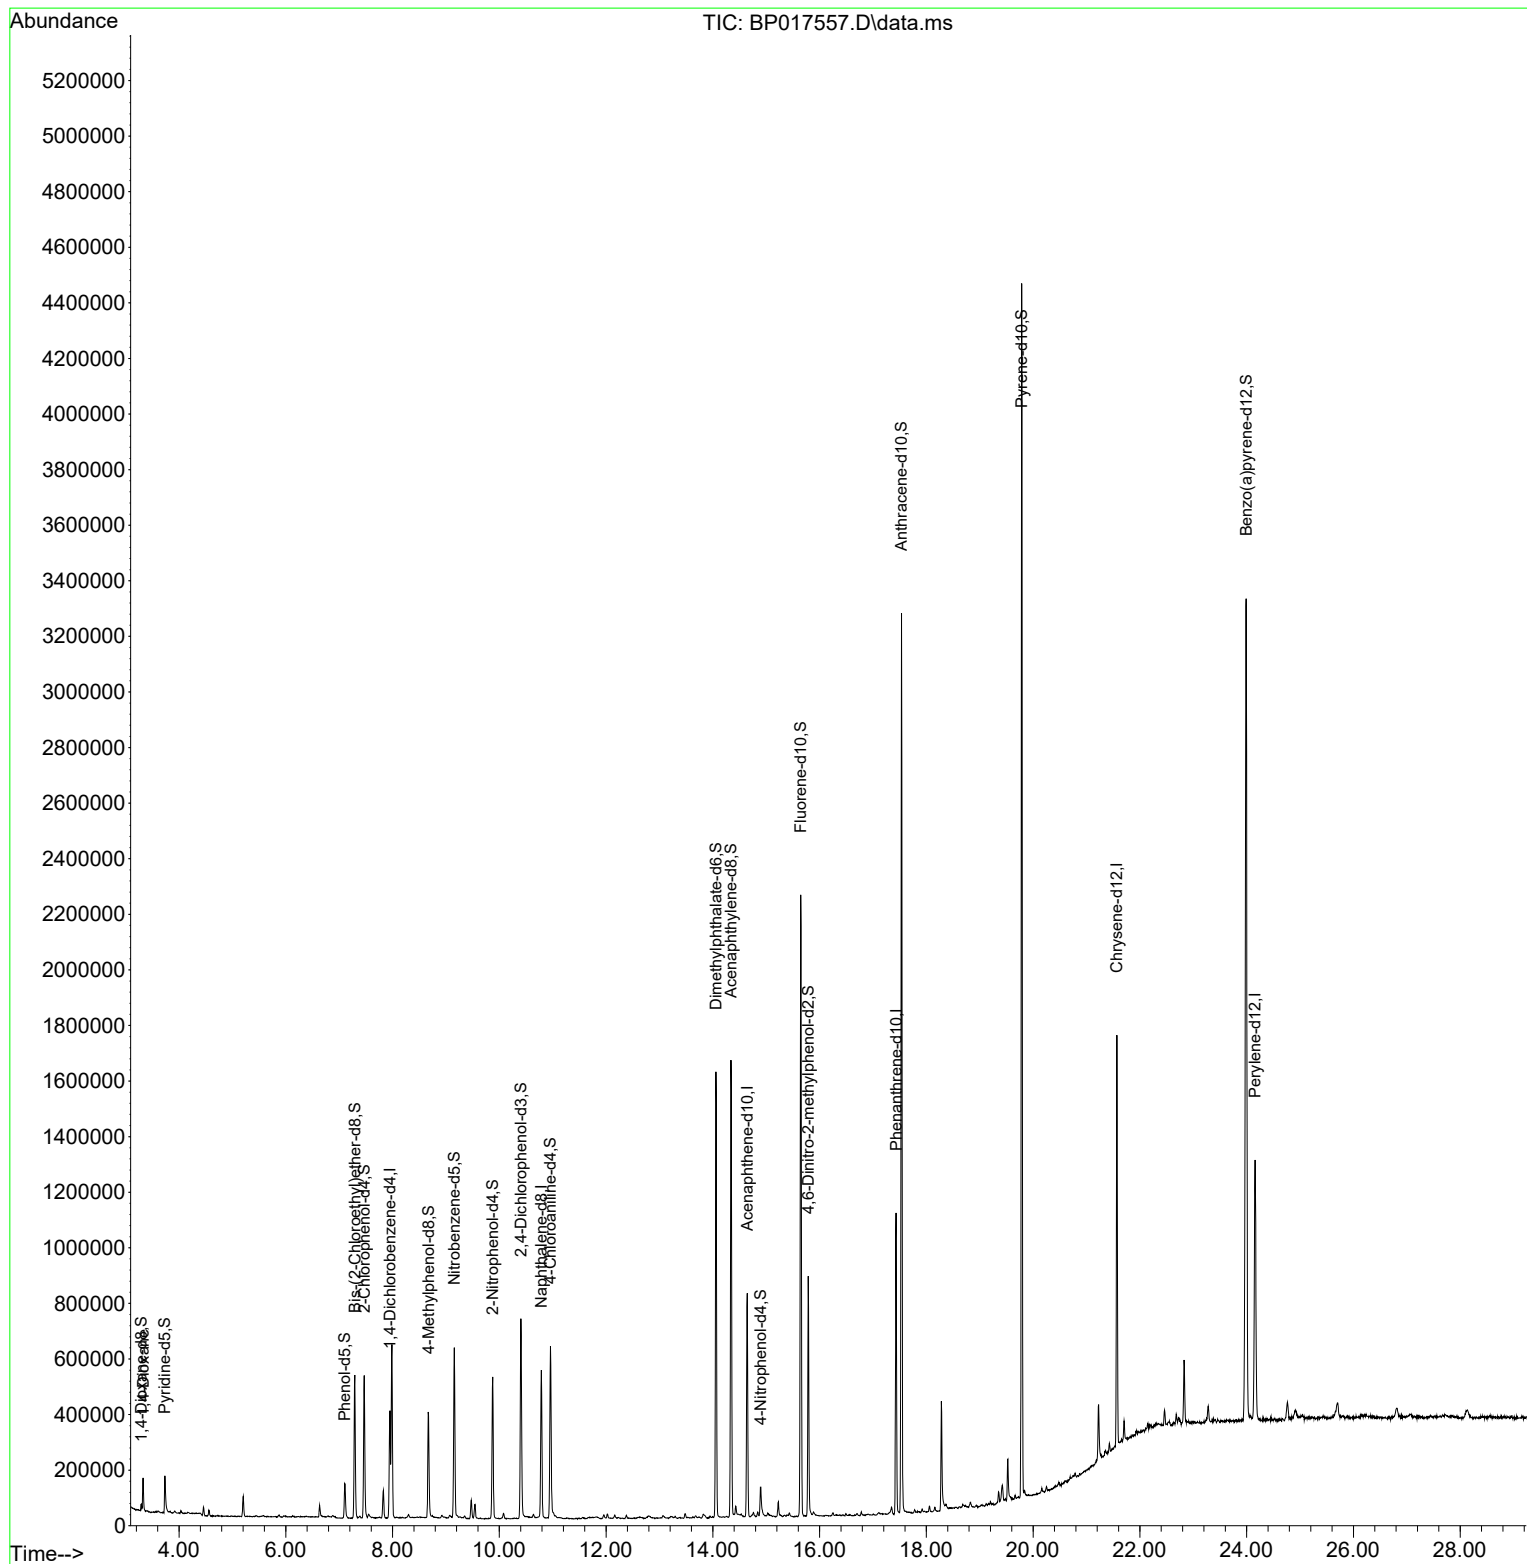

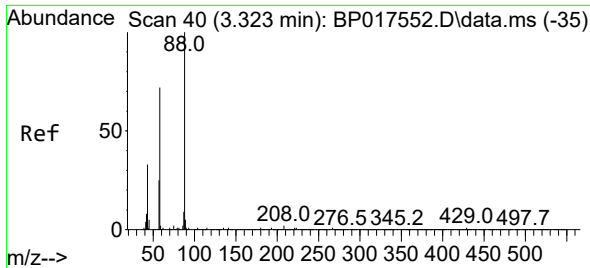

#2
 1,4-Dioxane
 Concen: 22.963 ng/uL
 RT: 3.329 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP017557.D
 Acq: 05 Oct 2023 10:11

Instrument :
 BNA_P
 ClientSampleId :
 PMW-8D(20230928)

Tgt Ion: 88 Resp: 57699
 Ion Ratio Lower Upper
 88 100
 43 30.0 22.6 34.0
 58 65.1 51.4 77.2

