




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017545.D
 Acq On : 04 Oct 2023 23:23
 Operator : MA/JU
 Sample : 04679-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DUP-1(20230928)

Manual IntegrationsAPPROVED

Quant Time: Oct 05 10:27:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 04 16:33:47 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/05/2023
 Supervised By :mohammad ahmed 10/07/2023

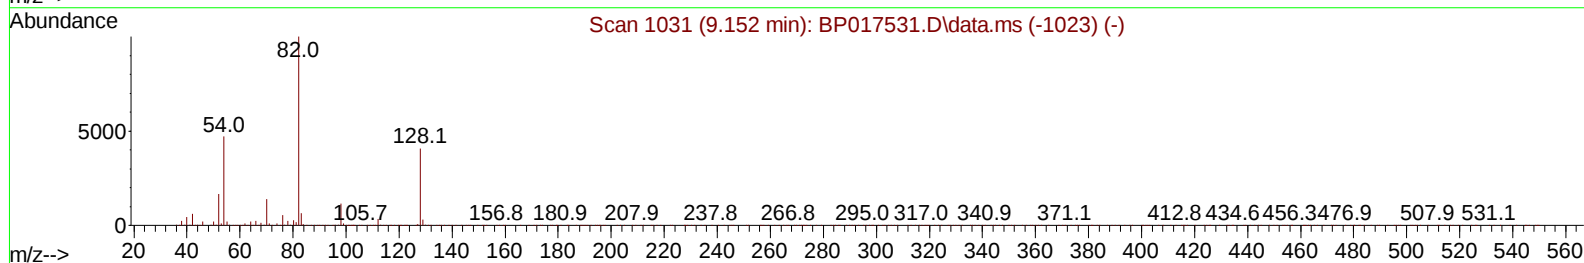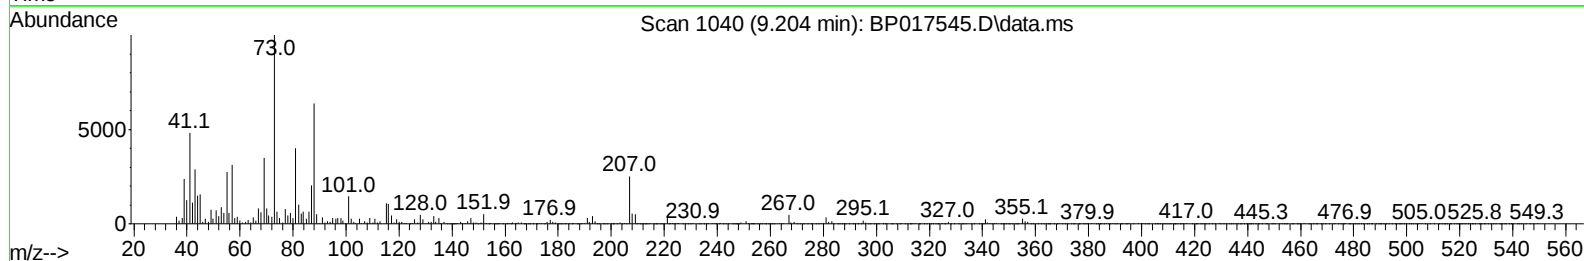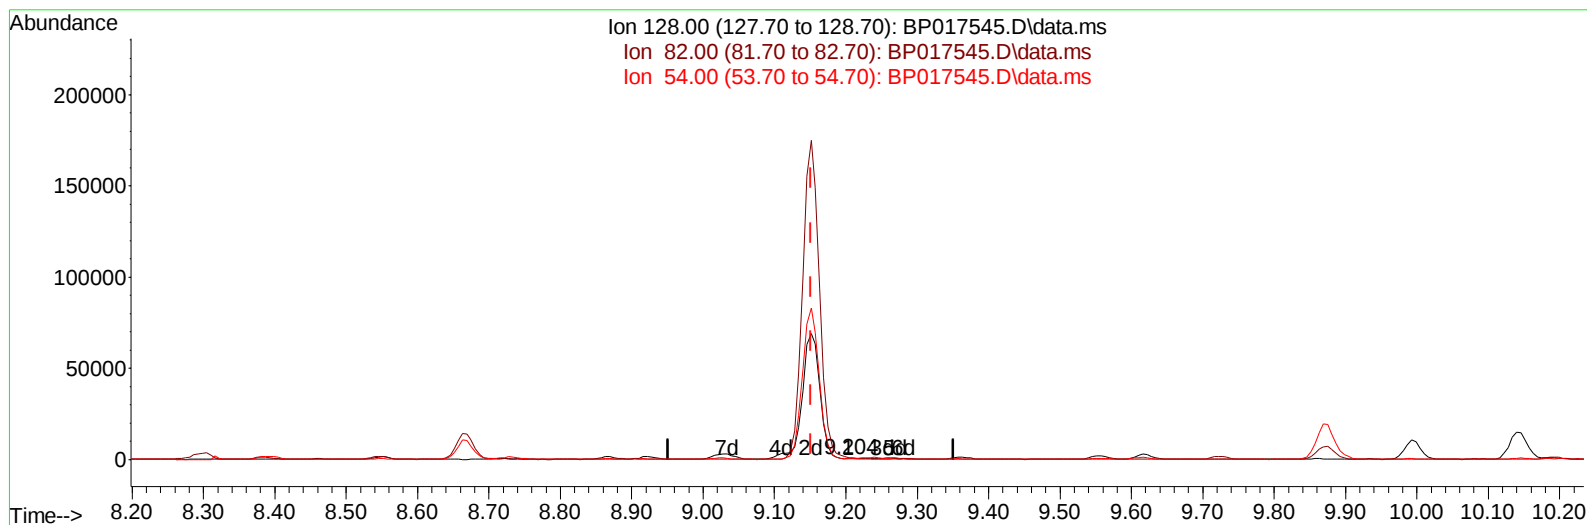

TIC: BP017545.D\data.ms

(21) Nitrobenzene-d5 (S)

9.204min (+ 0.053) 0.13 ng/u1

response 335

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	245.60	218.63
54.00	115.40	122.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017545.D
 Acq On : 04 Oct 2023 23:23
 Operator : MA/JU
 Sample : 04679-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DUP-1(20230928)

Manual IntegrationsAPPROVED

Quant Time: Oct 05 01:16:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 04 16:33:47 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/05/2023
 Supervised By :mohammad ahmed 10/07/2023

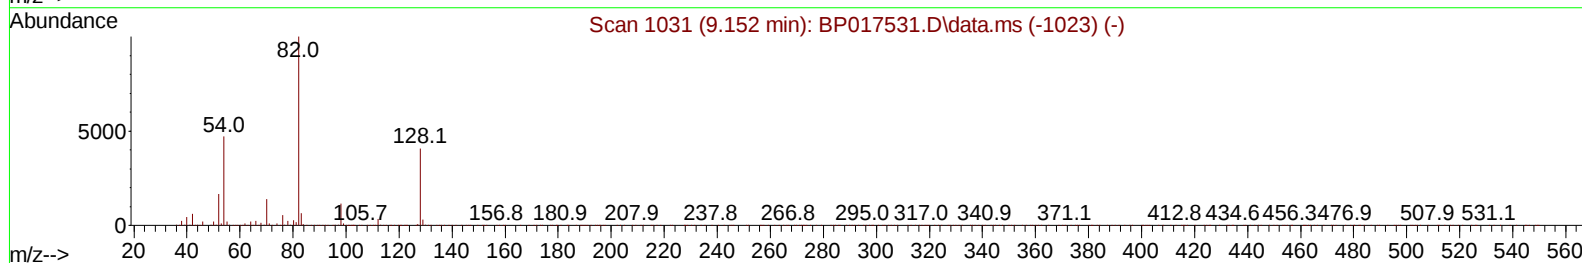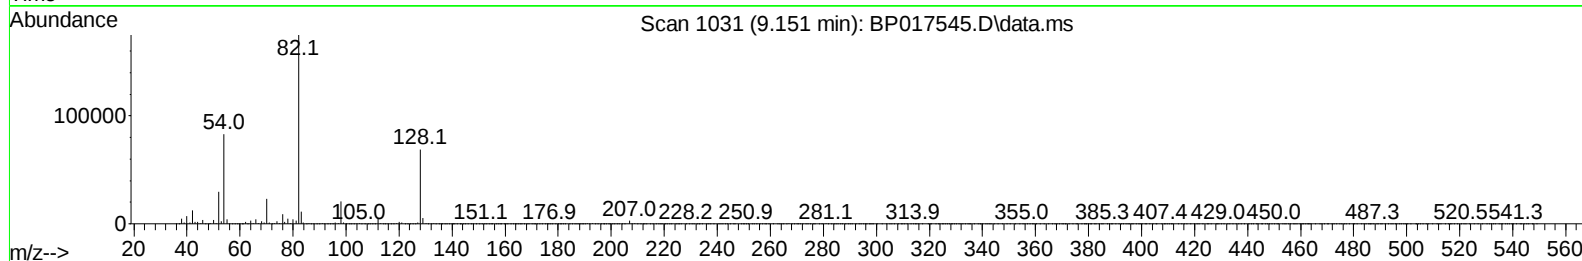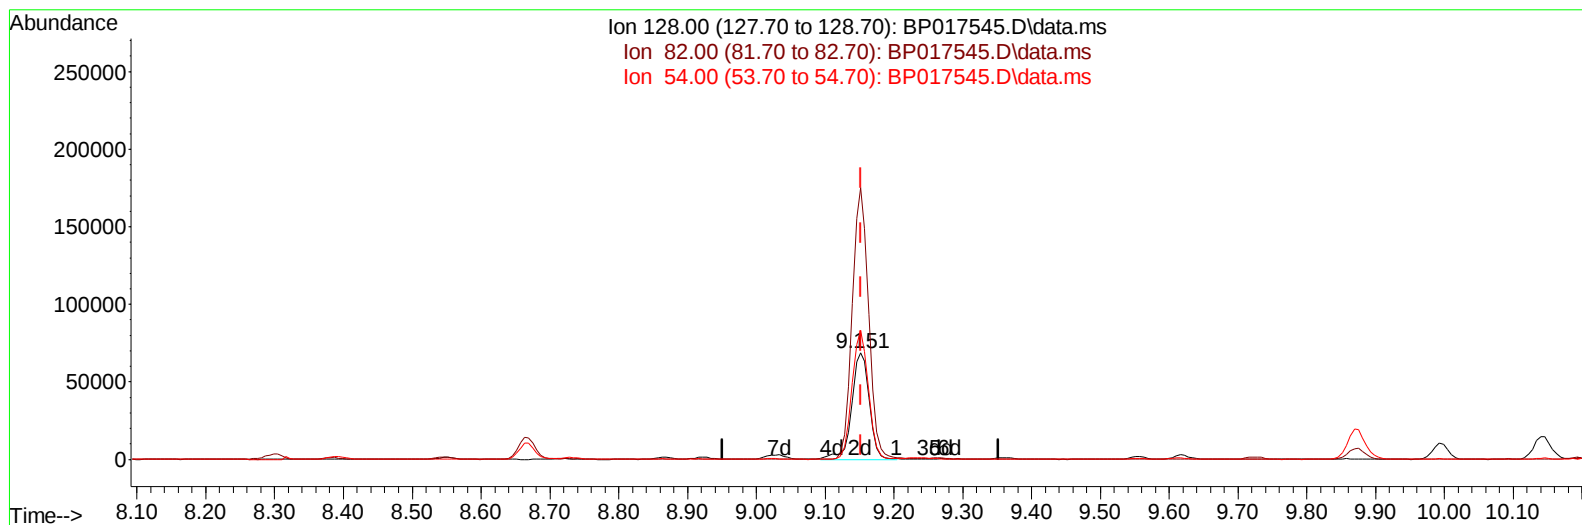

TIC: BP017545.D\data.ms

(21) Nitrobenzene-d5 (S)

9.151min (-0.000) 47.89 ng/u1 m

response 120848

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	245.60	254.15
54.00	115.40	120.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017545.D
 Acq On : 04 Oct 2023 23:23
 Operator : MA/JU
 Sample : 04679-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DUP-1(20230928)

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/05/2023
 Supervised By :mohammad ahmed 10/07/2023

Quant Time: Oct 05 01:16:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 04 16:33:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	88448	20.000	ng/ul	0.00
20) Naphthalene-d8	10.816	136	328040	20.000	ng/ul	0.04
38) Acenaphthene-d10	14.634	164	204513	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	445358	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	458469	20.000	ng/ul	0.00
88) Perylene-d12	24.133	264	530504	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	11956	5.404	ng/uL	0.00
4) Pyridine-d5	3.734	84	62686	10.825	ng/ul	0.00
7) Phenol-d5	7.105	99	62456	8.393	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	181380	39.943	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	190074	32.438	ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	113436	19.041	ng/ul	0.00
21) Nitrobenzene-d5	9.151	128	120848m	47.885	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	132502	46.550	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	223992	42.447	ng/ul	0.02
31) 4-Chloroaniline-d4	10.969	131	144747	19.255	ng/ul	0.02
46) Dimethylphthalate-d6	14.051	166	736850	46.190	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	808582	45.966	ng/ul	0.00
54) 4-Nitrophenol-d4	14.886	143	21557	7.717	ng/ul	0.01
60) Fluorene-d10	15.639	176	636225	47.020	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.781	200	92350	33.261	ng/ul	0.00
73) Anthracene-d10	17.522	188	991319	48.087	ng/ul	0.00
81) Pyrene-d10	19.774	212	1255923	49.299	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264	1311312	48.980	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017545.D
Acq On : 04 Oct 2023 23:23
Operator : MA/JU
Sample : 04679-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DUP-1(20230928)

Manual IntegrationsAPPROVED

Quant Time: Oct 05 01:16:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 04 16:33:47 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/05/2023
Supervised By :mohammad ahmed 10/07/2023

