




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017624.D
 Acq On : 07 Oct 2023 04:29
 Operator : MA/JU
 Sample : 04654-01
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJJ7

Manual IntegrationsAPPROVED

Quant Time: Oct 07 05:01:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 06 05:55:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2023
 Supervised By :mohammad ahmed 10/08/2023

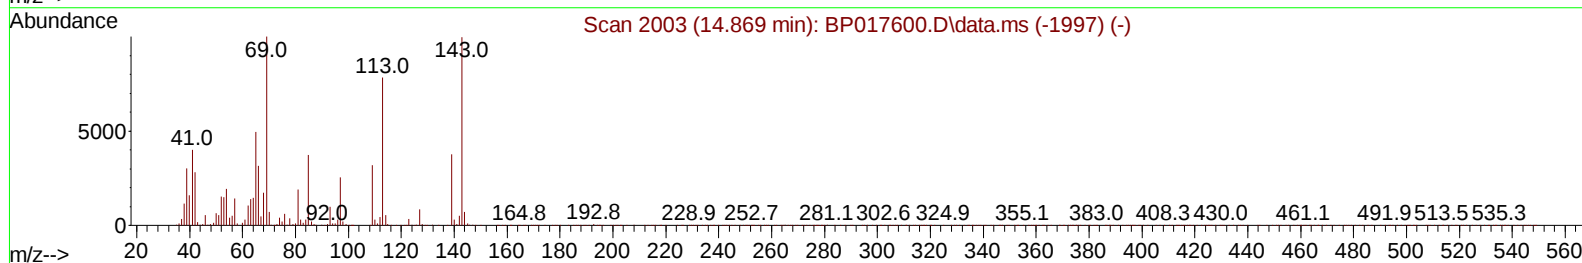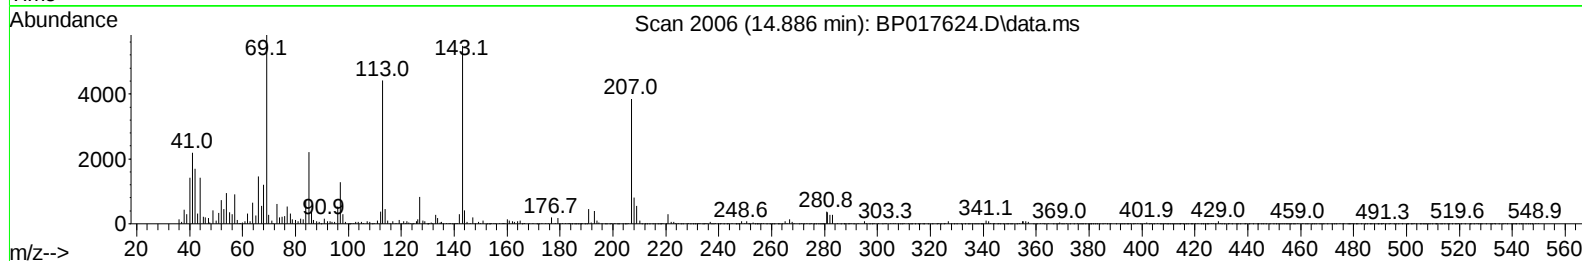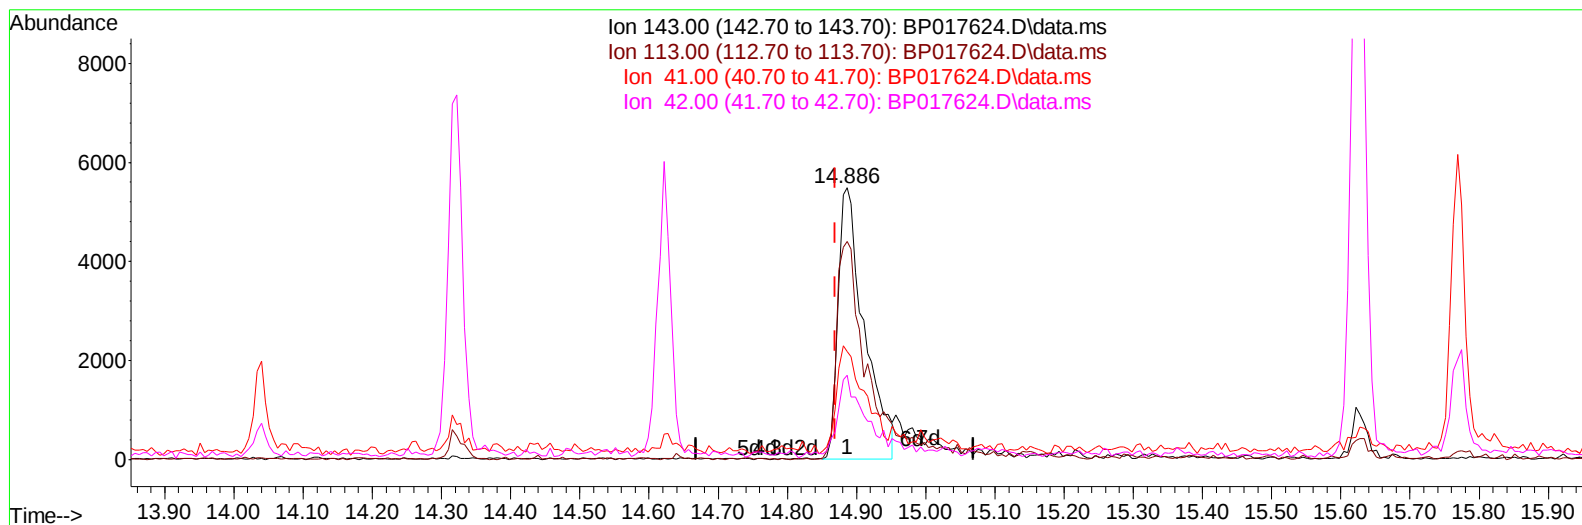

TIC: BP017624.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.886min (+ 0.018) 5.05 ng/u1

response 14305

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.00	80.40
41.00	43.80	39.85
42.00	29.00	30.90




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017624.D
 Acq On : 07 Oct 2023 04:29
 Operator : MA/JU
 Sample : 04654-01
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJJ7

Manual IntegrationsAPPROVED

Quant Time: Oct 07 05:01:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 06 05:55:05 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2023
 Supervised By :mohammad ahmed 10/08/2023

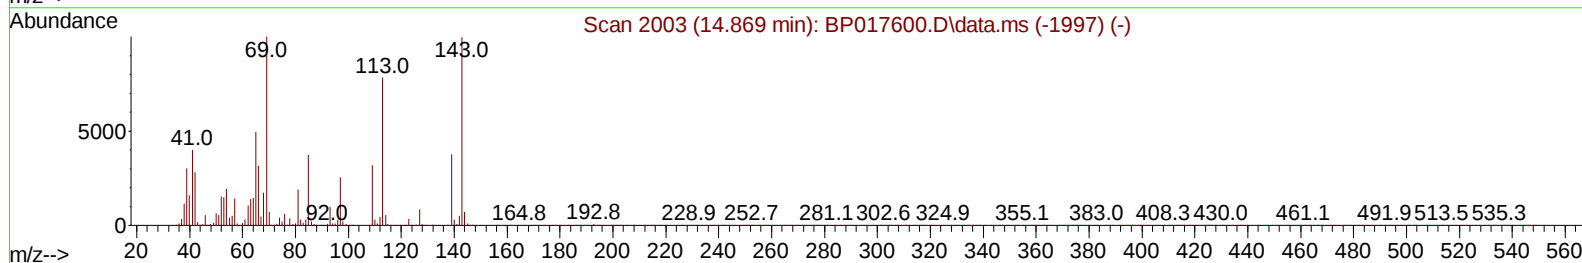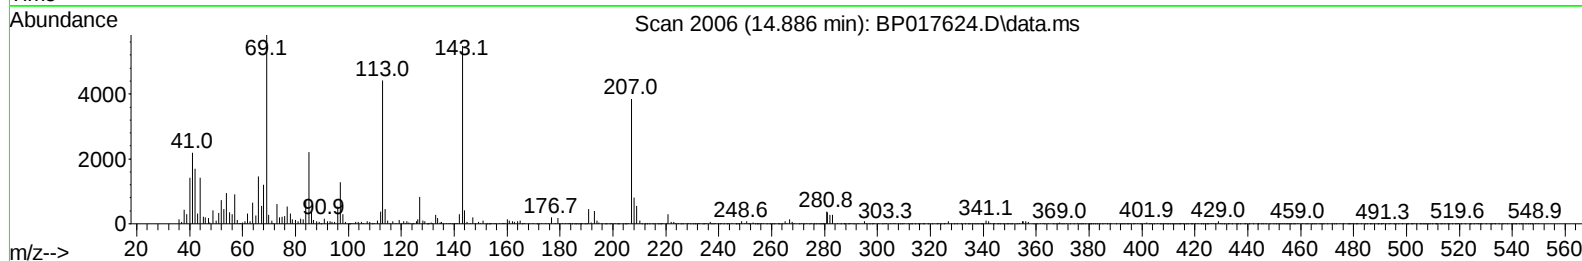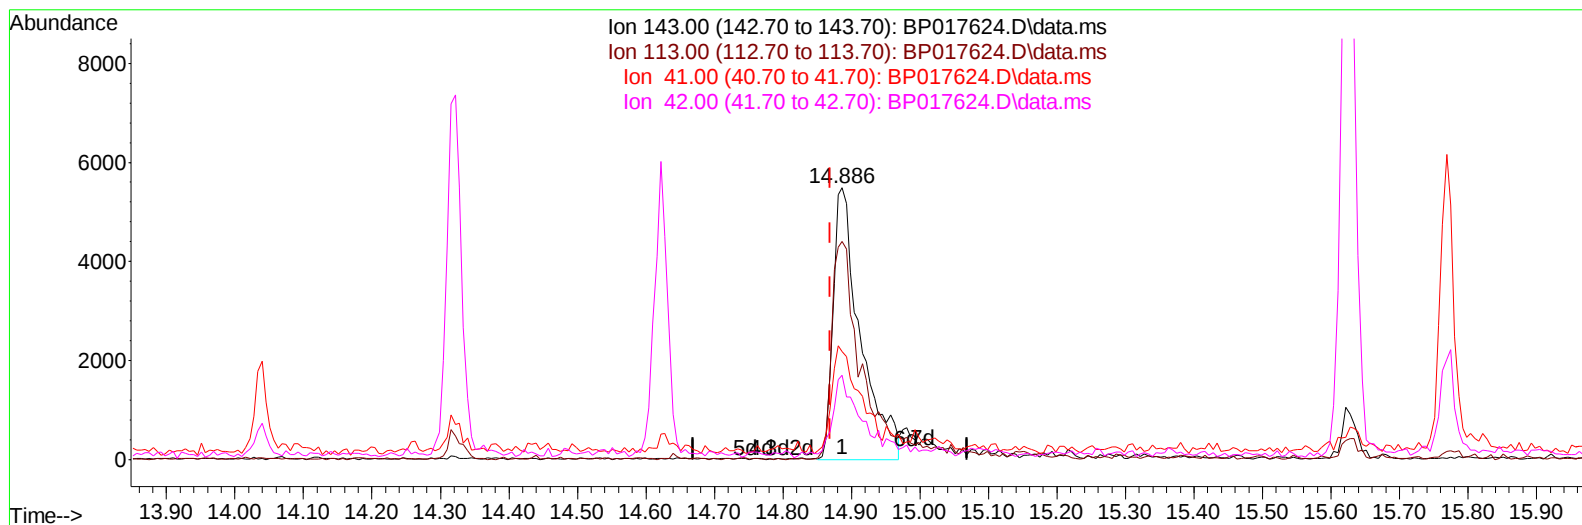

TIC: BP017624.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.886min (+ 0.018) 5.33 ng/ul m

response 15103

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.00	80.40
41.00	43.80	39.85
42.00	29.00	30.90

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017624.D
 Acq On : 07 Oct 2023 04:29
 Operator : MA/JU
 Sample : 04654-01
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJJ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/08/2023
 Supervised By :mohammad ahmed 10/08/2023

Quant Time: Oct 07 05:02:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 06 05:55:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	78912	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	324142	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	207329	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.410	188	481058	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	481514	20.000	ng/ul	0.00
88) Perylene-d12	24.121	264	546634	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	10293	5.215	ng/uL	0.00
4) Pyridine-d5	3.728	84	42833	8.291	ng/ul	0.00
7) Phenol-d5	7.087	99	54056	8.142	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	169103	41.740	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	168192	32.173	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	104868	19.730	ng/ul	0.00
21) Nitrobenzene-d5	9.140	128	104586	41.940	ng/ul	0.00
24) 2-Nitrophenol-d4	9.851	143	112124	39.865	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	193808	37.169	ng/ul	0.00
31) 4-Chloroaniline-d4	10.940	131	220395	29.671	ng/ul	0.00
46) Dimethylphthalate-d6	14.039	166	738539	45.667	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	765007	42.898	ng/ul	0.00
54) 4-Nitrophenol-d4	14.886	143	15103m	5.333	ng/ul	0.02
60) Fluorene-d10	15.628	176	654736	47.730	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.769	200	97430	32.487	ng/ul	0.00
73) Anthracene-d10	17.510	188	1149035	51.601	ng/ul	0.00
81) Pyrene-d10	19.769	212	1433507	53.577	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	1448144	52.494	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017624.D
Acq On : 07 Oct 2023 04:29
Operator : MA/JU
Sample : 04654-01
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJJ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/08/2023
Supervised By :mohammad ahmed 10/08/2023

Quant Time: Oct 07 05:02:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 06 05:55:05 2023
Response via : Initial Calibration

