

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017578.D
 Acq On : 05 Oct 2023 22:13
 Operator : MA/JU
 Sample : 04588-20
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK29

Quant Time: Oct 06 03:17:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 04 16:33:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	87642	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.775	136	368001	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	245725	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.416	188	572185	20.000	ng/ul	-0.01
79) Chrysene-d12	21.551	240	562398	20.000	ng/ul	-0.01
88) Perylene-d12	24.127	264	609781	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	9078	4.141	ng/uL	0.00
4) Pyridine-d5	3.728	84	74639	13.008	ng/ul	0.00
7) Phenol-d5	7.093	99	51935	7.043	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	197906	43.983	ng/ul	0.00
11) 2-Chlorophenol-d4	7.458	132	178738	30.784	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	111568	18.900	ng/ul	-0.01
21) Nitrobenzene-d5	9.146	128	123597	43.656	ng/ul	0.00
24) 2-Nitrophenol-d4	9.858	143	130335	40.817	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.393	165	228808	38.651	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131	228631	27.112	ng/ul	0.00
46) Dimethylphthalate-d6	14.046	166	853922	44.551	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	931969	44.095	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	19687	5.865	ng/ul	0.01
60) Fluorene-d10	15.634	176	757000	46.562	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.775	200	126247	35.391	ng/ul	0.00
73) Anthracene-d10	17.522	188	1236496	46.685	ng/ul	0.00
81) Pyrene-d10	19.775	212	1496413	47.884	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.963	264	1477119	48.000	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.329	88	3921	1.740	ng/uL#	83
8) Phenol	7.128	94	20345	2.755	ng/ul#	85
30) Naphthalene	10.822	128	155254	7.907	ng/ul	99
36) 2-Methylnaphthalene	12.440	142	121251	9.037	ng/ul	98
37) 1-Methylnaphthalene	12.657	142	123163	8.947	ng/ul#	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017578.D
Acq On : 05 Oct 2023 22:13
Operator : MA/JU
Sample : 04588-20
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK29

Quant Time: Oct 06 03:17:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 04 16:33:47 2023
Response via : Initial Calibration




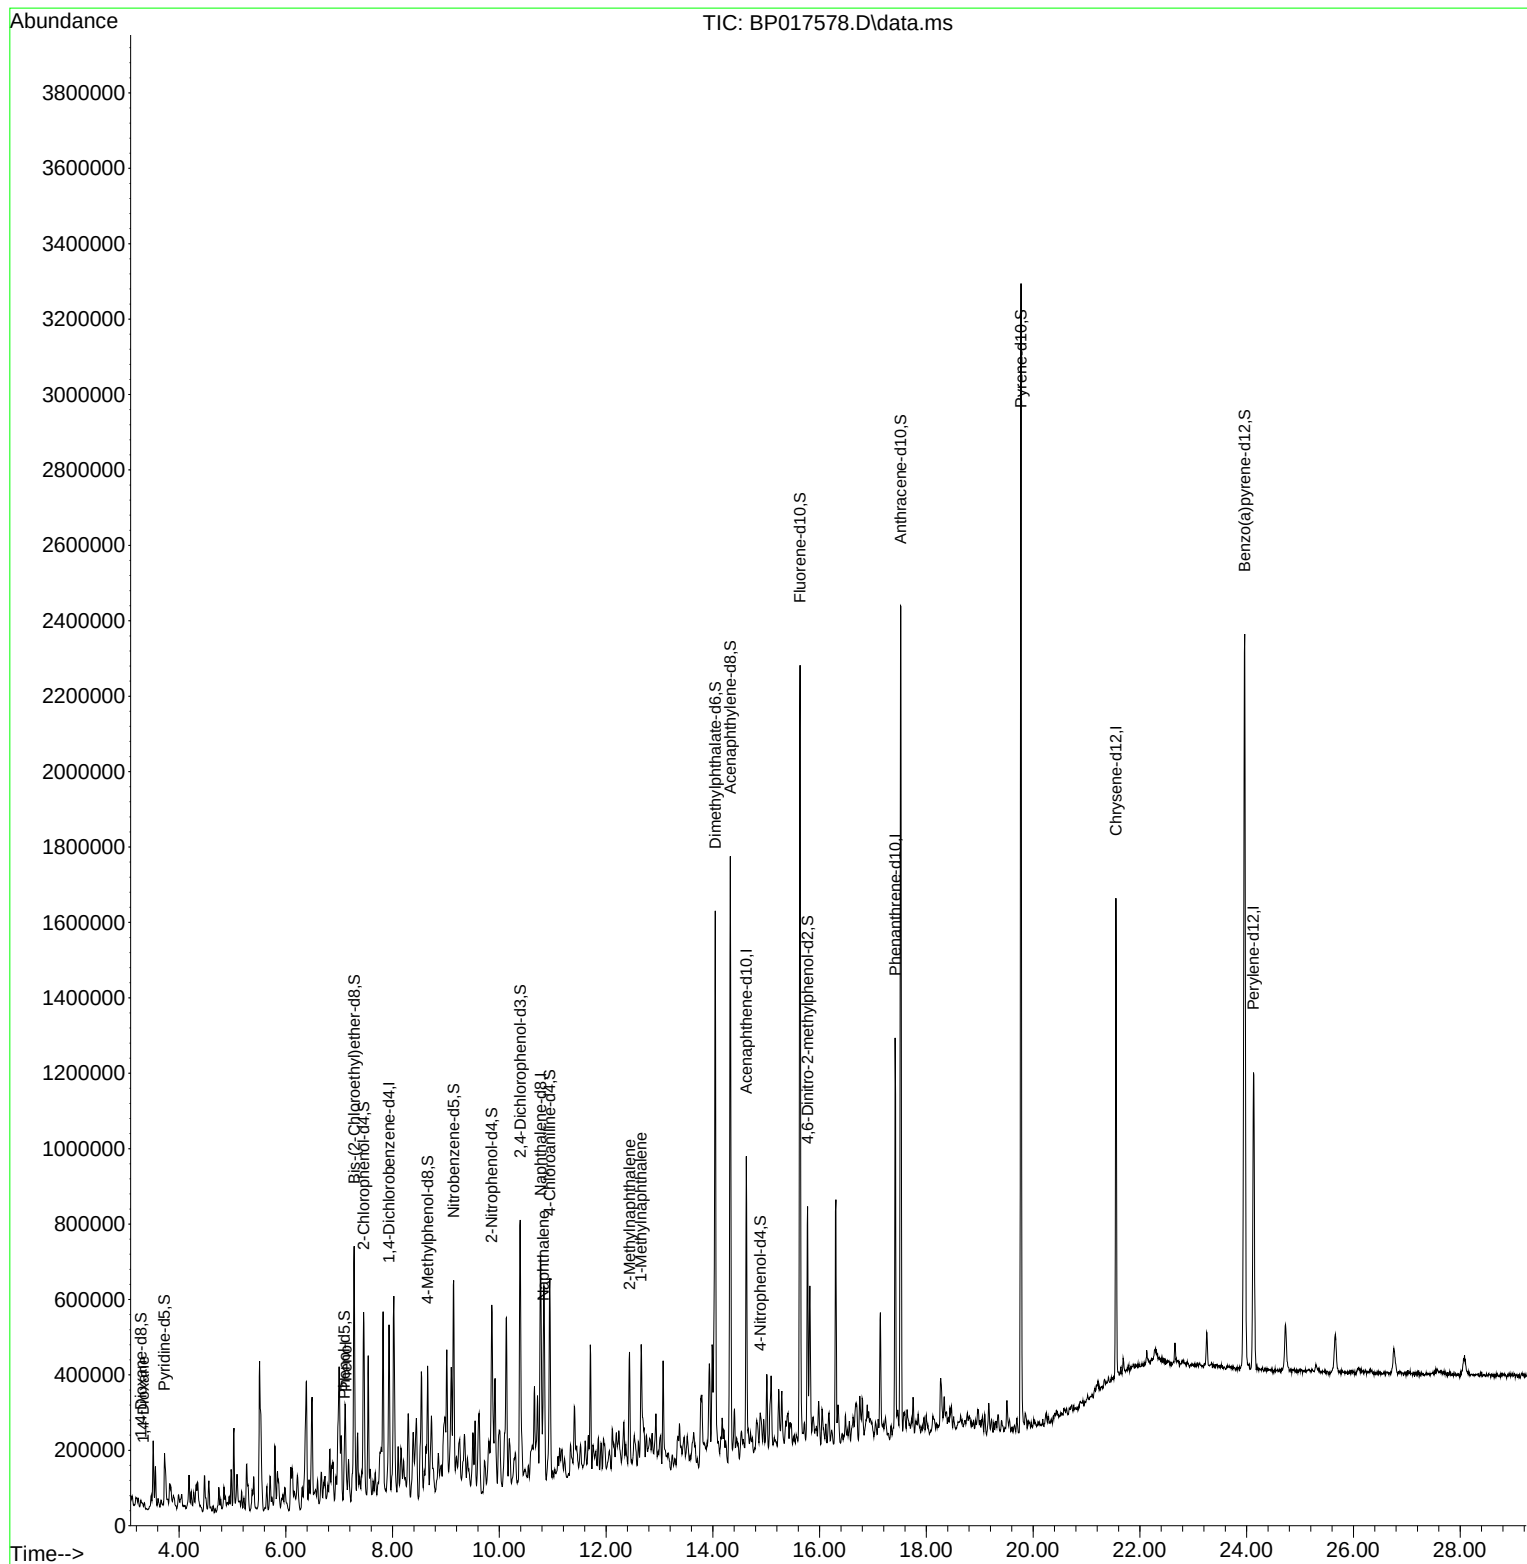


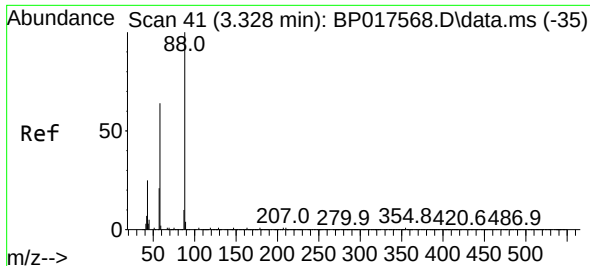

#2
 1,4-Dioxane
 Concen: 1.740 ng/uL
 RT: 3.329 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP017578.D
 Acq: 05 Oct 2023 22:13




Instrument :
 BNA_P
 ClientSampleId :
 BBK29


Tgt Ion: 88 Resp: 3921
 Ion Ratio Lower Upper
 88 100
 43 44.0 22.6 34.0#
 58 55.5 51.4 77.2

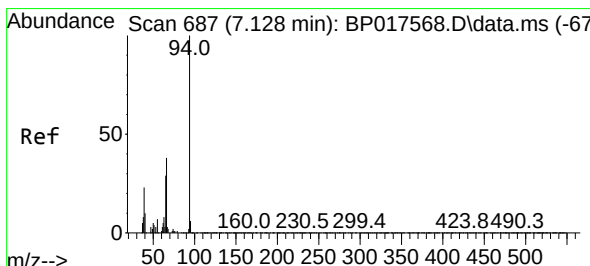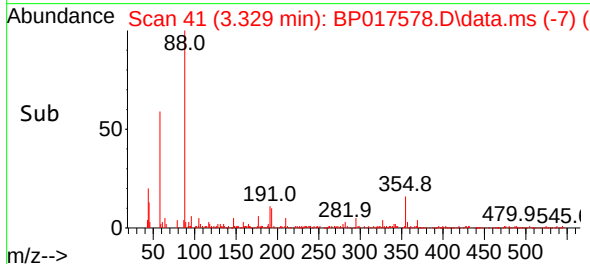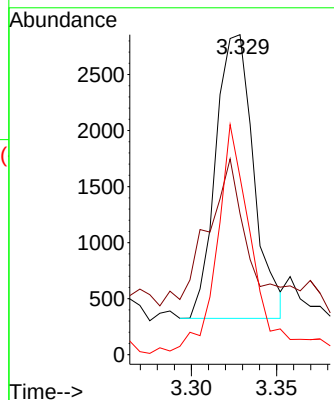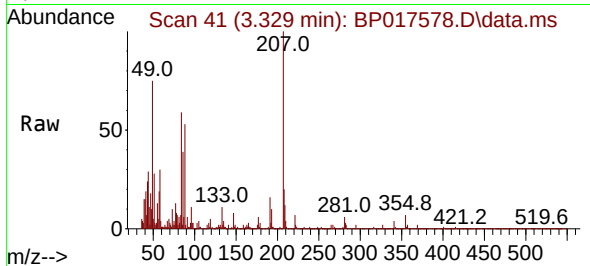

#8
 Phenol
 Concen: 2.755 ng/uL
 RT: 7.128 min Scan# 687
 Delta R.T. 0.000 min
 Lab File: BP017578.D
 Acq: 05 Oct 2023 22:13

Tgt Ion: 94 Resp: 20345
 Ion Ratio Lower Upper
 94 100
 65 46.4 23.5 35.3#
 66 41.8 32.3 48.5


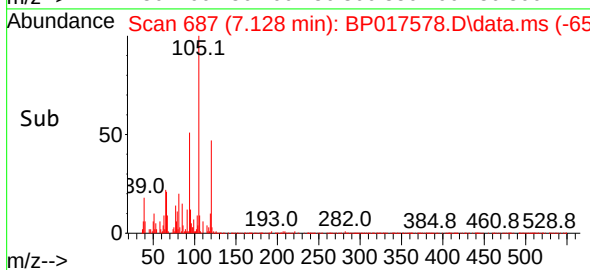
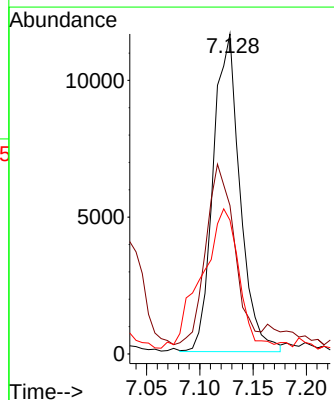
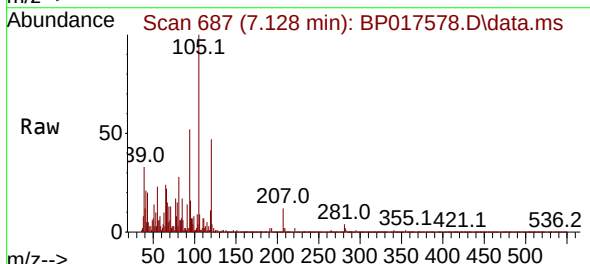


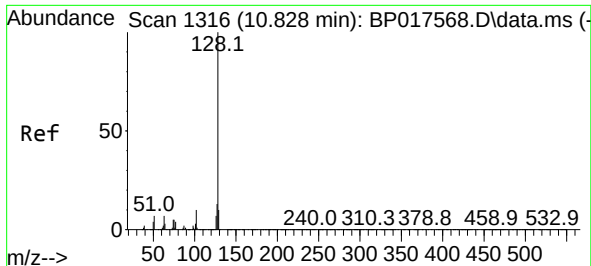

#30
Naphthalene
Concen: 7.907 ng/ul
RT: 10.822 min Scan# 1315
Delta R.T. -0.012 min
Lab File: BP017578.D
Acq: 05 Oct 2023 22:13




Instrument :
BNA_P
ClientSampleId :
BBK29


Tgt Ion:128 Resp: 155254
Ion Ratio Lower Upper
128 100
129 11.4 8.6 13.0
127 13.0 10.2 15.4

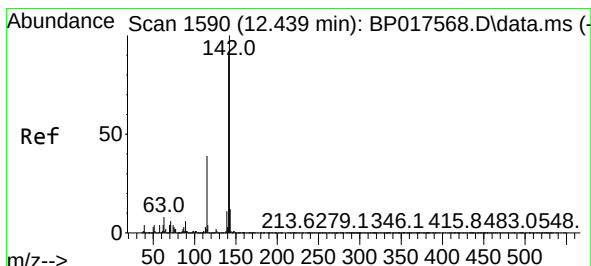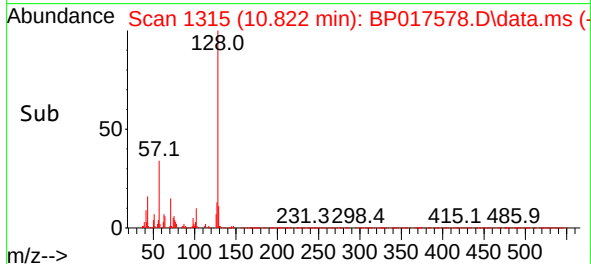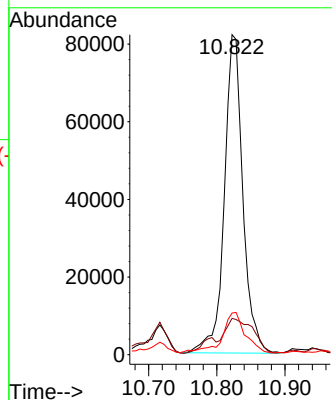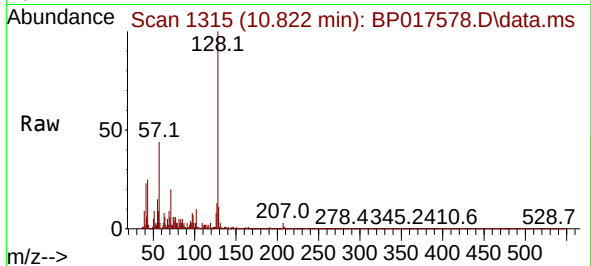

#36
2-Methylnaphthalene
Concen: 9.037 ng/ul
RT: 12.440 min Scan# 1590
Delta R.T. -0.006 min
Lab File: BP017578.D
Acq: 05 Oct 2023 22:13

Tgt Ion:142 Resp: 121251
Ion Ratio Lower Upper
142 100
141 91.4 71.4 107.2

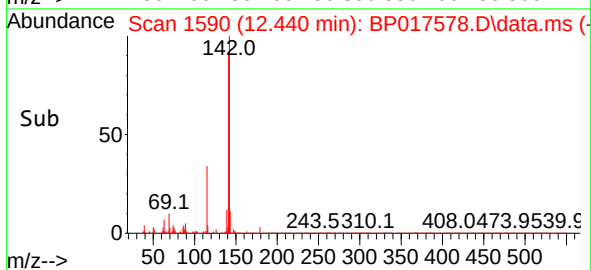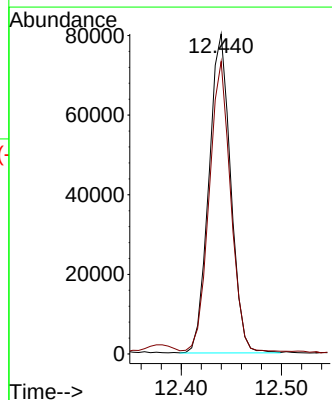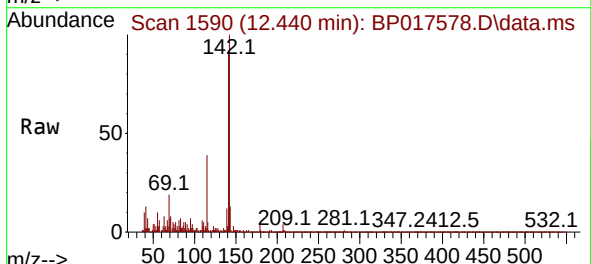

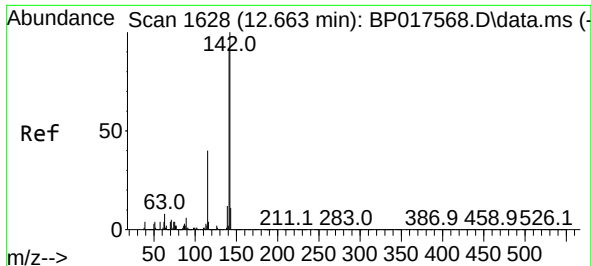

#37

1-Methylnaphthalene

Concen: 8.947 ng/ul

RT: 12.657 min Scan# 1

Delta R.T. -0.012 min

Lab File: BP017578.D


Acq: 05 Oct 2023 22:13

Instrument :

BNA_P

ClientSampleId :

BBK29

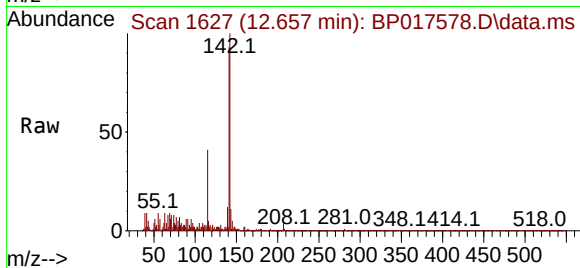

Tgt Ion:142 Resp: 123163

Ion Ratio Lower Upper

142 100

141 92.7 74.1 111.1

116 5.5 3.4 5.0#

