

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017604.D
 Acq On : 06 Oct 2023 16:29
 Operator : MA/JU
 Sample : 04624-08
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJJ5

Quant Time: Oct 06 23:34:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 06 05:55:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	70775	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	295843	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.622	164	203593	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	481667	20.000	ng/u1	0.00
79) Chrysene-d12	21.551	240	524906	20.000	ng/u1	0.00
88) Perylene-d12	24.127	264	580564	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	10040	5.671	ng/uL	0.00
4) Pyridine-d5	3.728	84	77593	16.745	ng/u1	0.00
7) Phenol-d5	7.093	99	52585	8.831	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	155417	42.772	ng/u1	0.00
11) 2-Chlorophenol-d4	7.452	132	158151	33.730	ng/u1	0.00
15) 4-Methylphenol-d8	8.658	113	101432	21.277	ng/u1	0.00
21) Nitrobenzene-d5	9.140	128	95657	42.029	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	103710	40.401	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	185964	39.076	ng/u1	0.00
31) 4-Chloroaniline-d4	10.940	131	232067	34.231	ng/u1	0.00
46) Dimethylphthalate-d6	14.040	166	719792	45.325	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	724525	41.374	ng/u1	0.00
54) 4-Nitrophenol-d4	14.881	143	24646	8.862	ng/u1	0.01
60) Fluorene-d10	15.628	176	632680	46.969	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.775	200	113133	37.675	ng/u1	0.00
73) Anthracene-d10	17.516	188	1148958	51.532	ng/u1	0.00
81) Pyrene-d10	19.769	212	1497850	51.354	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	1578201	53.865	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.822	128	255472	16.185	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017604.D
Acq On : 06 Oct 2023 16:29
Operator : MA/JU
Sample : 04624-08
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJJ5


Quant Time: Oct 06 23:34:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 06 05:55:05 2023
Response via : Initial Calibration

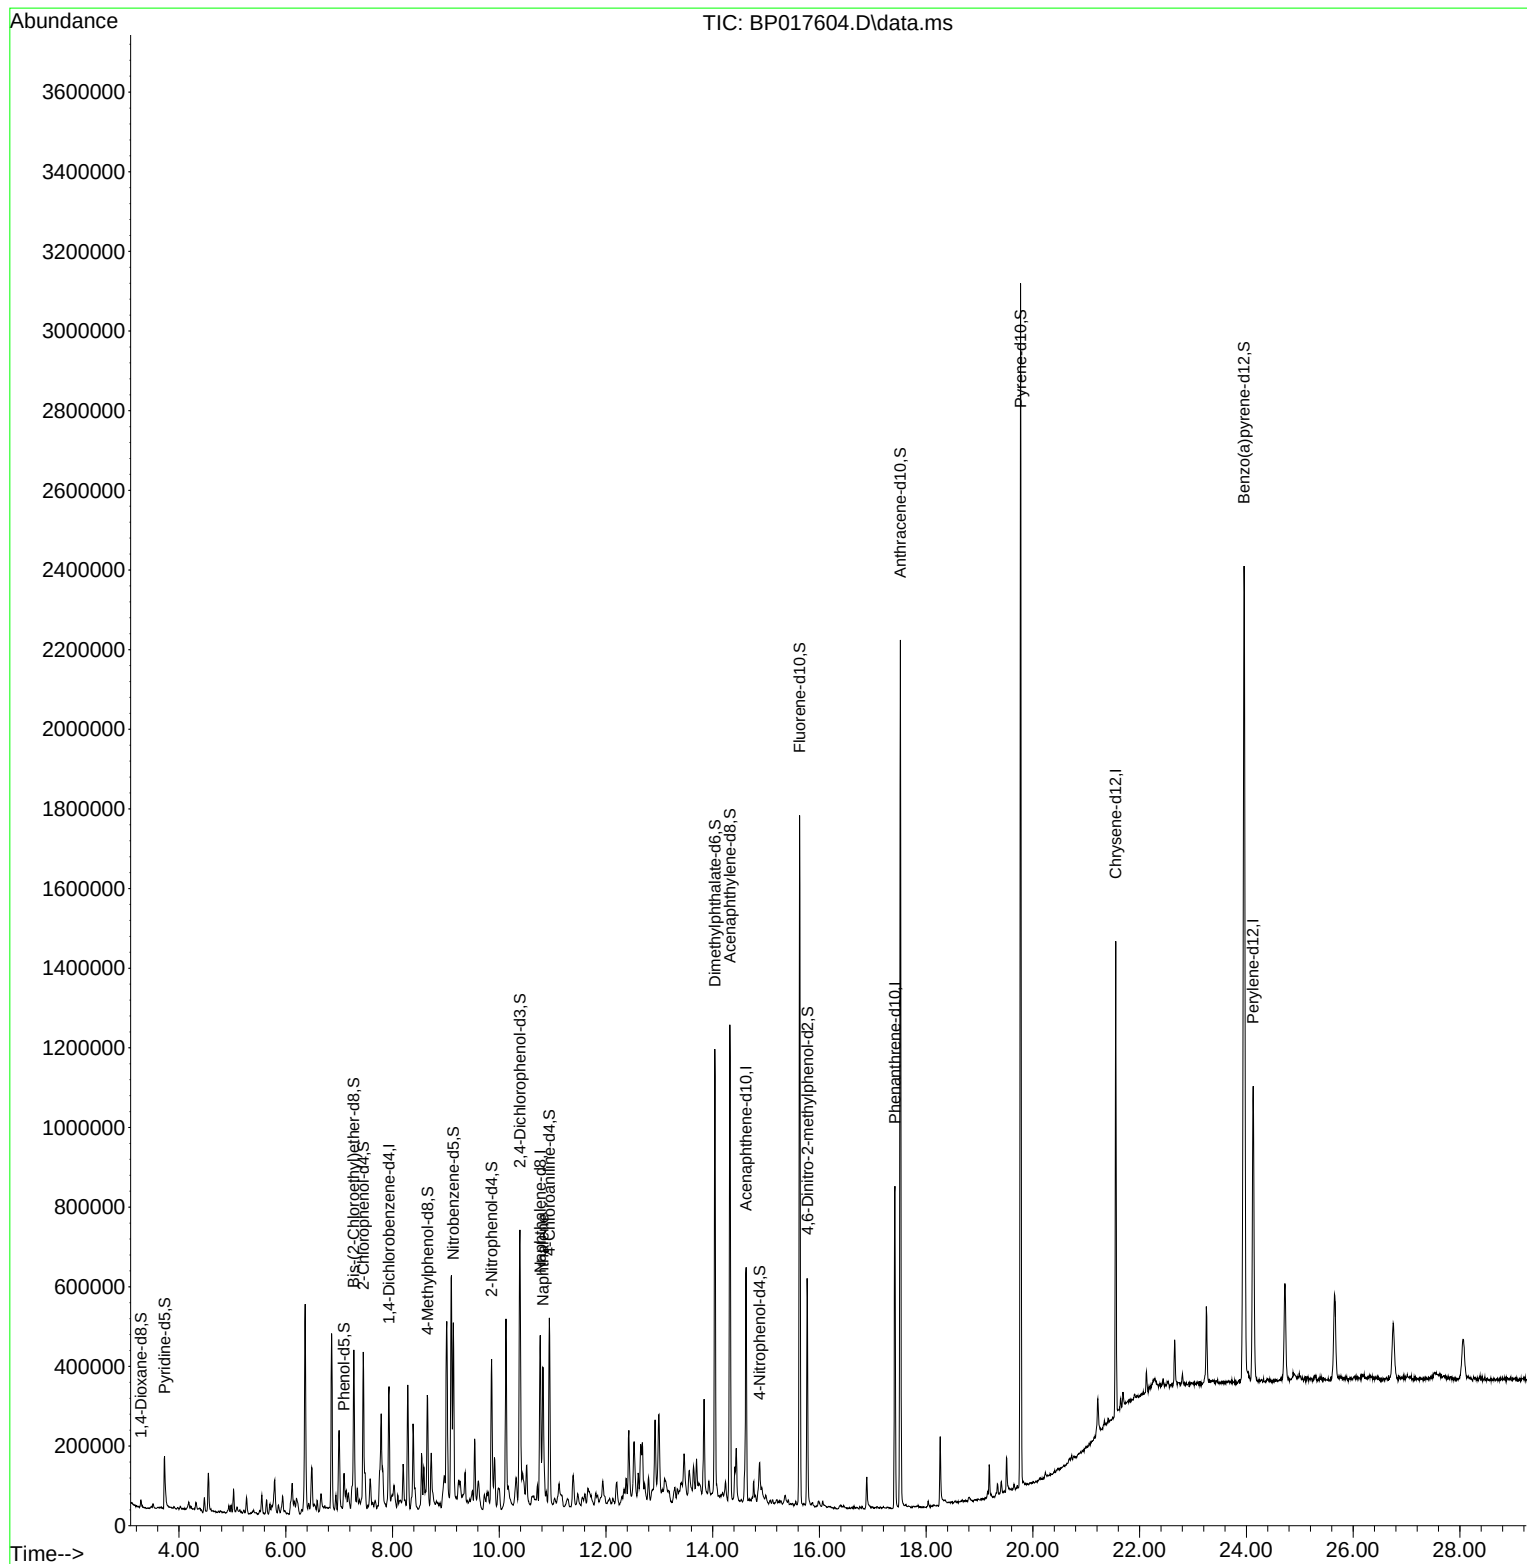

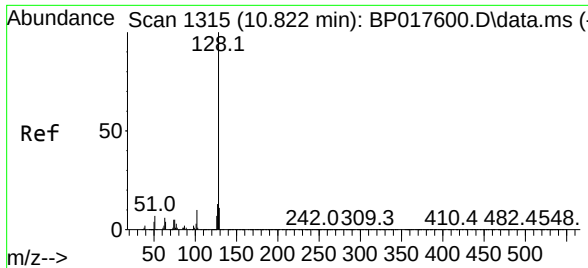

#30
Naphthalene
Concen: 16.185 ng/ul
RT: 10.822 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP017604.D
Acq: 06 Oct 2023 16:29

Instrument :
BNA_P
ClientSampleId :
BBJJ5

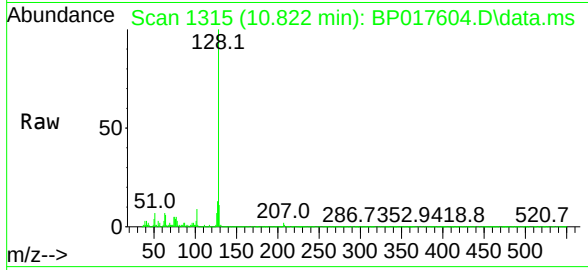

Tgt Ion:128 Resp: 255472
Ion Ratio Lower Upper
128 100
129 10.9 8.6 13.0
127 13.0 10.2 15.4

