

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017610.D
 Acq On : 06 Oct 2023 19:55
 Operator : MA/JU
 Sample : 04624-13
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHB5

Quant Time: Oct 06 23:59:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 06 05:55:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	84495	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	351268	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	222055	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	523751	20.000	ng/u1	0.00
79) Chrysene-d12	21.551	240	529517	20.000	ng/u1	0.00
88) Perylene-d12	24.127	264	587952	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	12185	5.765	ng/uL	0.00
4) Pyridine-d5	3.722	84	100982	18.254	ng/u1	0.00
7) Phenol-d5	7.087	99	87264	12.275	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	201406	46.428	ng/u1	0.00
11) 2-Chlorophenol-d4	7.452	132	212456	37.954	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	150856	26.507	ng/u1	0.00
21) Nitrobenzene-d5	9.140	128	125309	46.370	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	134546	44.143	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	244992	43.357	ng/u1	0.00
31) 4-Chloroaniline-d4	10.940	131	298533	37.087	ng/u1	0.00
46) Dimethylphthalate-d6	14.039	166	878612	50.725	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	912596	47.781	ng/u1	0.00
54) 4-Nitrophenol-d4	14.881	143	27111	8.938	ng/u1	0.01
60) Fluorene-d10	15.628	176	764855	52.060	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.769	200	122378	37.479	ng/u1	0.00
73) Anthracene-d10	17.516	188	1280718	52.826	ng/u1	0.00
81) Pyrene-d10	19.769	212	1617246	54.964	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	1632220	55.009	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.322	88	2248	1.035 ng/uL#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017610.D
Acq On : 06 Oct 2023 19:55
Operator : MA/JU
Sample : 04624-13
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHB5


Quant Time: Oct 06 23:59:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 06 05:55:05 2023
Response via : Initial Calibration

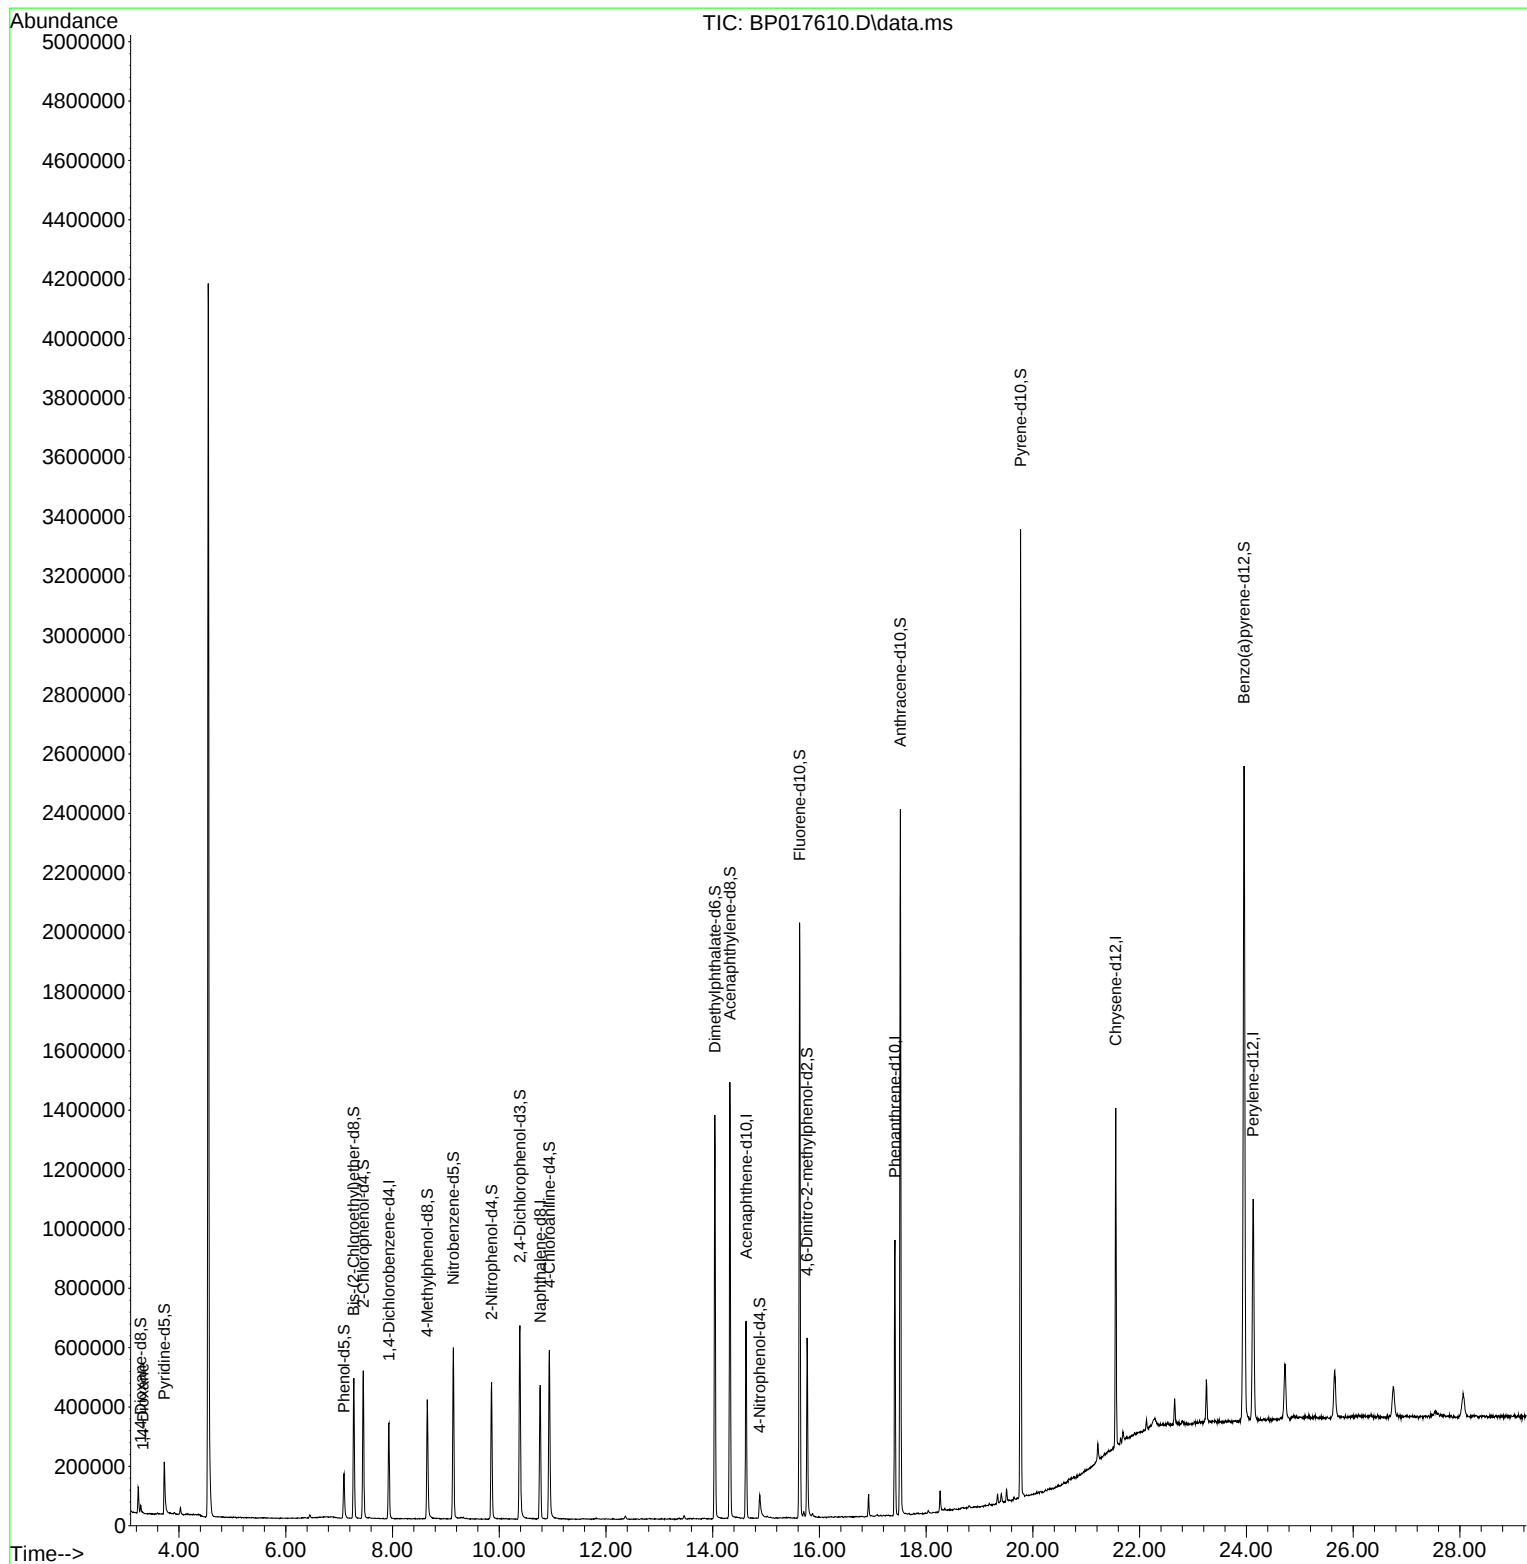

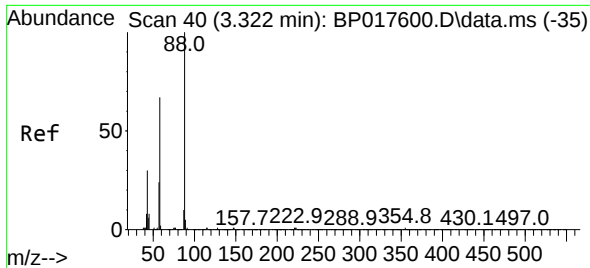

#2
 1,4-Dioxane
 Concen: 1.035 ng/uL
 RT: 3.322 min Scan# 40
 Delta R.T. -0.000 min
 Lab File: BP017610.D
 Acq: 06 Oct 2023 19:55

Instrument :
 BNA_P
 ClientSampleId :
 BBHB5

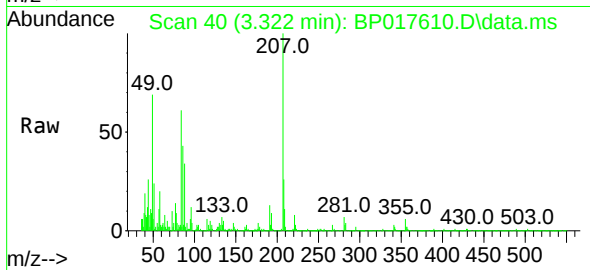

Tgt Ion: 88 Resp: 2248

Ion	Ratio	Lower	Upper
88	100		
43	35.6	22.6	34.0#
58	58.0	51.4	77.2

