

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017611.D
 Acq On : 06 Oct 2023 20:29
 Operator : MA/JU
 Sample : 04624-14
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBBS0

Quant Time: Oct 06 23:15:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 06 05:55:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	88297	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	361218	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.628	164	225779	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	527997	20.000	ng/u1	0.00
79) Chrysene-d12	21.551	240	547937	20.000	ng/u1	0.00
88) Perylene-d12	24.127	264	609788	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	12471	5.647	ng/uL	0.00
4) Pyridine-d5	3.728	84	78891	13.647	ng/u1	0.00
7) Phenol-d5	7.093	99	71815	9.667	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	208323	45.955	ng/u1	0.00
11) 2-Chlorophenol-d4	7.452	132	211139	36.095	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	130771	21.988	ng/u1	0.00
21) Nitrobenzene-d5	9.140	128	128807	46.351	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	141063	45.006	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	241992	41.646	ng/u1	0.00
31) 4-Chloroaniline-d4	10.940	131	320089	38.670	ng/u1	0.00
46) Dimethylphthalate-d6	14.039	166	852776	48.422	ng/u1	0.00
49) Acenaphthylene-d8	14.322	160	918251	47.284	ng/u1	0.00
54) 4-Nitrophenol-d4	14.881	143	19964	6.473	ng/u1	0.01
60) Fluorene-d10	15.628	176	744495	49.839	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.769	200	119828	36.403	ng/u1	0.00
73) Anthracene-d10	17.516	188	1245916	50.978	ng/u1	0.00
81) Pyrene-d10	19.769	212	1577275	51.804	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	1614894	52.476	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.322	88	2934	1.292	ng/uL#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017611.D
Acq On : 06 Oct 2023 20:29
Operator : MA/JU
Sample : 04624-14
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBS0


Quant Time: Oct 06 23:15:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 06 05:55:05 2023
Response via : Initial Calibration

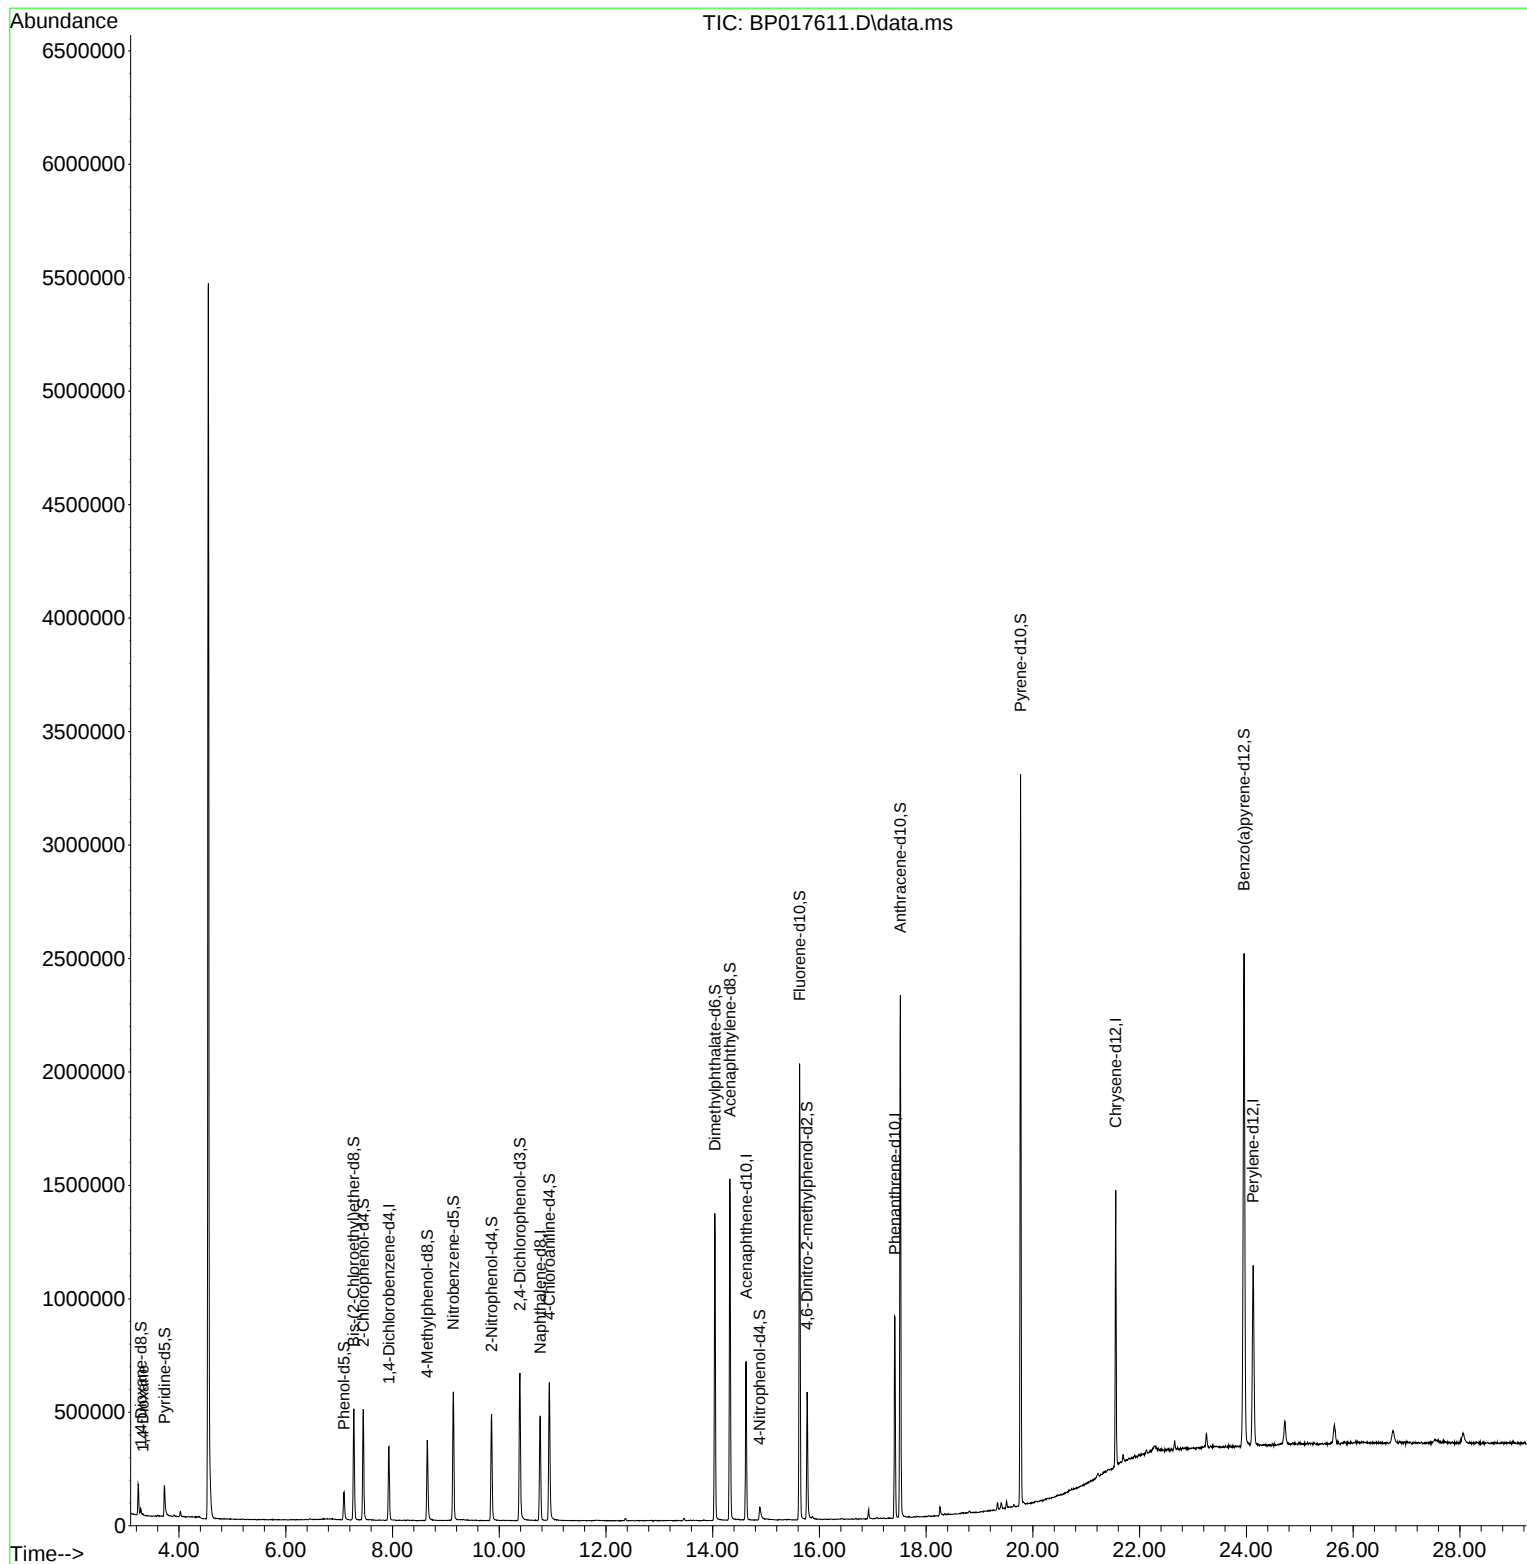

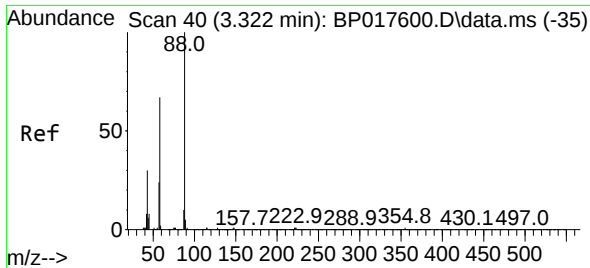

#2
 1,4-Dioxane
 Concen: 1.292 ng/uL
 RT: 3.322 min Scan# 40
 Delta R.T. -0.000 min
 Lab File: BP017611.D
 Acq: 06 Oct 2023 20:29

Instrument :
 BNA_P
 ClientSampleId :
 BBBS0

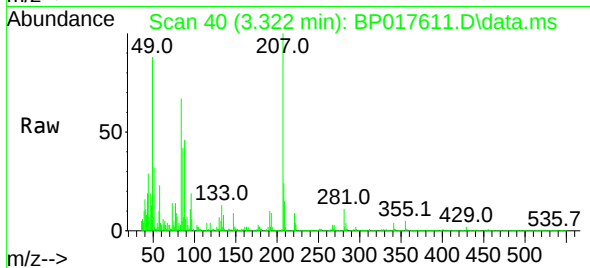

Tgt Ion: 88 Resp: 2934

Ion	Ratio	Lower	Upper
88	100		
43	41.1	22.6	34.0#
58	50.1	51.4	77.2#

