

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017540.D
 Acq On : 04 Oct 2023 19:24
 Operator : MA/JU
 Sample : PB156008BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK008

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	40	rVB	31240	38513	1.20%	0.139%
2	3.728	105	109	126	rBV	395336	595302	18.53%	2.154%
3	4.034	158	161	167	rVB5	6329	11294	0.35%	0.041%
4	4.264	198	200	204	rVB4	6242	6366	0.20%	0.023%
5	4.681	268	271	277	rVB6	4423	7665	0.24%	0.028%
6	4.775	285	287	290	rBV3	3479	4760	0.15%	0.017%
7	7.099	675	682	693	rBV	475718	755340	23.52%	2.733%
8	7.287	707	714	724	rBV	388059	604758	18.83%	2.188%
9	7.463	737	744	755	rBV	488477	780469	24.30%	2.824%
10	7.946	818	826	833	rBV	295673	475040	14.79%	1.719%
11	8.663	942	948	962	rBV	570472	917303	28.56%	3.319%
12	9.152	1023	1031	1041	rBV	441006	731396	22.77%	2.646%
13	9.487	1085	1088	1091	rVB5	2670	3612	0.11%	0.013%
14	9.869	1145	1153	1162	rBV	372425	627723	19.54%	2.271%
15	10.399	1235	1243	1259	rBV	527526	935468	29.13%	3.385%
16	10.775	1300	1307	1317	rBV	382082	652755	20.32%	2.362%
17	10.952	1324	1337	1350	rBV	524615	948417	29.53%	3.432%
18	12.369	1572	1578	1587	rVB6	7800	18044	0.56%	0.065%
19	14.045	1857	1863	1874	rVV	1055791	1465663	45.63%	5.303%
20	14.334	1903	1912	1920	rBV	1127148	1639932	51.06%	5.934%
21	14.634	1955	1963	1973	rBV	603650	861931	26.84%	3.119%
22	14.869	1994	2003	2021	rBV	362934	704231	21.93%	2.548%
23	15.634	2125	2133	2148	rBV	1476346	2106159	65.57%	7.621%
24	15.775	2152	2157	2168	rVV	480396	653736	20.35%	2.365%
25	15.875	2170	2174	2178	rVB5	6322	10504	0.33%	0.038%
26	16.492	2274	2279	2281	rBV6	2898	4694	0.15%	0.017%
27	17.304	2413	2417	2423	rBV9	4160	6975	0.22%	0.025%
28	17.422	2431	2437	2447	rBV	760922	1048058	32.63%	3.792%
29	17.522	2447	2454	2467	rBV	1711522	2345585	73.03%	8.487%
30	17.916	2516	2521	2524	rBV7	2526	5809	0.18%	0.021%
31	18.269	2578	2581	2586	rBV7	3672	5712	0.18%	0.021%
32	19.339	2760	2763	2767	rBV3	23202	29901	0.93%	0.108%
33	19.416	2772	2776	2779	rVB	19566	26048	0.81%	0.094%
34	19.775	2831	2837	2843	rBV	2324795	2911386	90.64%	10.534%
35	21.557	3135	3140	3145	rBV	912639	1194202	37.18%	4.321%
36	23.963	3542	3549	3560	rVB2	1549364	3211906	100.00%	11.622%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017540.D
Acq On : 04 Oct 2023 19:24
Operator : MA/JU
Sample : PB156008BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION

37	24.133	3572	3578	3587	rVB	634301	1290306	40.17%	4.669%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 27636963

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017540.D
Acq On : 04 Oct 2023 19:24
Operator : MA/JU
Sample : PB156008BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

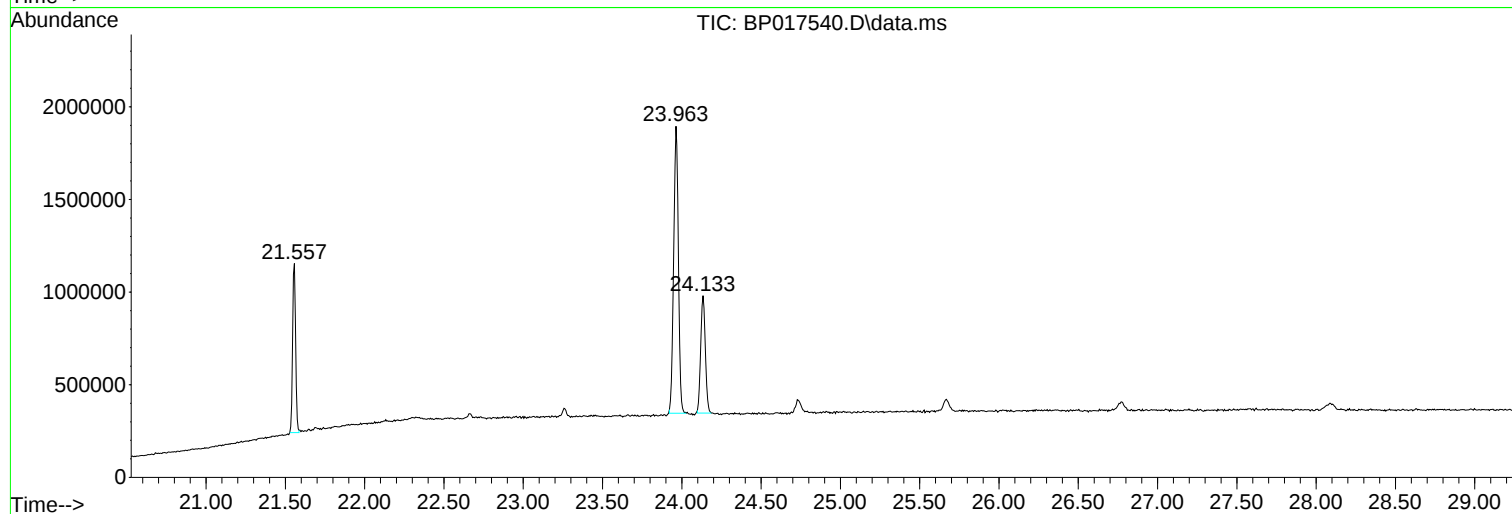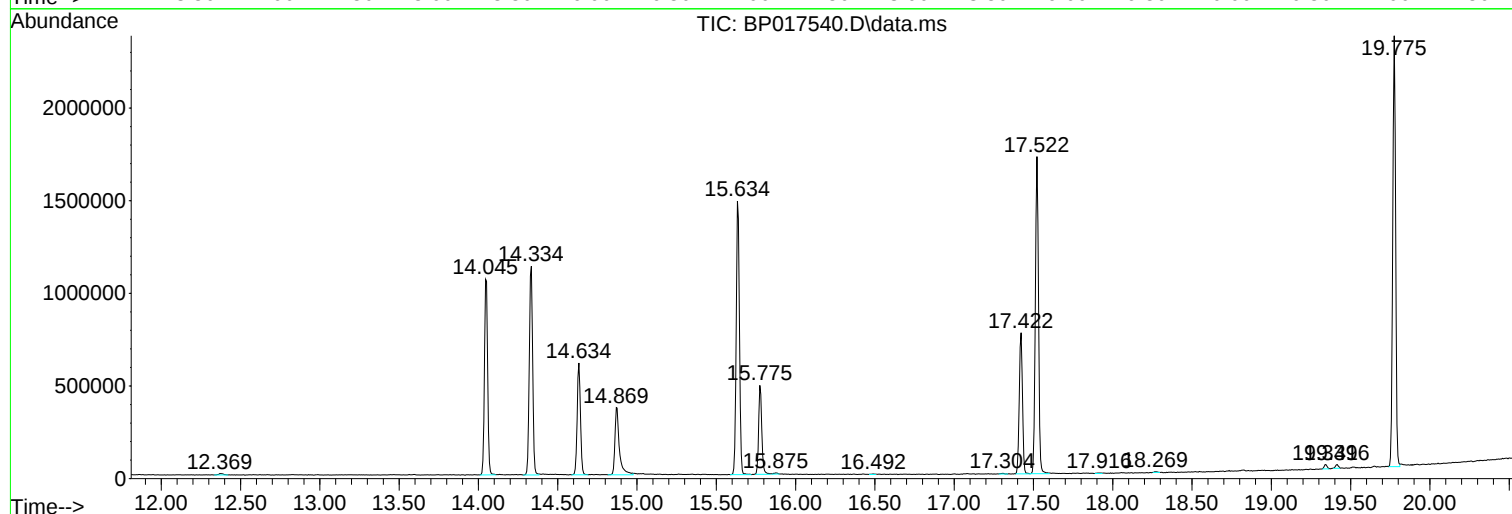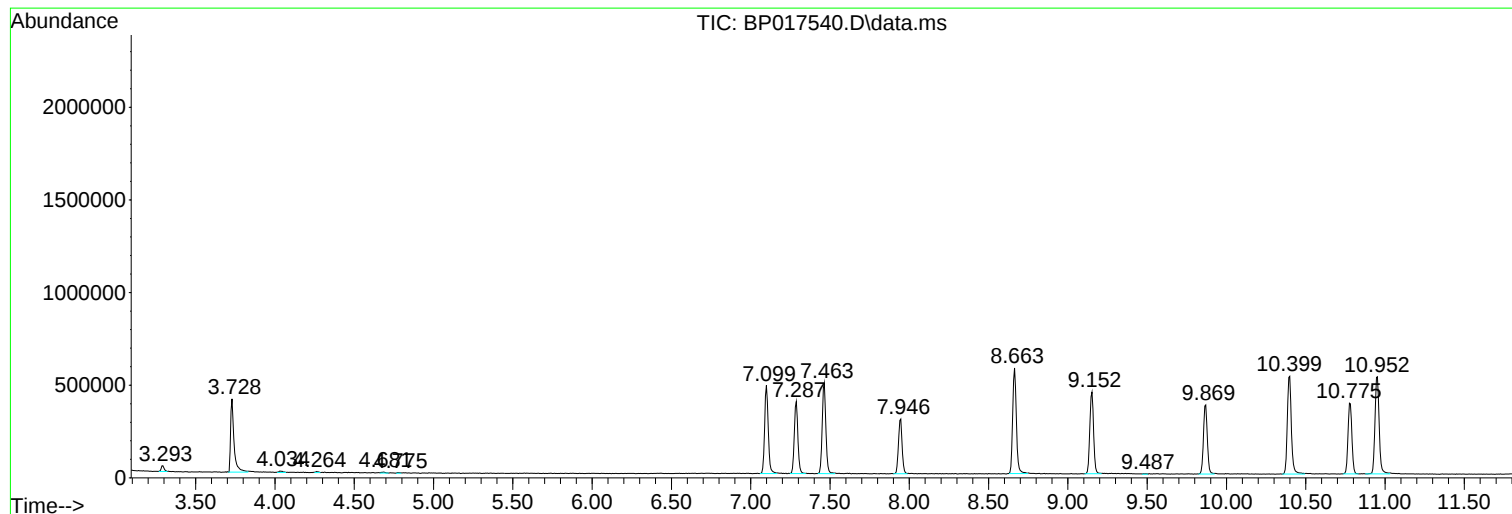

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017540.D
Acq On : 04 Oct 2023 19:24
Operator : MA/JU
Sample : PB156008BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017540.D
Acq On : 04 Oct 2023 19:24
Operator : MA/JU
Sample : PB156008BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc