

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017553.D
 Acq On : 05 Oct 2023 06:46
 Operator : MA/JU
 Sample : PB156005BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017559.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	31	34	39	rBV	37159	46062	1.06%	0.120%
2	3.722	105	108	120	rBV	447758	675232	15.60%	1.763%
3	4.028	158	160	170	rVB3	9036	13165	0.30%	0.034%
4	7.093	674	681	696	rBV	574260	943210	21.78%	2.463%
5	7.281	706	713	722	rVB	459721	706485	16.32%	1.844%
6	7.457	733	743	754	rBV	605985	936371	21.63%	2.445%
7	7.940	818	825	833	rBV	471102	749825	17.32%	1.958%
8	8.657	940	947	970	rBV	688554	1158380	26.75%	3.024%
9	9.146	1022	1030	1042	rBV	546572	895885	20.69%	2.339%
10	9.863	1143	1152	1162	rBV	474811	775756	17.92%	2.025%
11	10.393	1234	1242	1252	rBV	683828	1183071	27.32%	3.089%
12	10.775	1295	1307	1316	rVV	657928	1094873	25.29%	2.858%
13	10.945	1328	1336	1353	rBV	691579	1206344	27.86%	3.150%
14	11.481	1423	1427	1432	rBV8	3098	4368	0.10%	0.011%
15	11.834	1484	1487	1493	rVB7	2506	5110	0.12%	0.013%
16	12.375	1572	1579	1584	rBV2	10602	19062	0.44%	0.050%
17	14.045	1857	1863	1878	rVV	1377183	1854659	42.84%	4.842%
18	14.328	1904	1911	1922	rBV	1411789	2092224	48.32%	5.462%
19	14.634	1956	1963	1973	rBV	1018779	1504839	34.76%	3.929%
20	14.875	1997	2004	2021	rBV	503772	935874	21.62%	2.443%
21	15.039	2029	2032	2037	rVB7	4235	7404	0.17%	0.019%
22	15.263	2066	2070	2073	rBV6	3383	5184	0.12%	0.014%
23	15.428	2092	2098	2099	rBV6	3197	4632	0.11%	0.012%
24	15.633	2125	2133	2146	rBV	1855390	2697593	62.31%	7.043%
25	15.775	2151	2157	2169	rVV	567296	767661	17.73%	2.004%
26	15.875	2171	2174	2180	rVB8	8833	16079	0.37%	0.042%
27	16.422	2265	2267	2272	rVB4	4045	6204	0.14%	0.016%
28	17.422	2430	2437	2447	rBV	1384334	1919736	44.34%	5.012%
29	17.522	2447	2454	2467	rVV2	2172785	3069481	70.89%	8.014%
30	17.827	2503	2506	2508	rBV4	4266	4750	0.11%	0.012%
31	18.269	2577	2581	2586	rBV6	10570	16922	0.39%	0.044%
32	19.345	2760	2764	2769	rVB3	27338	38207	0.88%	0.100%
33	19.416	2772	2776	2782	rVB	28168	41050	0.95%	0.107%
34	19.510	2790	2792	2796	rBV4	10336	14492	0.33%	0.038%
35	19.774	2831	2837	2843	rBV	2949471	3883449	89.69%	10.139%
36	21.557	3135	3140	3146	rBV	1769199	2267555	52.37%	5.920%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017553.D
Acq On : 05 Oct 2023 06:46
Operator : MA/JU
Sample : PB156005BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION

37	23.968	3542	3550	3561	rVB2	2132343	4329648	100.00%	11.304%
38	24.139	3572	3579	3588	rVB	1138671	2411573	55.70%	6.296%




Sum of corrected areas: 38302415

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017553.D
Acq On : 05 Oct 2023 06:46
Operator : MA/JU
Sample : PB156005BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

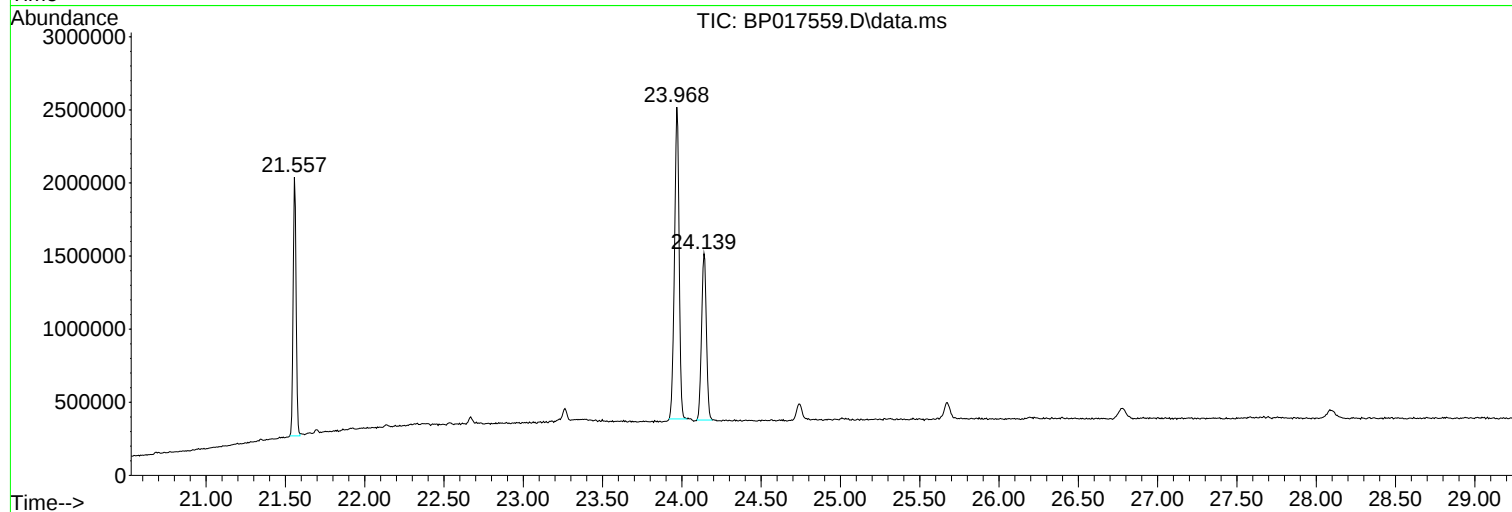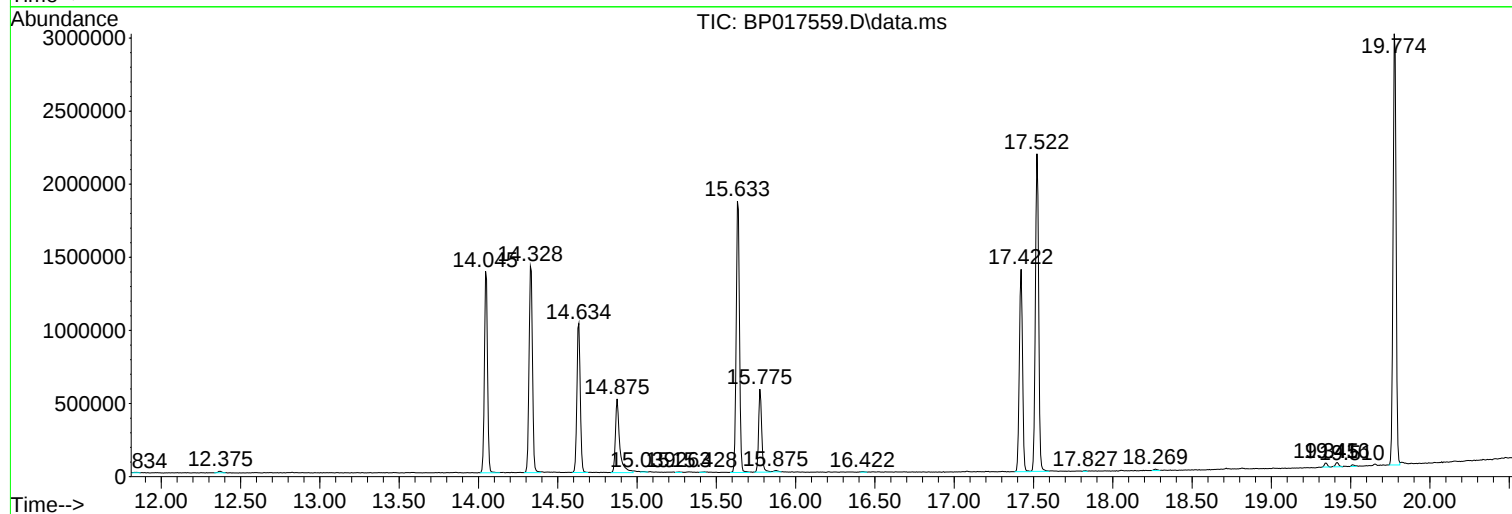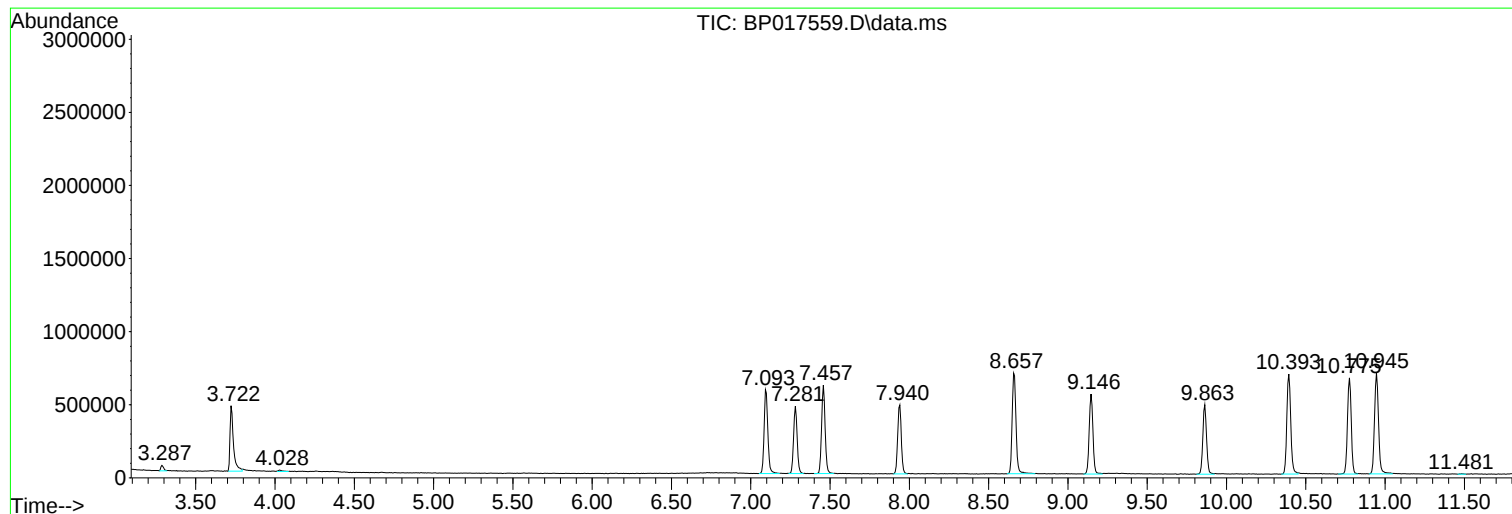

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017553.D
Acq On : 05 Oct 2023 06:46
Operator : MA/JU
Sample : PB156005BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017553.D
Acq On : 05 Oct 2023 06:46
Operator : MA/JU
Sample : PB156005BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------