

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017555.D
 Acq On : 05 Oct 2023 07:53
 Operator : MA/JU
 Sample : PB156007BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	31	34	39	rBV	33442	41613	1.08%	0.133%
2	3.722	105	108	125	rBV	412737	633796	16.40%	2.033%
3	4.028	157	160	168	rVB6	8233	14223	0.37%	0.046%
4	4.681	266	271	273	rBV6	2452	4928	0.13%	0.016%
5	6.934	652	654	657	rVB4	4566	4226	0.11%	0.014%
6	7.093	674	681	693	rBV	514987	831060	21.51%	2.665%
7	7.281	704	713	725	rBV	412043	638955	16.54%	2.049%
8	7.457	737	743	760	rVB	534197	852829	22.07%	2.735%
9	7.940	818	825	834	rBV	319347	506816	13.12%	1.625%
10	8.193	867	868	873	rBV5	2864	4111	0.11%	0.013%
11	8.657	940	947	963	rBV	612972	1029236	26.64%	3.301%
12	9.146	1022	1030	1038	rBV	479036	780315	20.20%	2.503%
13	9.257	1046	1049	1050	rBV3	4557	4601	0.12%	0.015%
14	9.863	1145	1152	1162	rVV	413900	671099	17.37%	2.152%
15	10.393	1234	1242	1254	rBV	604289	1046471	27.08%	3.356%
16	10.775	1297	1307	1314	rBV	430704	720863	18.66%	2.312%
17	10.945	1328	1336	1353	rBV	604379	1055793	27.33%	3.386%
18	11.834	1481	1487	1492	rBV10	3178	7863	0.20%	0.025%
19	12.375	1571	1579	1585	rBV3	11610	21090	0.55%	0.068%
20	12.728	1636	1639	1642	rBV5	2764	4655	0.12%	0.015%
21	12.822	1651	1655	1658	rBV6	2651	4440	0.11%	0.014%
22	13.469	1763	1765	1770	rVB6	3021	4357	0.11%	0.014%
23	14.045	1857	1863	1874	rBV	1190586	1589590	41.14%	5.098%
24	14.328	1904	1911	1922	rBV	1226472	1796751	46.50%	5.762%
25	14.634	1955	1963	1976	rVB	651114	969131	25.08%	3.108%
26	14.875	1998	2004	2018	rBV	403604	762698	19.74%	2.446%
27	15.069	2036	2037	2046	rVB9	3276	6954	0.18%	0.022%
28	15.633	2123	2133	2141	rBV	1699057	2354351	60.93%	7.551%
29	15.775	2152	2157	2169	rBV	475045	643255	16.65%	2.063%
30	15.875	2171	2174	2182	rVB8	9162	16572	0.43%	0.053%
31	16.498	2277	2280	2284	rVB6	3316	4504	0.12%	0.014%
32	17.075	2374	2378	2381	rBV5	4200	6751	0.17%	0.022%
33	17.422	2428	2437	2443	rBV	861638	1222314	31.63%	3.920%
34	17.522	2447	2454	2466	rVV	1916758	2651413	68.62%	8.503%
35	18.263	2577	2580	2585	rBV6	7057	11465	0.30%	0.037%
36	19.345	2760	2764	2767	rBV4	25458	33040	0.86%	0.106%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017555.D
Acq On : 05 Oct 2023 07:53
Operator : MA/JU
Sample : PB156007BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK007

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION

37	19.416	2772	2776	2780	rVV	24055	31729	0.82%	0.102%
38	19.774	2831	2837	2843	rBV	2781429	3368998	87.19%	10.805%
39	21.557	3135	3140	3148	rBV	1146435	1449104	37.50%	4.647%
40	23.962	3541	3549	3559	rVB2	1795836	3863815	100.00%	12.392%
41	24.133	3572	3578	3587	rVB	741206	1514954	39.21%	4.859%




Sum of corrected areas: 31180729

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017555.D
Acq On : 05 Oct 2023 07:53
Operator : MA/JU
Sample : PB156007BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

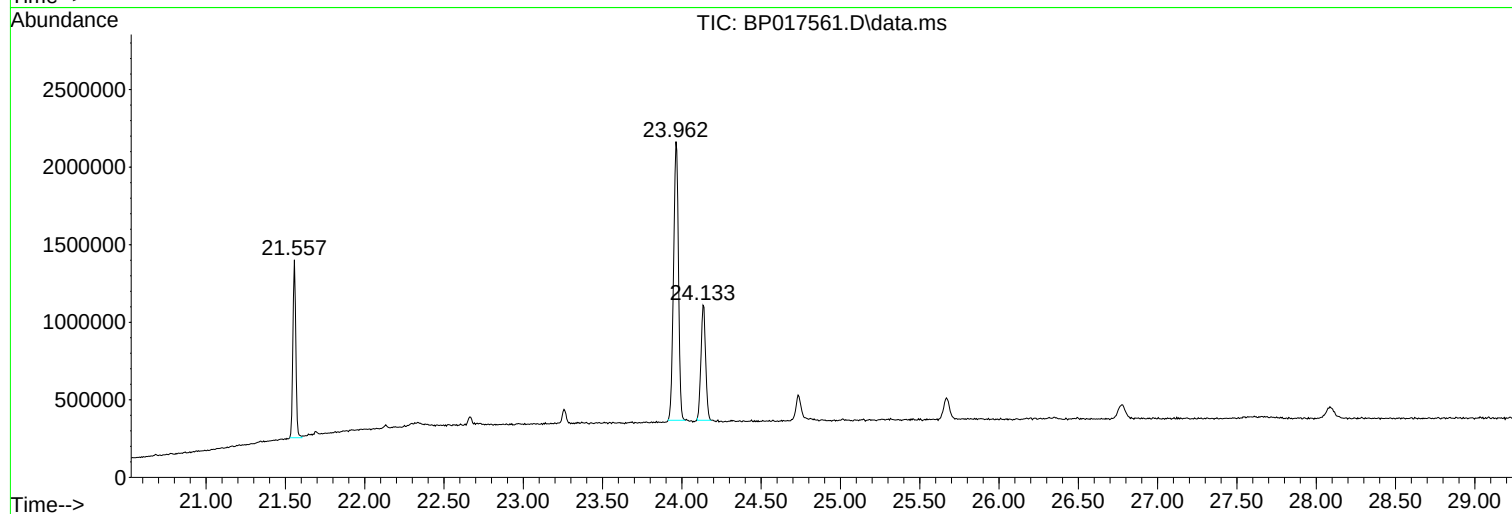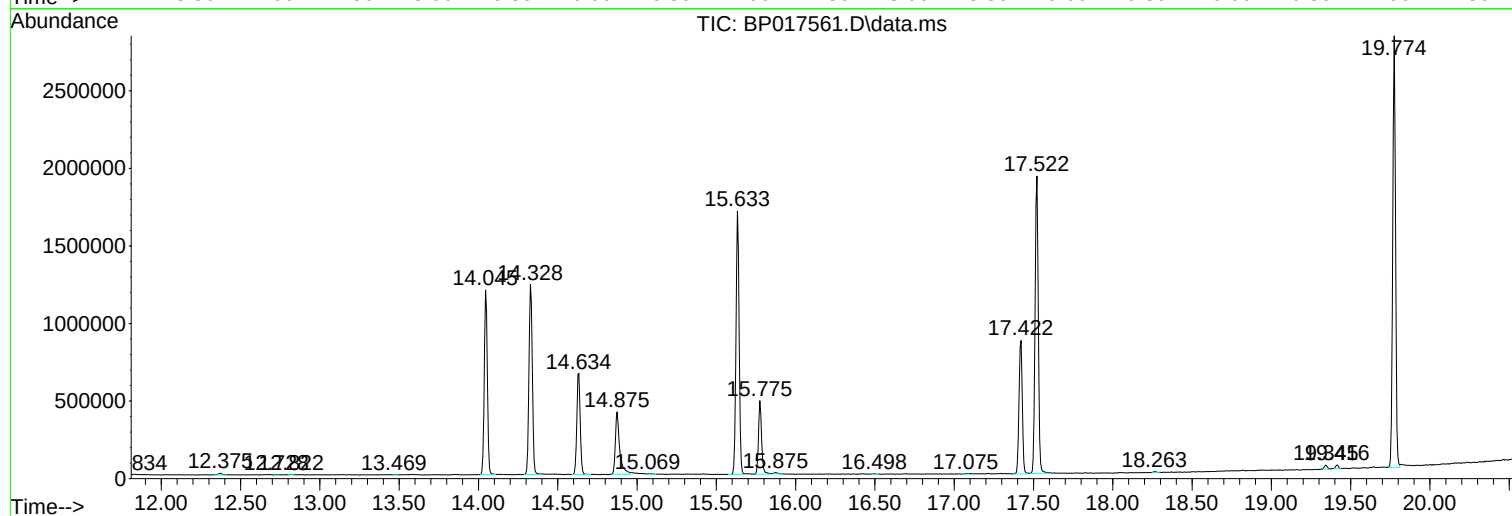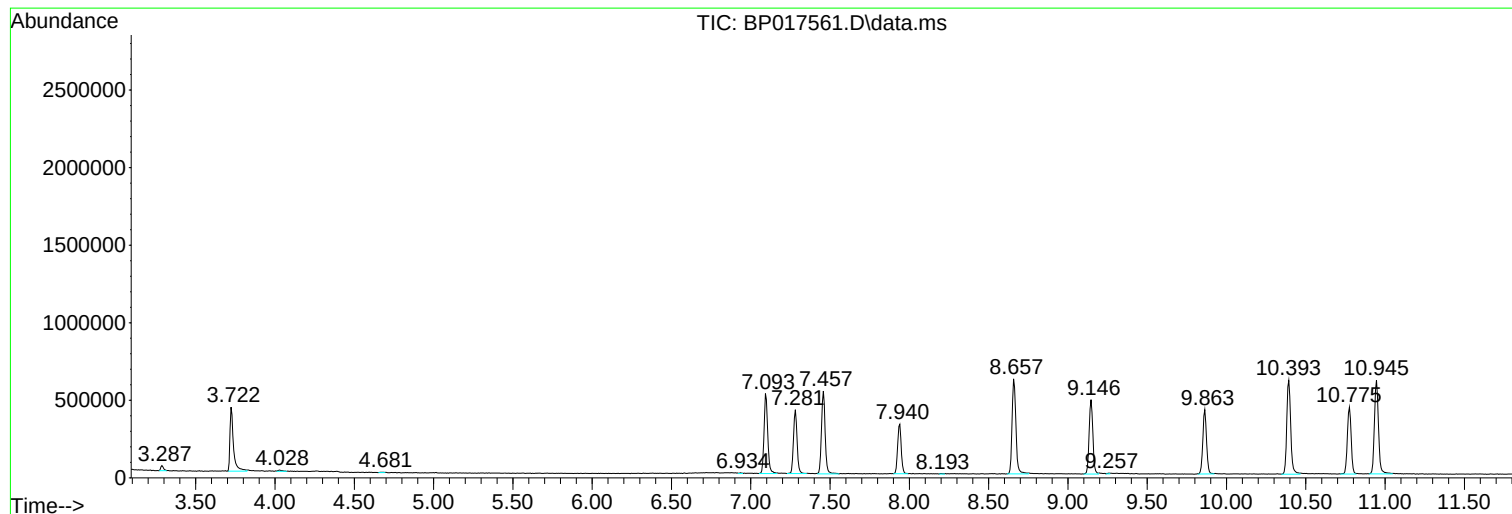

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017555.D
Acq On : 05 Oct 2023 07:53
Operator : MA/JU
Sample : PB156007BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017555.D
Acq On : 05 Oct 2023 07:53
Operator : MA/JU
Sample : PB156007BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------