

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017558.D
 Acq On : 05 Oct 2023 10:50
 Operator : MA/JU
 Sample : 04679-22
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EB(20230928)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	39	rBV2	17729	24896	0.78%	0.092%
2	3.640	91	94	98	rVB2	8199	11162	0.35%	0.041%
3	3.740	107	111	121	rBV	60481	108475	3.38%	0.401%
4	3.917	137	141	144	rBV6	5344	9642	0.30%	0.036%
5	4.034	157	161	165	rBV2	12464	15666	0.49%	0.058%
6	4.552	247	249	252	rBV4	3665	4775	0.15%	0.018%
7	4.611	258	259	265	rVB6	3110	3909	0.12%	0.014%
8	4.834	296	297	301	rBV4	3531	5037	0.16%	0.019%
9	5.381	386	390	392	rBV5	2572	4313	0.13%	0.016%
10	6.781	625	628	631	rBV4	2832	3326	0.10%	0.012%
11	7.105	675	683	697	rVB	85718	155380	4.84%	0.574%
12	7.287	707	714	725	rBV	341427	543398	16.94%	2.007%
13	7.463	737	744	755	rBV	333903	534096	16.65%	1.972%
14	7.552	758	759	766	rVB6	3590	6553	0.20%	0.024%
15	7.946	819	826	837	rBV	384388	635925	19.83%	2.348%
16	8.669	941	949	958	rBV	230955	408264	12.73%	1.508%
17	8.805	968	972	976	rVB3	11425	17271	0.54%	0.064%
18	8.899	985	988	992	rVB5	2158	3329	0.10%	0.012%
19	9.069	1014	1017	1020	rBV5	3004	4144	0.13%	0.015%
20	9.152	1020	1031	1038	rBV	408053	672199	20.96%	2.482%
21	9.346	1060	1064	1068	rVB7	5118	7701	0.24%	0.028%
22	9.869	1143	1153	1164	rBV	338595	552091	17.21%	2.039%
23	10.399	1236	1243	1261	rBV	450185	794713	24.78%	2.935%
24	10.781	1298	1308	1316	rBV	549310	872785	27.21%	3.223%
25	10.851	1318	1320	1326	rVB7	3226	4899	0.15%	0.018%
26	10.951	1326	1337	1352	rBV	470009	824291	25.70%	3.044%
27	11.275	1387	1392	1398	rBV	18047	29921	0.93%	0.110%
28	11.340	1398	1403	1412	rBV2	23010	40602	1.27%	0.150%
29	11.475	1423	1426	1429	rVB4	2850	4187	0.13%	0.015%
30	11.516	1429	1433	1436	rBV6	2602	3564	0.11%	0.013%
31	11.563	1436	1441	1443	rBV6	2990	4080	0.13%	0.015%
32	11.616	1448	1450	1452	rVB3	3367	3234	0.10%	0.012%
33	11.787	1472	1479	1481	rBV8	2329	4591	0.14%	0.017%
34	12.375	1574	1579	1586	rVB3	9318	15478	0.48%	0.057%
35	12.628	1619	1622	1624	rBV4	3395	3617	0.11%	0.013%
36	12.822	1652	1655	1660	rVB6	3684	5215	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017558.D
 Acq On : 05 Oct 2023 10:50
 Operator : MA/JU
 Sample : 04679-22
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EB(20230928)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

37	13.475	1760	1766	1772	rVB3	17738	27829	0.87%	0.103%
38	13.569	1778	1782	1784	rBV5	2370	3416	0.11%	0.013%
39	13.593	1784	1786	1790	rVB5	3907	4662	0.15%	0.017%
40	13.851	1827	1830	1834	rVB6	4971	5855	0.18%	0.022%
41	13.951	1843	1847	1850	rBV6	3142	3319	0.10%	0.012%
42	14.051	1858	1864	1877	rBV	960071	1313943	40.97%	4.852%
43	14.263	1895	1900	1905	rVB8	2989	4755	0.15%	0.018%
44	14.334	1905	1912	1923	rBV	1061948	1521374	47.43%	5.618%
45	14.640	1956	1964	1972	rBV	792300	1182039	36.85%	4.365%
46	14.781	1983	1988	1989	rBV5	2405	3212	0.10%	0.012%
47	14.898	2002	2008	2015	rBV	40978	93776	2.92%	0.346%
48	15.428	2094	2098	2101	rBV6	3713	5192	0.16%	0.019%
49	15.639	2127	2134	2150	rBV	1429495	1993330	62.15%	7.361%
50	15.781	2153	2158	2167	rVV	373700	539025	16.81%	1.991%
51	15.881	2171	2175	2181	rVV9	9686	21086	0.66%	0.078%
52	15.922	2181	2182	2187	rVB5	3677	3632	0.11%	0.013%
53	16.492	2274	2279	2281	rBV5	3042	3433	0.11%	0.013%
54	16.569	2289	2292	2296	rVB6	2266	3899	0.12%	0.014%
55	16.775	2324	2327	2332	rBV6	3189	5427	0.17%	0.020%
56	17.098	2376	2382	2384	rBV7	3633	5881	0.18%	0.022%
57	17.157	2387	2392	2395	rBV7	4019	6907	0.22%	0.026%
58	17.216	2397	2402	2405	rBV7	3962	6043	0.19%	0.022%
59	17.310	2414	2418	2422	rBV7	2509	3329	0.10%	0.012%
60	17.428	2431	2438	2448	rBV	1055336	1443332	45.00%	5.330%
61	17.528	2449	2455	2467	rVV	1673055	2325899	72.52%	8.589%
62	18.145	2558	2560	2564	rBV4	3049	5432	0.17%	0.020%
63	18.275	2577	2582	2591	rBV	86962	139378	4.35%	0.515%
64	18.663	2646	2648	2649	rBV2	5148	4429	0.14%	0.016%
65	19.345	2761	2764	2768	rBV3	23598	29599	0.92%	0.109%
66	19.404	2770	2774	2784	rVV3	69472	131832	4.11%	0.487%
67	19.516	2790	2793	2798	rBV3	34290	41217	1.29%	0.152%
68	19.780	2833	2838	2845	rBV	2410102	2975754	92.78%	10.989%
69	21.216	3080	3082	3089	rVB6	51945	68516	2.14%	0.253%
70	21.563	3136	3141	3147	rBV	1388804	1756069	54.75%	6.485%
71	23.974	3544	3551	3562	rVB	1594058	3207378	100.00%	11.845%
72	24.145	3574	3580	3589	rVB	886149	1845879	57.55%	6.817%




Sum of corrected areas: 27078807

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017558.D
Acq On : 05 Oct 2023 10:50
Operator : MA/JU
Sample : 04679-22
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB(20230928)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

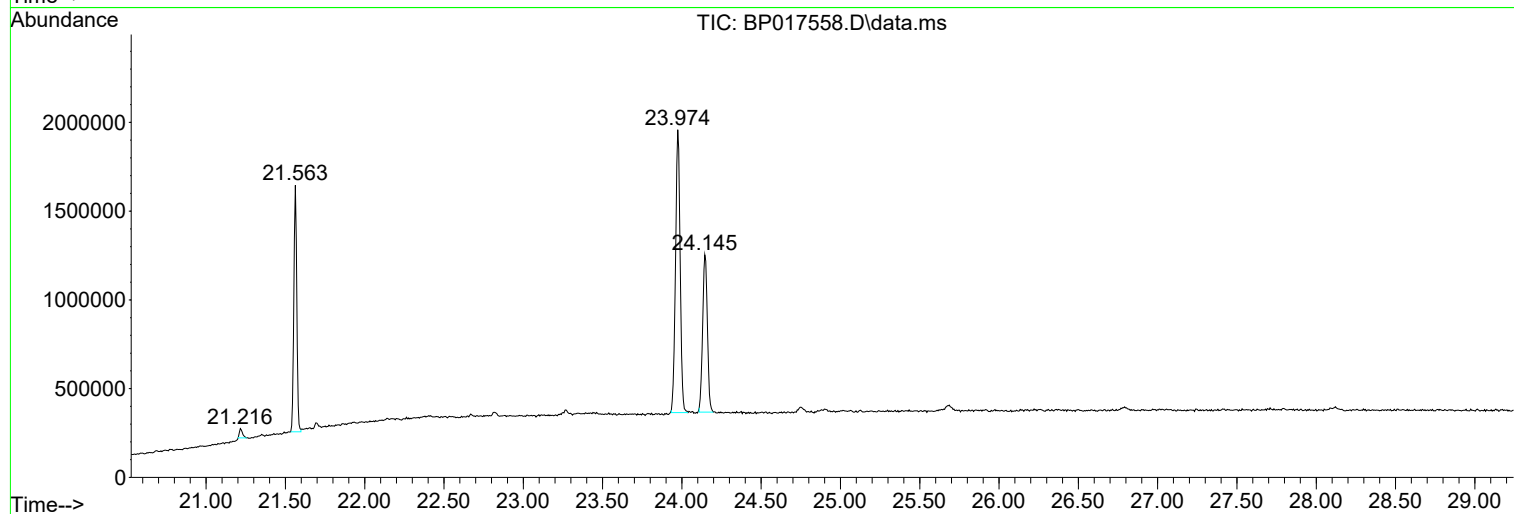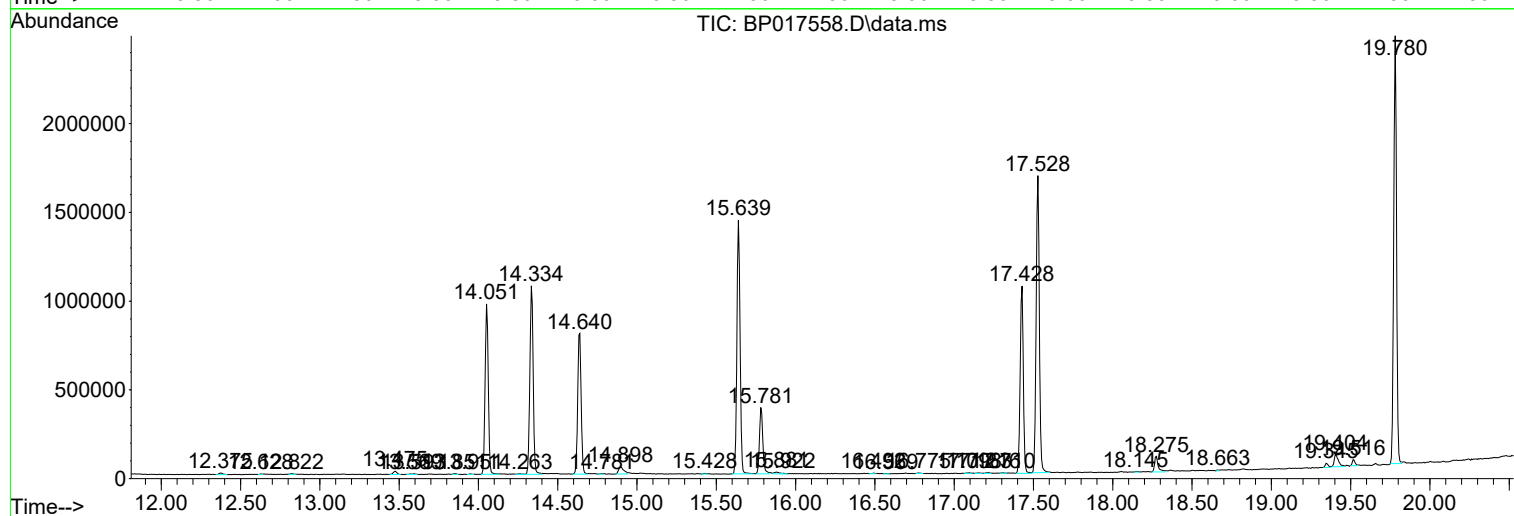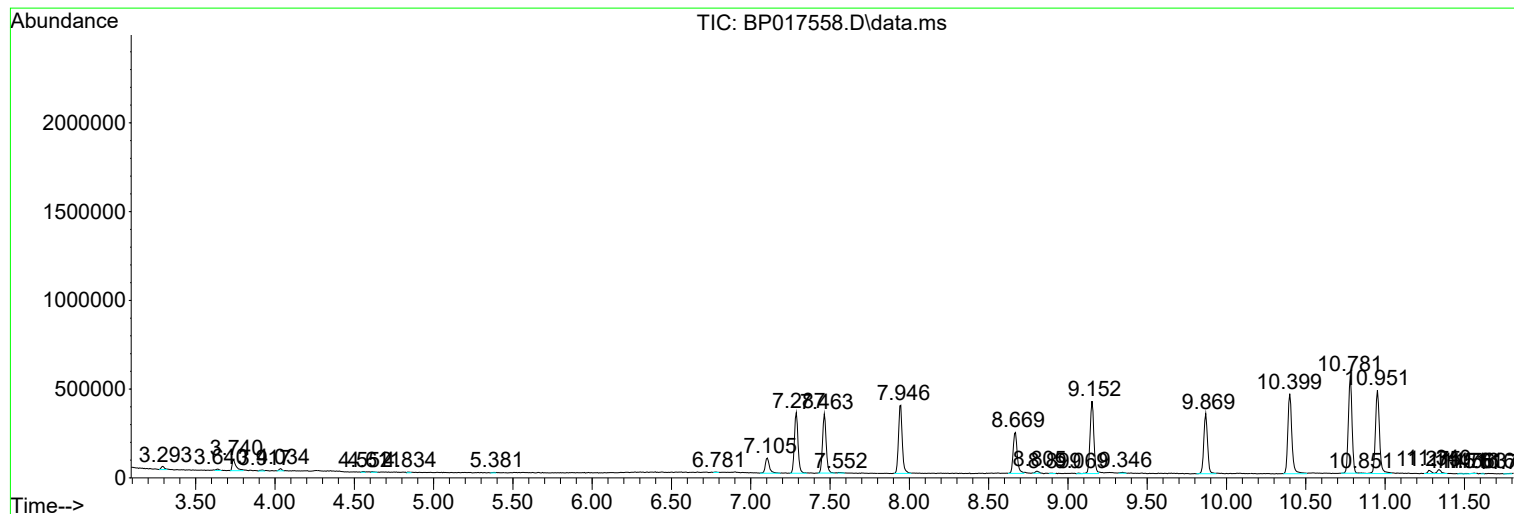

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017558.D
Acq On : 05 Oct 2023 10:50
Operator : MA/JU
Sample : 04679-22
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB(20230928)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017558.D
Acq On : 05 Oct 2023 10:50
Operator : MA/JU
Sample : 04679-22
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB(20230928)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc