

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017569.D
 Acq On : 05 Oct 2023 17:05
 Operator : MA/JU
 Sample : PB155909BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK909

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017569.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	39	rVB	36877	44156	1.24%	0.138%
2	3.723	104	108	125	rBV	440818	669250	18.76%	2.097%
3	4.034	157	161	167	rVB7	6465	9071	0.25%	0.028%
4	5.452	400	402	407	rVB6	3044	3974	0.11%	0.012%
5	7.093	675	681	692	rBV	522494	847010	23.74%	2.654%
6	7.281	705	713	720	rBV	422877	641939	17.99%	2.011%
7	7.458	737	743	757	rBV	551731	865623	24.26%	2.712%
8	7.940	817	825	832	rBV	339355	546425	15.32%	1.712%
9	8.658	940	947	959	rBV	615303	1032819	28.95%	3.236%
10	9.146	1023	1030	1040	rVV	485673	806980	22.62%	2.528%
11	9.863	1143	1152	1161	rBV	436346	708536	19.86%	2.220%
12	10.393	1235	1242	1256	rBV	637242	1098241	30.78%	3.441%
13	10.775	1298	1307	1314	rBV	456859	765319	21.45%	2.398%
14	10.946	1326	1336	1352	rBV	629964	1097793	30.77%	3.439%
15	12.375	1573	1579	1588	rBV6	9502	17732	0.50%	0.056%
16	13.469	1760	1765	1770	rBV3	7686	12542	0.35%	0.039%
17	13.587	1781	1785	1788	rBV6	2510	3792	0.11%	0.012%
18	13.863	1828	1832	1836	rBV7	2550	4801	0.13%	0.015%
19	14.046	1857	1863	1873	rBV	1203449	1652998	46.33%	5.179%
20	14.328	1904	1911	1920	rBV	1273251	1865786	52.29%	5.845%
21	14.475	1934	1936	1943	rVB7	3189	5378	0.15%	0.017%
22	14.634	1957	1963	1974	rVB	726437	1038644	29.11%	3.254%
23	14.875	1998	2004	2020	rBV	407025	807707	22.64%	2.530%
24	14.998	2023	2025	2028	rVV4	7593	9530	0.27%	0.030%
25	15.028	2028	2030	2034	rVB5	3758	5325	0.15%	0.017%
26	15.428	2096	2098	2102	rVB5	4203	4779	0.13%	0.015%
27	15.634	2126	2133	2144	rBV	1658503	2378970	66.68%	7.453%
28	15.775	2152	2157	2169	rBV	476907	658817	18.47%	2.064%
29	15.869	2170	2173	2179	rVB7	7700	12768	0.36%	0.040%
30	16.428	2264	2268	2270	rBV4	4281	5928	0.17%	0.019%
31	16.692	2310	2313	2314	rBV3	3612	3619	0.10%	0.011%
32	17.422	2431	2437	2444	rBV	960105	1309946	36.72%	4.104%
33	17.522	2448	2454	2467	rVV2	1974325	2778499	77.88%	8.704%
34	17.822	2503	2505	2510	rBV6	2717	3801	0.11%	0.012%
35	19.345	2760	2764	2768	rBV3	23905	35588	1.00%	0.111%
36	19.416	2773	2776	2780	rVB2	21842	28359	0.79%	0.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017569.D
Acq On : 05 Oct 2023 17:05
Operator : MA/JU
Sample : PB155909BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK909

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION

37	19.775	2831	2837	2846	rBV	2562434	3426342	96.03%	10.734%
38	21.557	3135	3140	3148	rBV	1163724	1548082	43.39%	4.850%
39	23.969	3543	3550	3560	rVB	1726692	3567875	100.00%	11.177%
40	24.139	3573	3579	3589	rVB	793347	1595629	44.72%	4.999%




Sum of corrected areas: 31920373

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017569.D
Acq On : 05 Oct 2023 17:05
Operator : MA/JU
Sample : PB155909BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK909

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

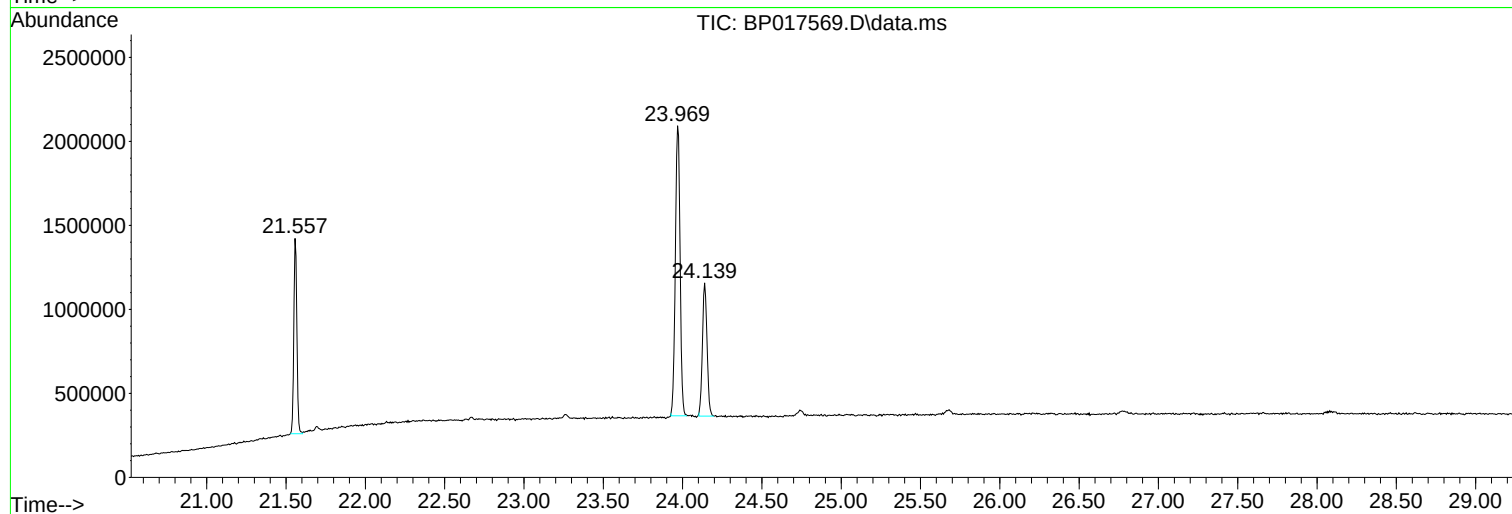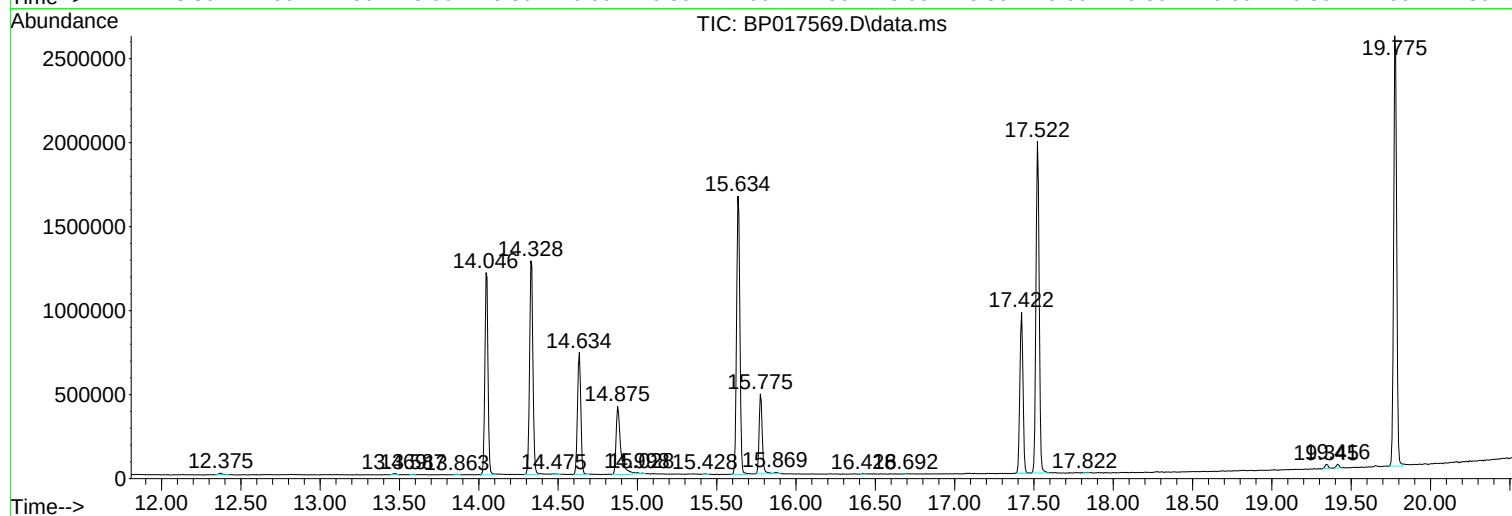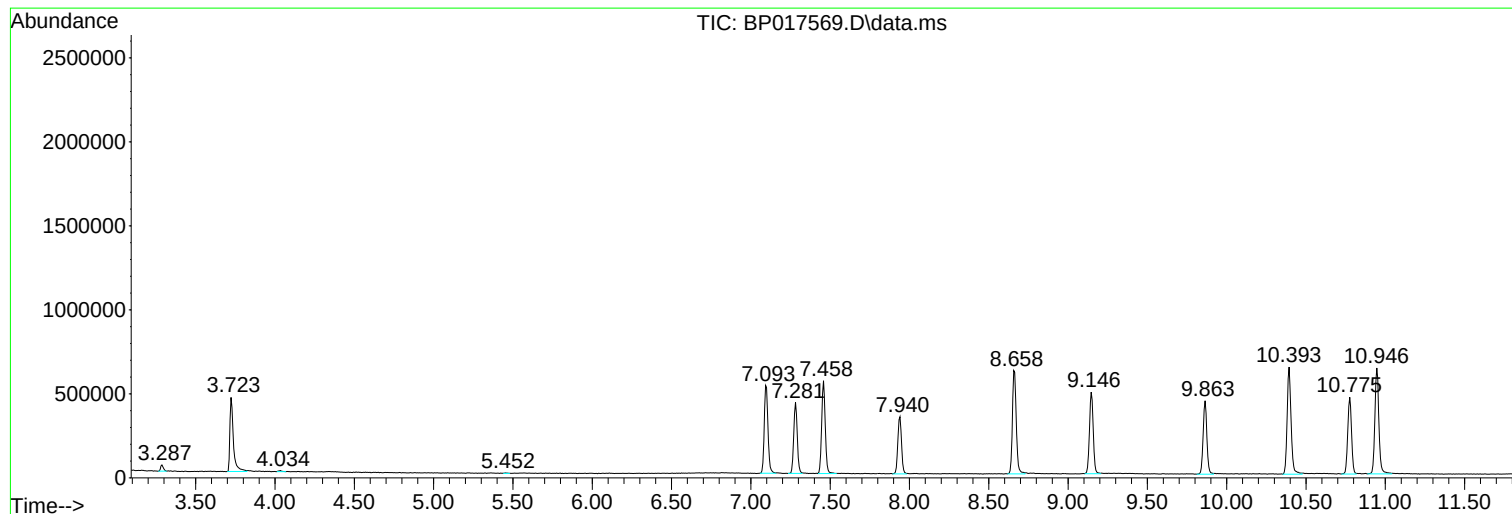

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017569.D
Acq On : 05 Oct 2023 17:05
Operator : MA/JU
Sample : PB155909BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK909

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017569.D
Acq On : 05 Oct 2023 17:05
Operator : MA/JU
Sample : PB155909BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK909

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------