

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017579.D
 Acq On : 05 Oct 2023 22:47
 Operator : MA/JU
 Sample : 04588-19
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	21	26	32	rBV	1234512	1616844	10.86%	3.441%
2	3.558	77	80	84	rVB	14620	19207	0.13%	0.041%
3	3.729	106	109	123	rBV	96753	159086	1.07%	0.339%
4	4.552	243	249	270	rVB	10026562	14882379	100.00%	31.675%
5	5.193	352	358	364	rBV	46106	68659	0.46%	0.146%
6	5.605	424	428	435	rVB6	13871	22295	0.15%	0.047%
7	5.740	447	451	456	rVB4	14019	18461	0.12%	0.039%
8	7.093	676	681	692	rVB	99438	173530	1.17%	0.369%
9	7.275	704	712	725	rBV	429453	673942	4.53%	1.434%
10	7.458	736	743	754	rBV	418883	714066	4.80%	1.520%
11	7.934	818	824	835	rBV	310435	503221	3.38%	1.071%
12	8.293	880	885	891	rVB4	9127	15441	0.10%	0.033%
13	8.658	939	947	958	rBV	325549	531082	3.57%	1.130%
14	8.828	971	976	983	rVB8	10079	17846	0.12%	0.038%
15	9.140	1022	1029	1040	rBV	504721	854880	5.74%	1.819%
16	9.228	1040	1044	1049	rVV4	12269	23901	0.16%	0.051%
17	9.293	1049	1055	1059	rVV7	16370	33335	0.22%	0.071%
18	9.346	1059	1064	1071	rVB8	9911	23769	0.16%	0.051%
19	9.787	1134	1139	1144	rBV2	9891	17554	0.12%	0.037%
20	9.858	1144	1151	1162	rVV	428589	704872	4.74%	1.500%
21	10.387	1234	1241	1256	rBV	583284	1038019	6.97%	2.209%
22	10.769	1299	1306	1318	rBV	420364	698155	4.69%	1.486%
23	10.946	1328	1336	1349	rBV	458929	825133	5.54%	1.756%
24	11.822	1475	1485	1486	rBV7	9844	19940	0.13%	0.042%
25	12.046	1518	1523	1530	rBV	27908	47630	0.32%	0.101%
26	12.240	1548	1556	1560	rBV6	9345	20226	0.14%	0.043%
27	12.340	1569	1573	1581	rVB4	12848	30228	0.20%	0.064%
28	13.469	1759	1765	1771	rBV9	11460	22976	0.15%	0.049%
29	14.046	1855	1863	1871	rBV	1238512	1696350	11.40%	3.610%
30	14.328	1903	1911	1923	rBV	1384214	1988208	13.36%	4.232%
31	14.628	1956	1962	1972	rBV	660855	958159	6.44%	2.039%
32	14.887	1997	2006	2015	rBV3	56021	143342	0.96%	0.305%
33	15.634	2126	2133	2144	rBV	1827430	2561895	17.21%	5.453%
34	15.775	2151	2157	2168	rBV	512543	745454	5.01%	1.587%
35	15.869	2170	2173	2182	rVB9	13571	25433	0.17%	0.054%
36	17.416	2430	2436	2446	rBV	857495	1201942	8.08%	2.558%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017579.D
 Acq On : 05 Oct 2023 22:47
 Operator : MA/JU
 Sample : 04588-19
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

37	17.516	2447	2453	2468	rVV	2144294	2928266	19.68%	6.232%
38	18.263	2576	2580	2589	rBV2	70885	111804	0.75%	0.238%
39	19.339	2759	2763	2768	rBV3	30377	45342	0.30%	0.097%
40	19.410	2772	2775	2778	rVV	28846	34243	0.23%	0.073%
41	19.445	2779	2781	2787	rVB2	23521	30419	0.20%	0.065%
42	19.510	2788	2792	2798	rBV3	56067	78020	0.52%	0.166%
43	19.769	2831	2836	2843	rBV	2772483	3657596	24.58%	7.785%
44	20.534	2963	2966	2969	rBV	52072	55627	0.37%	0.118%
45	21.551	3134	3139	3146	rBV	1122870	1443611	9.70%	3.073%
46	23.957	3540	3548	3558	rVB2	1874093	3995602	26.85%	8.504%
47	24.127	3571	3577	3590	rVB	727108	1506765	10.12%	3.207%




Sum of corrected areas: 46984755

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017579.D
Acq On : 05 Oct 2023 22:47
Operator : MA/JU
Sample : 04588-19
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHW1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

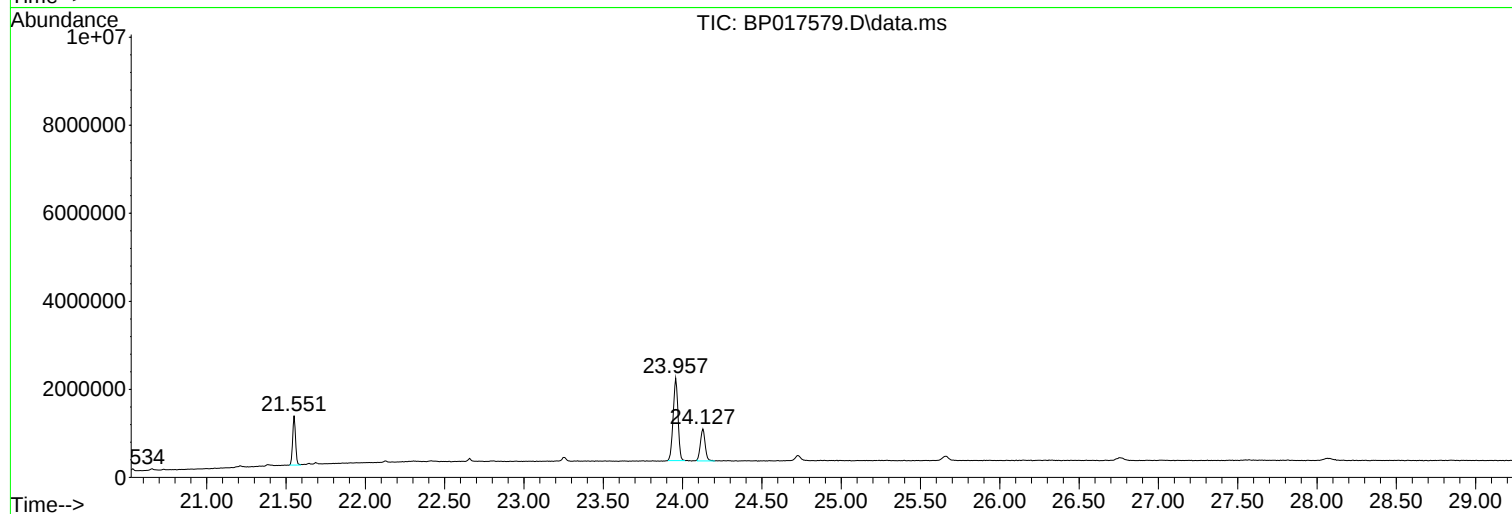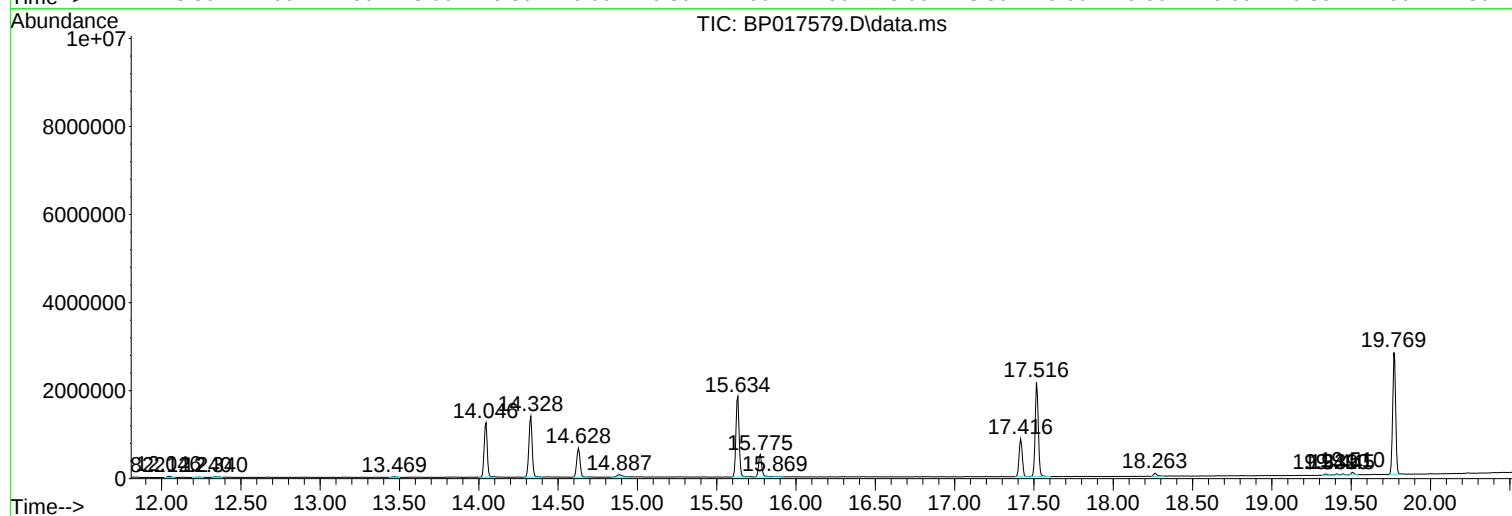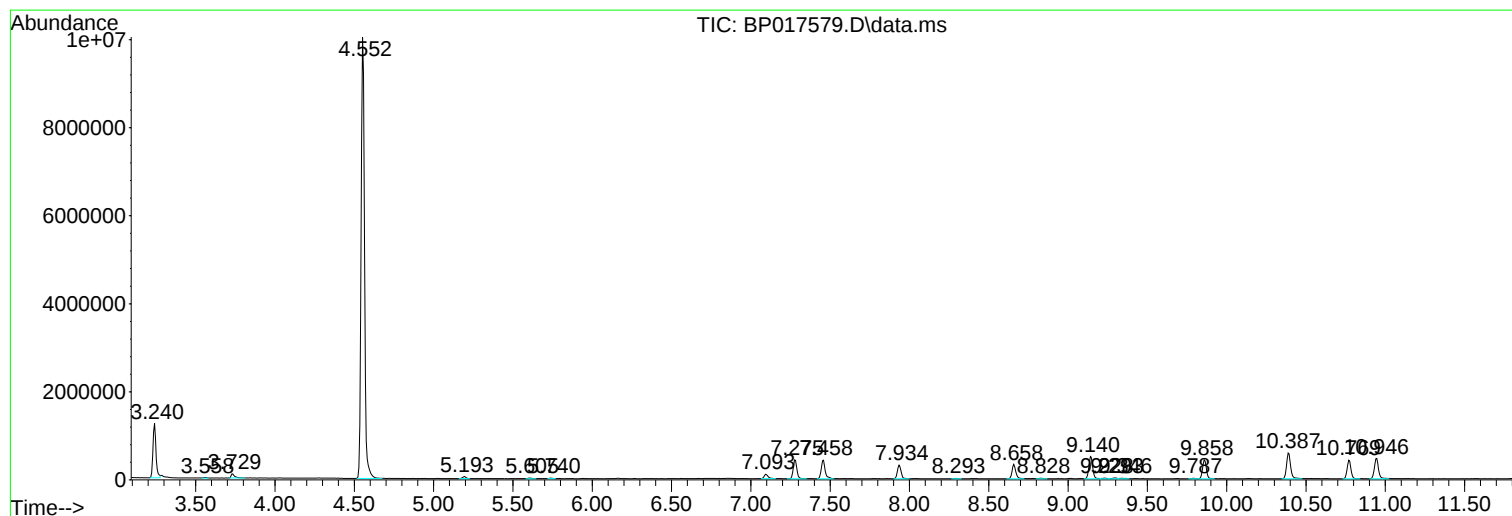

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017579.D
Acq On : 05 Oct 2023 22:47
Operator : MA/JU
Sample : 04588-19
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHW1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.552	591.49 ng/ul	14882400	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

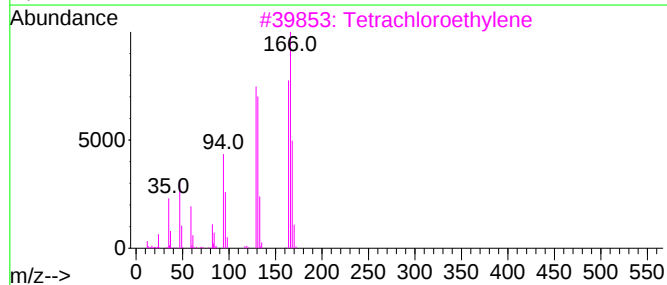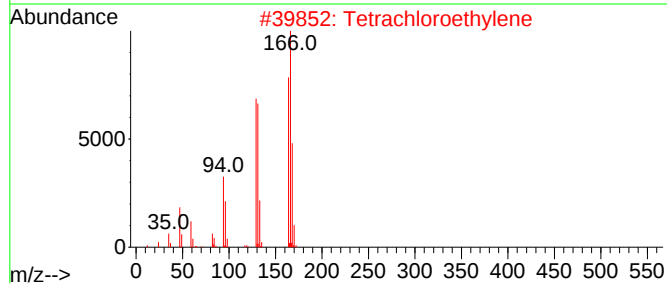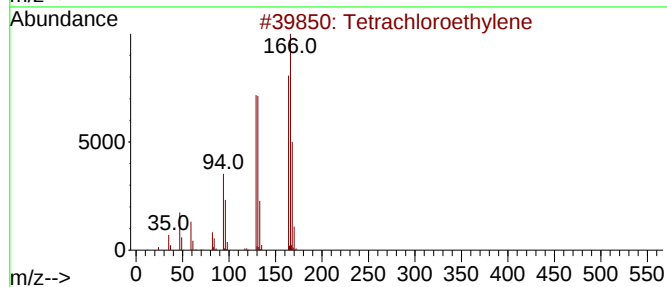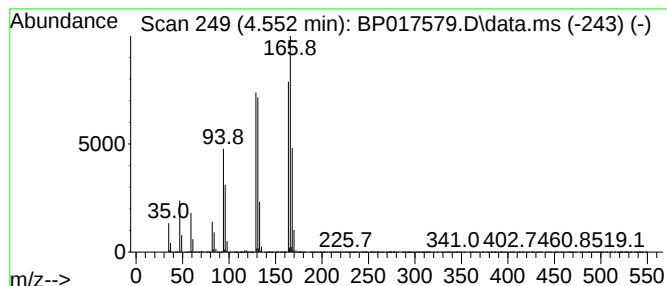

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017579.D
Acq On : 05 Oct 2023 22:47
Operator : MA/JU
Sample : 04588-19
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHW1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.193	2.73 ng/ul	68659	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, chloro-	112	C6H5Cl	000108-90-7	93
2			Benzene, chloro-	112	C6H5Cl	000108-90-7	93
3			Benzene, chloro-	112	C6H5Cl	000108-90-7	91
4			Benzene, chloro-	112	C6H5Cl	000108-90-7	91
5			Benzene, chloro-	112	C6H5Cl	000108-90-7	90

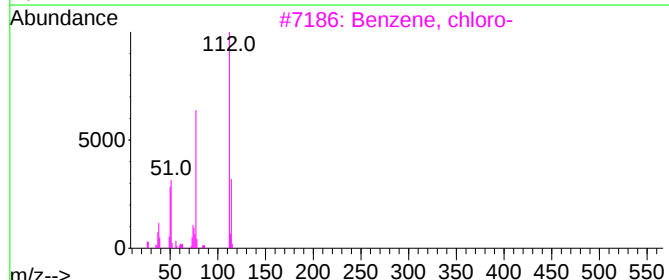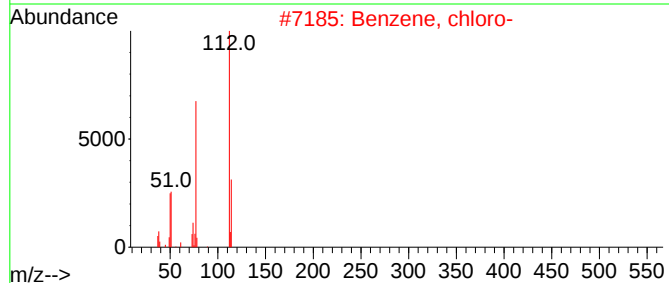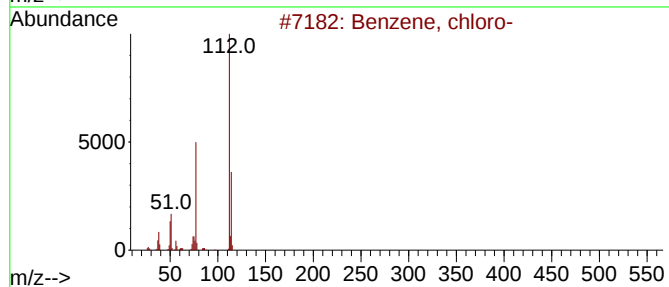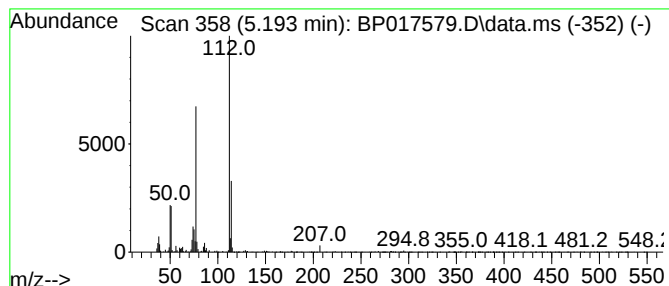

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017579.D
Acq On : 05 Oct 2023 22:47
Operator : MA/JU
Sample : 04588-19
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHW1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.552	591.5	ng/ul	14882400	1	7.934	503221	20.0
Benzene, chloro-	5.193	2.7	ng/ul	68659	1	7.934	503221	20.0