

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017580.D
 Acq On : 05 Oct 2023 23:21
 Operator : MA/JU
 Sample : 04588-10
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	38	rVB	21398	25408	0.64%	0.089%
2	3.475	64	66	69	rBV4	4506	4190	0.11%	0.015%
3	3.728	106	109	122	rBV	95821	168498	4.24%	0.593%
4	3.840	126	128	134	rVV7	10233	14806	0.37%	0.052%
5	3.893	134	137	146	rVB9	7548	16495	0.41%	0.058%
6	4.093	169	171	175	rVB4	7103	8321	0.21%	0.029%
7	4.187	182	187	190	rVB6	5002	7540	0.19%	0.027%
8	4.387	220	221	229	rVB8	6405	9507	0.24%	0.033%
9	4.552	245	249	254	rBV4	17084	23770	0.60%	0.084%
10	4.746	278	282	287	rBV5	6688	8004	0.20%	0.028%
11	4.846	295	299	302	rVB6	4796	5614	0.14%	0.020%
12	4.975	317	321	325	rVV4	8539	12128	0.30%	0.043%
13	5.022	325	329	334	rVB3	13588	19198	0.48%	0.068%
14	5.264	367	370	374	rBV5	13627	20808	0.52%	0.073%
15	5.399	390	393	399	rVB2	11526	15309	0.38%	0.054%
16	5.646	431	435	440	rVB7	6164	10866	0.27%	0.038%
17	5.705	441	445	450	rVV8	6857	12737	0.32%	0.045%
18	5.793	453	460	468	rVV2	17310	32935	0.83%	0.116%
19	5.864	468	472	476	rVB5	8945	12202	0.31%	0.043%
20	6.093	506	511	512	rBV4	10785	12038	0.30%	0.042%
21	6.216	528	532	539	rVB7	8322	15858	0.40%	0.056%
22	6.305	542	547	550	rBV7	5151	6835	0.17%	0.024%
23	6.387	550	561	567	rVV6	26172	70113	1.76%	0.247%
24	6.434	567	569	572	rVV4	5078	6351	0.16%	0.022%
25	6.487	573	578	584	rVB4	33523	55417	1.39%	0.195%
26	6.593	593	596	601	rVB7	5584	7840	0.20%	0.028%
27	6.664	602	608	611	rBV8	7465	13041	0.33%	0.046%
28	6.734	613	620	625	rVB10	6370	13909	0.35%	0.049%
29	6.822	632	635	639	rBV5	10031	12989	0.33%	0.046%
30	6.999	660	665	672	rVB6	17517	33088	0.83%	0.116%
31	7.093	677	681	687	rBV	56092	93324	2.35%	0.329%
32	7.169	692	694	703	rVB10	6050	11426	0.29%	0.040%
33	7.275	703	712	720	rBV	358587	575727	14.48%	2.027%
34	7.340	720	723	728	rVB4	8763	11212	0.28%	0.039%
35	7.458	734	743	752	rBV2	325188	588910	14.81%	2.073%
36	7.540	754	757	761	rVV6	5356	8097	0.20%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017580.D
 Acq On : 05 Oct 2023 23:21
 Operator : MA/JU
 Sample : 04588-10
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

37	7.581	761	764	770	rVV8	7169	11202	0.28%	0.039%
38	7.634	770	773	776	rVV4	3788	4215	0.11%	0.015%
39	7.675	776	780	784	rVB7	3477	4819	0.12%	0.017%
40	7.793	796	800	801	rBV4	3001	3980	0.10%	0.014%
41	7.822	801	805	809	rVB5	10815	15896	0.40%	0.056%
42	7.934	817	824	836	rVB	326207	514077	12.93%	1.810%
43	8.034	836	841	848	rVB	8481	21433	0.54%	0.075%
44	8.105	848	853	856	rBV7	4102	5680	0.14%	0.020%
45	8.158	856	862	868	rBV4	8893	16490	0.41%	0.058%
46	8.299	881	886	892	rVB10	4027	8945	0.22%	0.031%
47	8.393	896	902	904	rBV7	3860	7198	0.18%	0.025%
48	8.434	906	909	918	rVB7	3897	7948	0.20%	0.028%
49	8.522	918	924	925	rBV6	2946	4888	0.12%	0.017%
50	8.658	942	947	956	rBV	123259	208859	5.25%	0.735%
51	8.728	956	959	967	rVB9	7826	15348	0.39%	0.054%
52	9.016	1005	1008	1012	rVB6	3642	5509	0.14%	0.019%
53	9.140	1018	1029	1041	rBV	432930	733383	18.44%	2.582%
54	9.234	1041	1045	1053	rVB	5962	16225	0.41%	0.057%
55	9.334	1061	1062	1067	rVB5	5583	4972	0.13%	0.018%
56	9.616	1109	1110	1116	rVB6	3523	4358	0.11%	0.015%
57	9.857	1145	1151	1161	rBV	361162	590742	14.85%	2.080%
58	10.393	1235	1242	1261	rBV	417196	764907	19.23%	2.693%
59	10.769	1299	1306	1315	rBV	440273	713193	17.93%	2.511%
60	10.946	1328	1336	1346	rBV	137332	250950	6.31%	0.883%
61	11.610	1444	1449	1454	rVV8	5394	10431	0.26%	0.037%
62	11.793	1473	1480	1497	rBV	55611	143636	3.61%	0.506%
63	12.146	1538	1540	1546	rVB7	2700	4229	0.11%	0.015%
64	12.369	1574	1578	1584	rVB5	7388	14192	0.36%	0.050%
65	12.698	1630	1634	1643	rVB6	7135	15330	0.39%	0.054%
66	13.463	1758	1764	1770	rBV5	9866	17115	0.43%	0.060%
67	13.845	1825	1829	1833	rVB7	3678	5098	0.13%	0.018%
68	14.045	1856	1863	1874	rBV	1118221	1527976	38.42%	5.379%
69	14.328	1903	1911	1923	rBV	1145608	1654715	41.60%	5.825%
70	14.628	1955	1962	1969	rBV	705421	993832	24.99%	3.499%
71	14.804	1988	1992	2001	rVB	1977	4422	0.11%	0.016%
72	14.887	2001	2006	2020	rBV	45910	126928	3.19%	0.447%
73	15.428	2094	2098	2100	rBV5	2984	4599	0.12%	0.016%
74	15.634	2125	2133	2141	rBV	1674970	2341406	58.87%	8.243%
75	15.710	2142	2146	2151	rVV4	26208	46284	1.16%	0.163%
76	15.775	2151	2157	2170	rVV	476003	727788	18.30%	2.562%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017580.D
 Acq On : 05 Oct 2023 23:21
 Operator : MA/JU
 Sample : 04588-10
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

77	15.875	2170	2174	2181	rVB7	9548	18531	0.47%	0.065%
78	16.369	2250	2258	2260	rBV9	2183	4729	0.12%	0.017%
79	16.416	2262	2266	2269	rBV6	2639	4407	0.11%	0.016%
80	16.934	2352	2354	2357	rBV4	3437	4354	0.11%	0.015%
81	17.081	2375	2379	2384	rVB8	3531	7016	0.18%	0.025%
82	17.416	2429	2436	2446	rBV	942429	1287316	32.37%	4.532%
83	17.516	2447	2453	2467	rVV	1860550	2614932	65.75%	9.206%
84	17.675	2478	2480	2484	rVB4	3708	4789	0.12%	0.017%
85	17.775	2492	2497	2499	rBV5	3371	6448	0.16%	0.023%
86	18.051	2538	2544	2547	rBV8	6940	13677	0.34%	0.048%
87	18.263	2576	2580	2585	rBV	49203	64110	1.61%	0.226%
88	18.804	2667	2672	2677	rBV4	24133	41120	1.03%	0.145%
89	19.339	2759	2763	2766	rBV3	27618	36192	0.91%	0.127%
90	19.410	2772	2775	2779	rVB	25488	31387	0.79%	0.110%
91	19.504	2788	2791	2796	rBV3	35741	47885	1.20%	0.169%
92	19.769	2831	2836	2844	rBV	2680593	3451567	86.78%	12.151%
93	19.851	2847	2850	2857	rVB3	34710	54275	1.36%	0.191%
94	20.192	2905	2908	2917	rBV4	28394	48506	1.22%	0.171%
95	21.551	3134	3139	3145	rBV	1213601	1533041	38.54%	5.397%
96	23.957	3540	3548	3558	rVB2	1945673	3977346	100.00%	14.002%
97	24.127	3571	3577	3588	rVB	781310	1615987	40.63%	5.689%




Sum of corrected areas: 28405324

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017580.D
Acq On : 05 Oct 2023 23:21
Operator : MA/JU
Sample : 04588-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

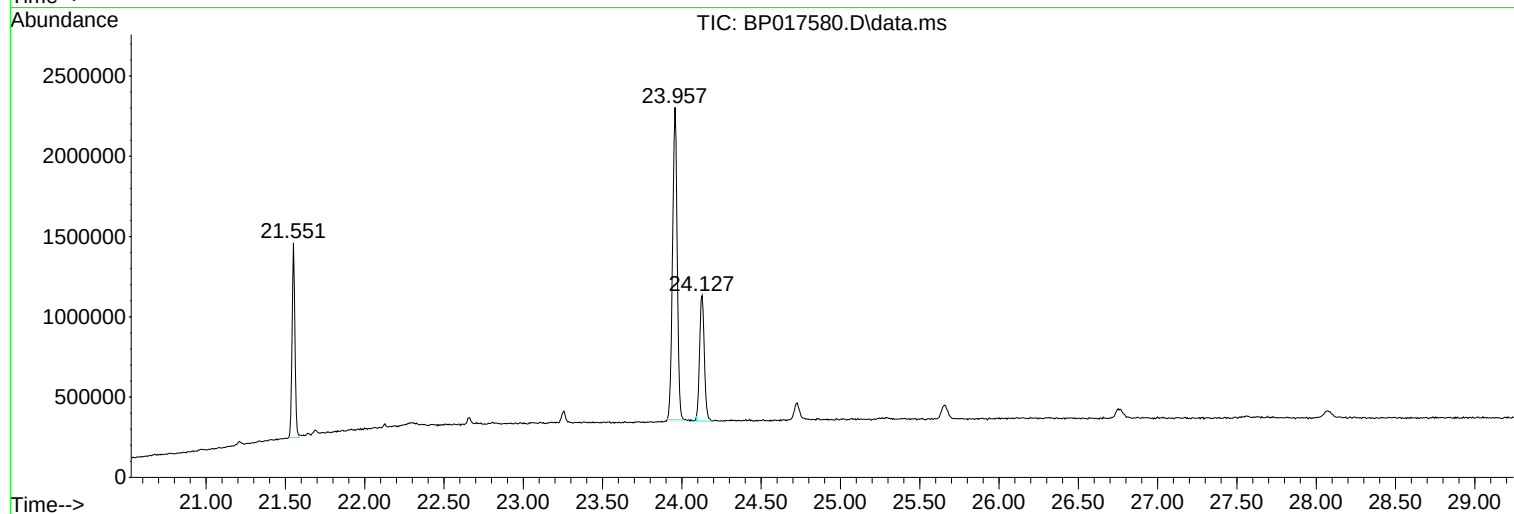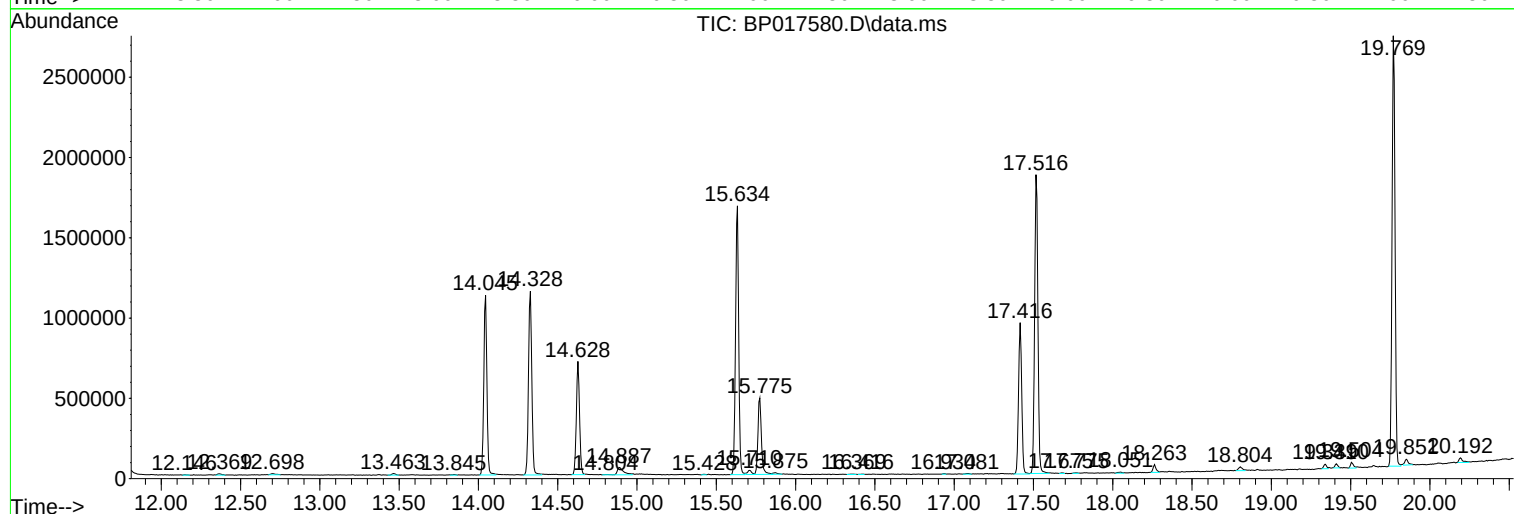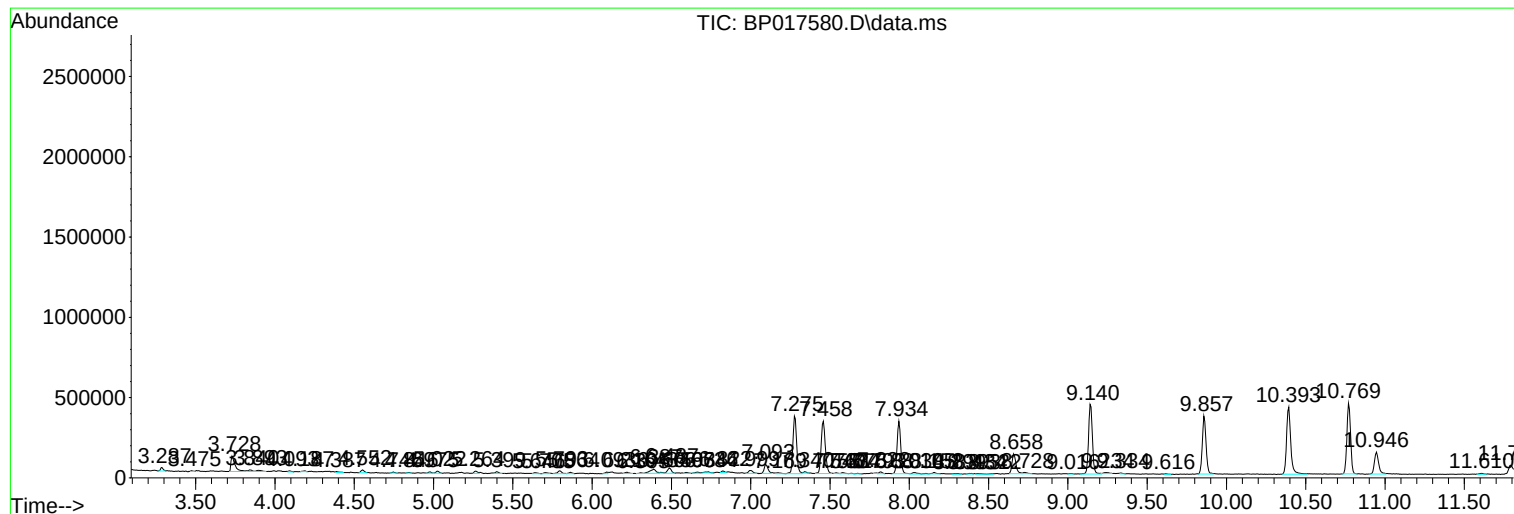

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017580.D
Acq On : 05 Oct 2023 23:21
Operator : MA/JU
Sample : 04588-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHP6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic6.387 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.387	2.73 ng/ul	70113	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentane, methyl-	84	C6H12	000096-37-7	43
2			1,4-Dioxaspiro[2.4]heptan-5-one,...	142	C7H10O3	126091-79-0	35
3			Octane, 2-methyl-	128	C9H20	003221-61-2	35
4			Tridecane, 7-methyl-	198	C14H30	026730-14-3	27
5			4-Ethylpiperidine	113	C7H15N	003230-23-7	27

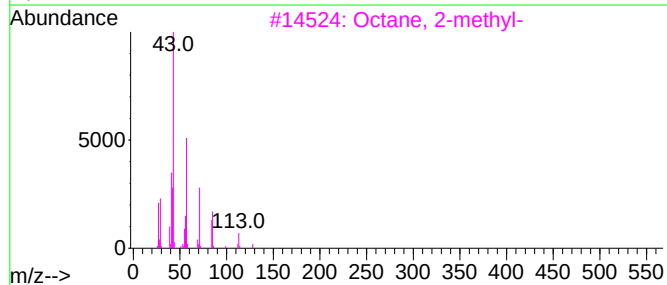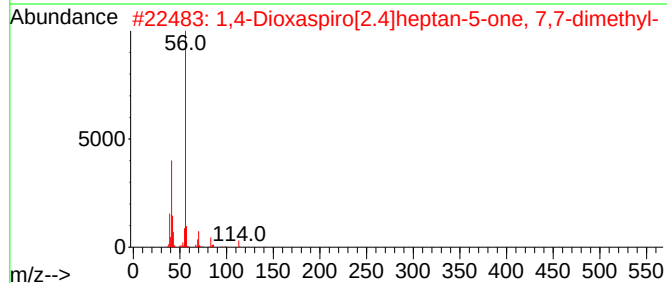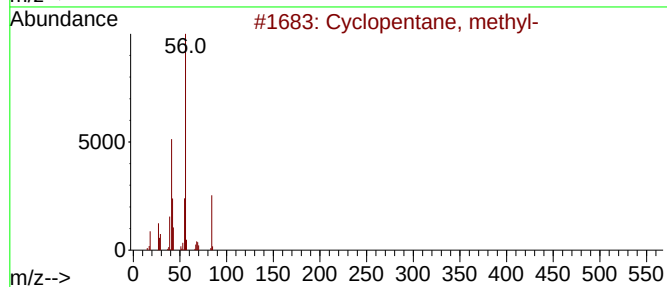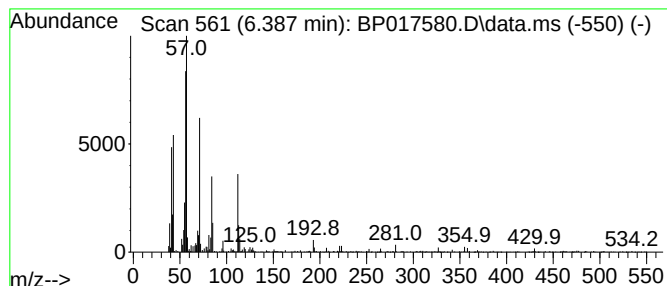

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017580.D
Acq On : 05 Oct 2023 23:21
Operator : MA/JU
Sample : 04588-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHP6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Cyclohexanone, 2,3-dimethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.487	2.16 ng/ul	55417	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexanone, 2,3-dimethyl-	126	C8H14O	013395-76-1	83
2			Cyclohexane, propyl-	126	C9H18	001678-92-8	80
3			Cyclohexane, propyl-	126	C9H18	001678-92-8	80
4			Cyclohexane, propyl-	126	C9H18	001678-92-8	80
5			Cyclohexane, 1,1'-(1,4-butanedi...	222	C16H30	006165-44-2	64

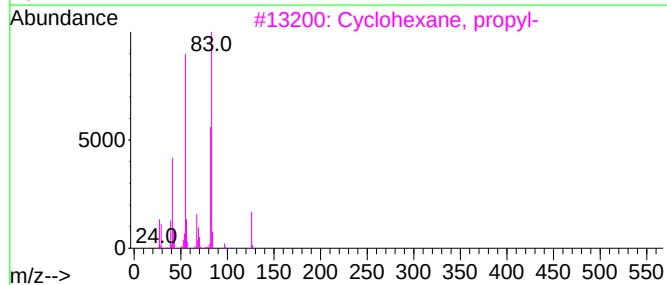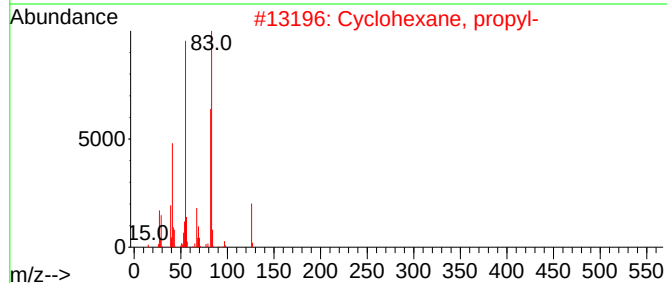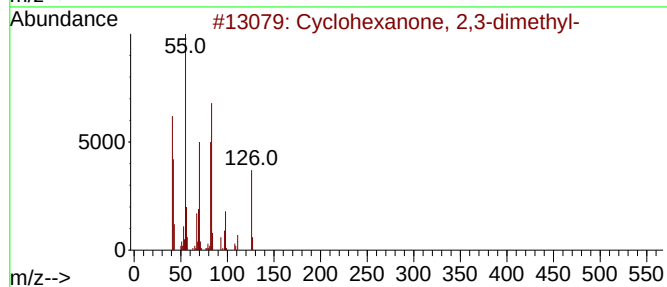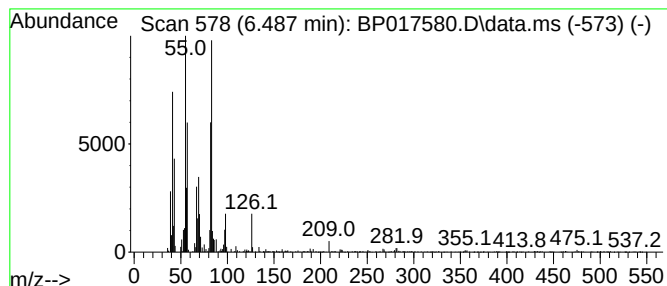

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017580.D
Acq On : 05 Oct 2023 23:21
Operator : MA/JU
Sample : 04588-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	6.387	2.7	ng/u1	70113	1	7.934	514077	20.0
Cyclohexanone, ...	6.487	2.2	ng/u1	55417	1	7.934	514077	20.0