

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017582.D
 Acq On : 06 Oct 2023 00:29
 Operator : MA/JU
 Sample : 04588-21
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	21	26	32	rBV	1642527	2164998	5.65%	3.004%
2	3.728	106	109	119	rBV	137064	221821	0.58%	0.308%
3	4.558	242	250	252	rBV	22370803	38289824	100.00%	53.129%
4	7.093	674	681	696	rVB	106122	180792	0.47%	0.251%
5	7.275	705	712	727	rBV	448503	713534	1.86%	0.990%
6	7.452	736	742	751	rBV	427868	693747	1.81%	0.963%
7	7.934	817	824	834	rBV	332793	525435	1.37%	0.729%
8	8.658	940	947	961	rBV	301592	513963	1.34%	0.713%
9	9.140	1021	1029	1042	rBV	519049	888968	2.32%	1.233%
10	9.858	1144	1151	1167	rBV	445170	734397	1.92%	1.019%
11	10.387	1234	1241	1259	rBV	593895	1047449	2.74%	1.453%
12	10.769	1299	1306	1319	rBV	446731	749307	1.96%	1.040%
13	10.940	1327	1335	1353	rBV	513678	898206	2.35%	1.246%
14	13.463	1759	1764	1772	rBV	59387	101408	0.26%	0.141%
15	14.046	1856	1863	1874	rBV	1288739	1806540	4.72%	2.507%
16	14.322	1903	1910	1923	rBV	1371130	2062111	5.39%	2.861%
17	14.628	1953	1962	1975	rBV	698028	1022972	2.67%	1.419%
18	14.887	1999	2006	2020	rBV2	55727	145014	0.38%	0.201%
19	15.628	2125	2132	2142	rBV	1906143	2734214	7.14%	3.794%
20	15.769	2150	2156	2169	rBV	518989	740301	1.93%	1.027%
21	17.416	2429	2436	2446	rBV	902911	1294603	3.38%	1.796%
22	17.516	2446	2453	2467	rVV	2263271	3097248	8.09%	4.298%
23	18.263	2575	2580	2587	rBV3	46474	69380	0.18%	0.096%
24	19.504	2788	2791	2796	rBV4	31564	43060	0.11%	0.060%
25	19.769	2830	2836	2845	rBV	3060965	3946185	10.31%	5.475%
26	21.551	3134	3139	3147	rBV	1190345	1560020	4.07%	2.165%
27	23.957	3540	3548	3558	rVB2	1981552	4139805	10.81%	5.744%
28	24.121	3570	3576	3589	rVB	779242	1684817	4.40%	2.338%




Sum of corrected areas: 72070119

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017582.D
Acq On : 06 Oct 2023 00:29
Operator : MA/JU
Sample : 04588-21
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

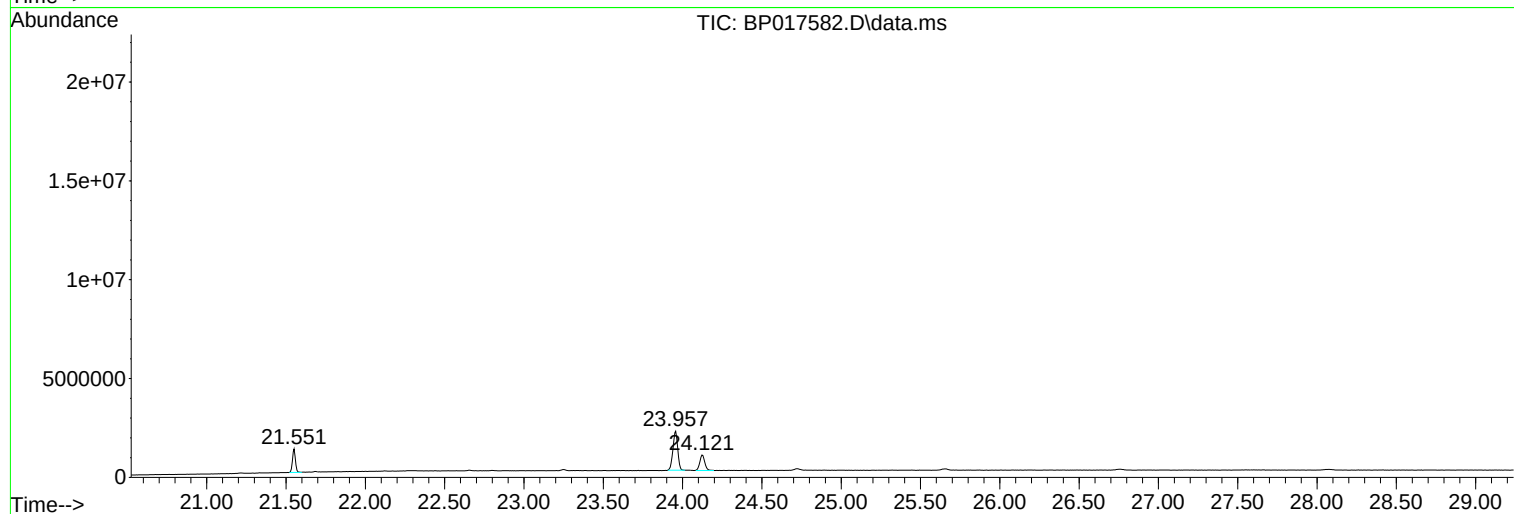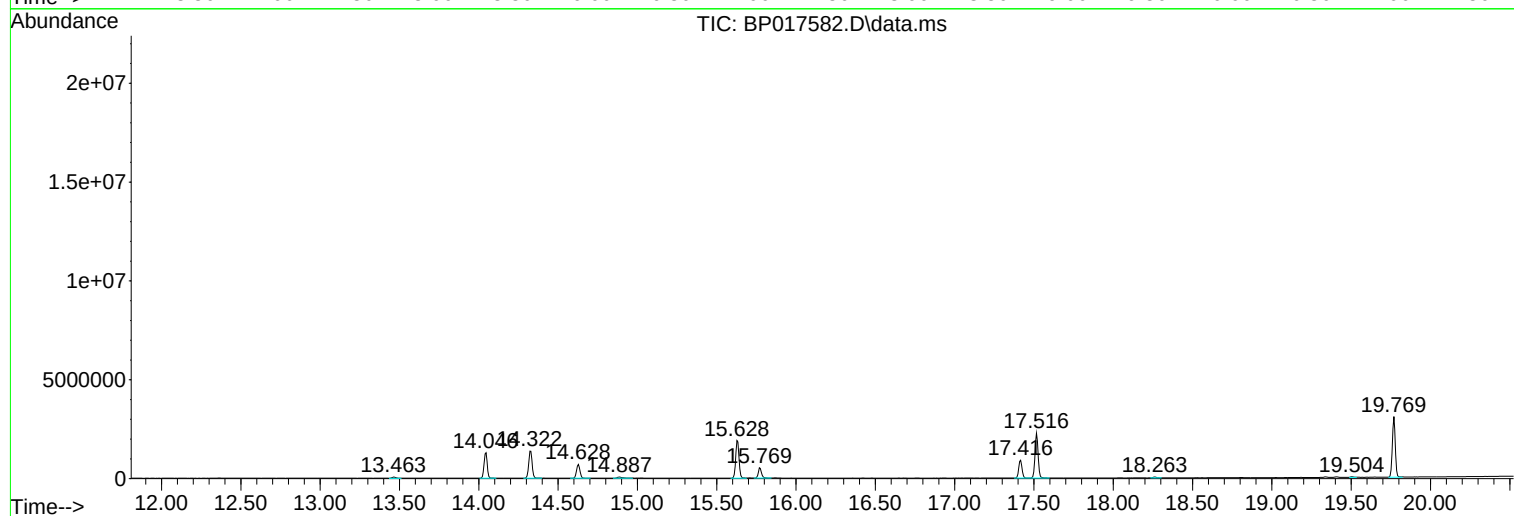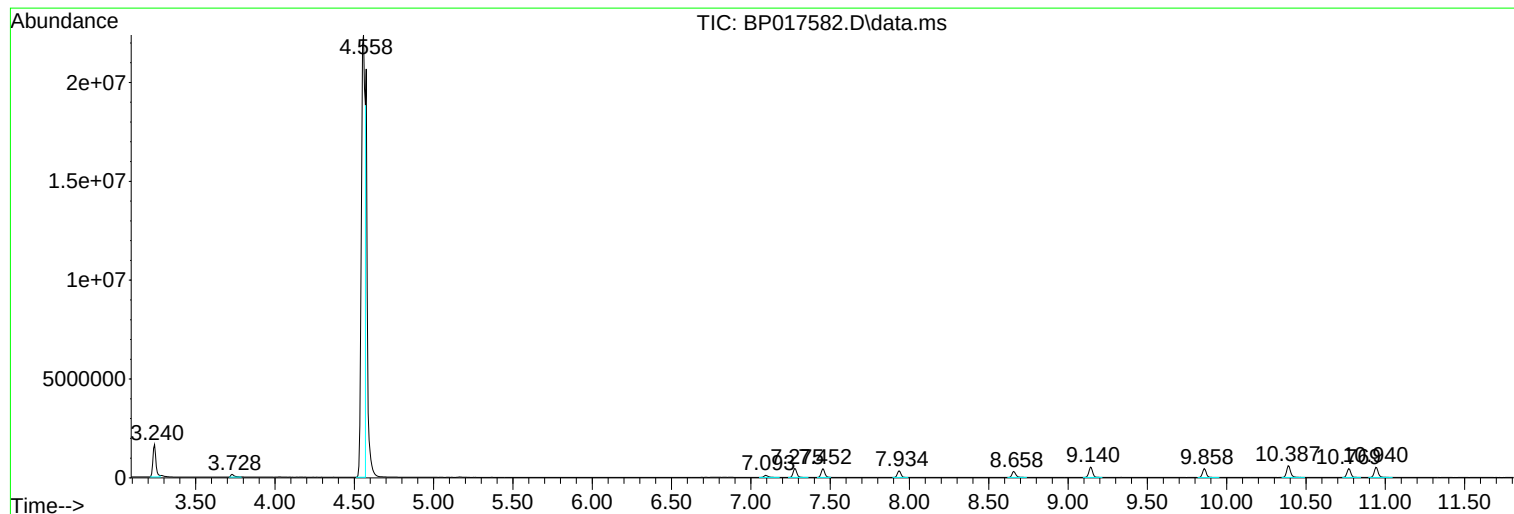

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017582.D
Acq On : 06 Oct 2023 00:29
Operator : MA/JU
Sample : 04588-21
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHQ0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.558	1457.45 ng/ul	38289800	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			2,4-Dichloro-6-fluoropyrimidine	166	C4HC12FN2	003833-57-6	38

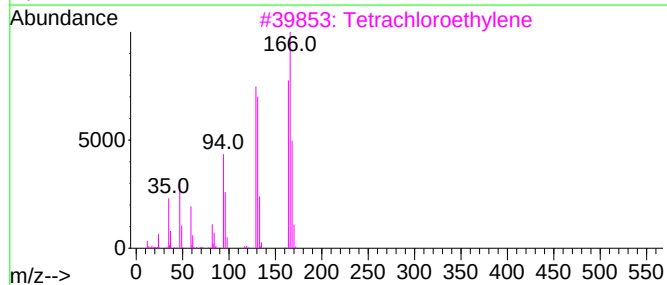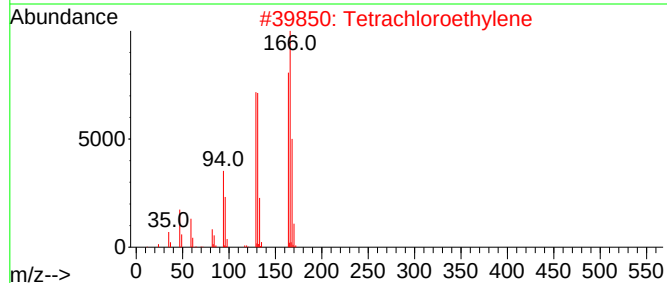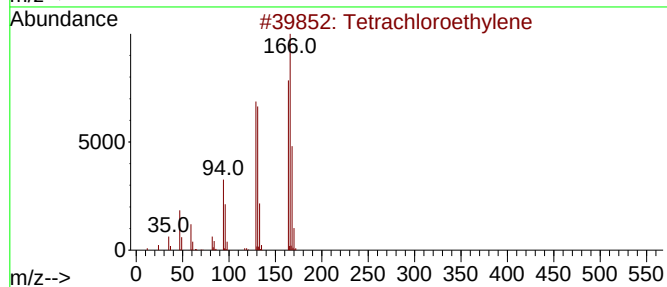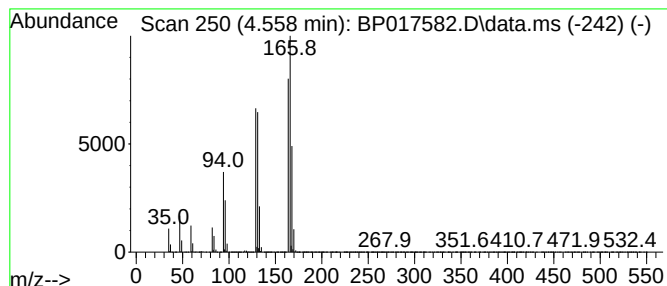

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017582.D
Acq On : 06 Oct 2023 00:29
Operator : MA/JU
Sample : 04588-21
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.558	1457.5	ng/ul	38289800	1	7.934	525435	20.0