

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017587.D
 Acq On : 06 Oct 2023 04:27
 Operator : MA/JU
 Sample : PB155912BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK912

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	43	rVB	45114	63790	1.36%	0.158%
2	3.722	104	108	125	rBV	538113	850357	18.17%	2.109%
3	4.028	157	160	164	rVB2	7171	10126	0.22%	0.025%
4	6.840	636	638	641	rBV4	2893	4826	0.10%	0.012%
5	7.087	674	680	695	rBV	670012	1108231	23.68%	2.749%
6	7.275	706	712	723	rBV	541196	834212	17.83%	2.069%
7	7.452	735	742	753	rBV	703976	1114080	23.81%	2.764%
8	7.934	815	824	831	rBV	400952	631980	13.50%	1.568%
9	8.652	939	946	961	rBV	809555	1356445	28.99%	3.365%
10	9.140	1022	1029	1041	rBV	649731	1056162	22.57%	2.620%
11	9.857	1143	1151	1160	rBV	570290	913451	19.52%	2.266%
12	10.387	1232	1241	1259	rBV	779669	1386702	29.63%	3.440%
13	10.769	1298	1306	1315	rVB	546106	882020	18.85%	2.188%
14	10.940	1327	1335	1354	rBV	836564	1423337	30.42%	3.531%
15	12.363	1573	1577	1587	rVB4	12820	29446	0.63%	0.073%
16	13.463	1757	1764	1773	rBV9	7395	14024	0.30%	0.035%
17	14.040	1855	1862	1872	rBV	1574053	2119504	45.29%	5.258%
18	14.322	1903	1910	1923	rBV	1665573	2404207	51.38%	5.964%
19	14.628	1955	1962	1975	rBV	814967	1198209	25.60%	2.972%
20	14.869	1996	2003	2021	rBV	523875	1042996	22.29%	2.587%
21	15.628	2125	2132	2144	rBV	2275018	3124179	66.76%	7.750%
22	15.769	2149	2156	2169	rVV	630121	861361	18.41%	2.137%
23	15.869	2169	2173	2178	rVB5	11339	17885	0.38%	0.044%
24	17.081	2374	2379	2384	rBV9	5235	9695	0.21%	0.024%
25	17.198	2395	2399	2402	rBV6	3786	5715	0.12%	0.014%
26	17.416	2429	2436	2446	rBV	1096313	1511555	32.30%	3.750%
27	17.516	2447	2453	2468	rVV	2700539	3591949	76.76%	8.911%
28	18.686	2650	2652	2655	rBV3	4333	5308	0.11%	0.013%
29	19.339	2759	2763	2768	rVB2	28213	38378	0.82%	0.095%
30	19.410	2771	2775	2780	rVB3	25995	36746	0.79%	0.091%
31	19.769	2830	2836	2845	rBV	3503824	4373568	93.46%	10.850%
32	21.551	3134	3139	3145	rBV	1345989	1757953	37.57%	4.361%
33	23.957	3540	3548	3559	rVB2	2311465	4679718	100.00%	11.609%
34	24.127	3570	3577	3590	rVB	895202	1852861	39.59%	4.596%

Sum of corrected areas: 40310976




Instrument :
BNA_P
ClientSampleId :
SBLK912

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017587.D
Acq On : 06 Oct 2023 04:27
Operator : MA/JU
Sample : PB155912BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

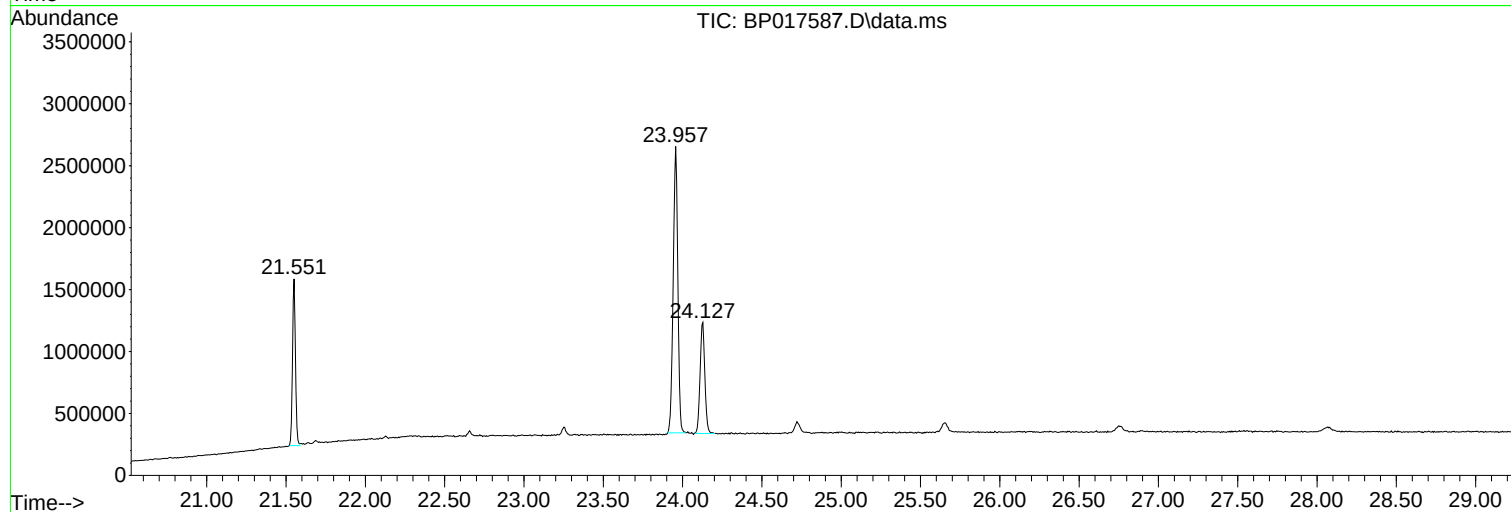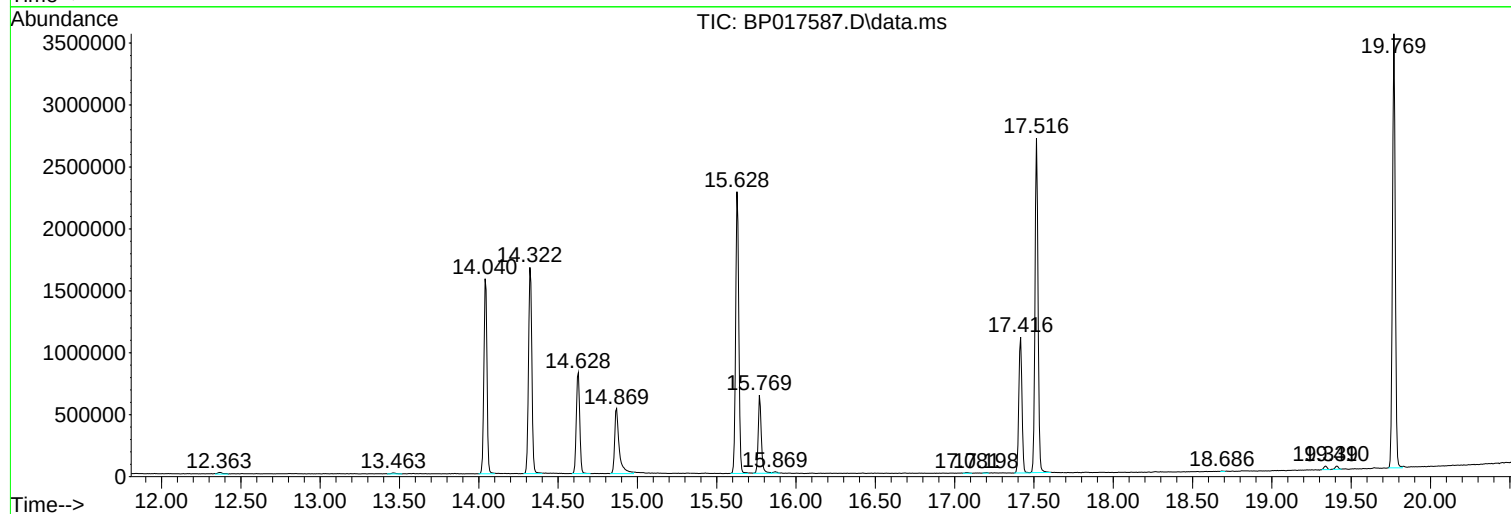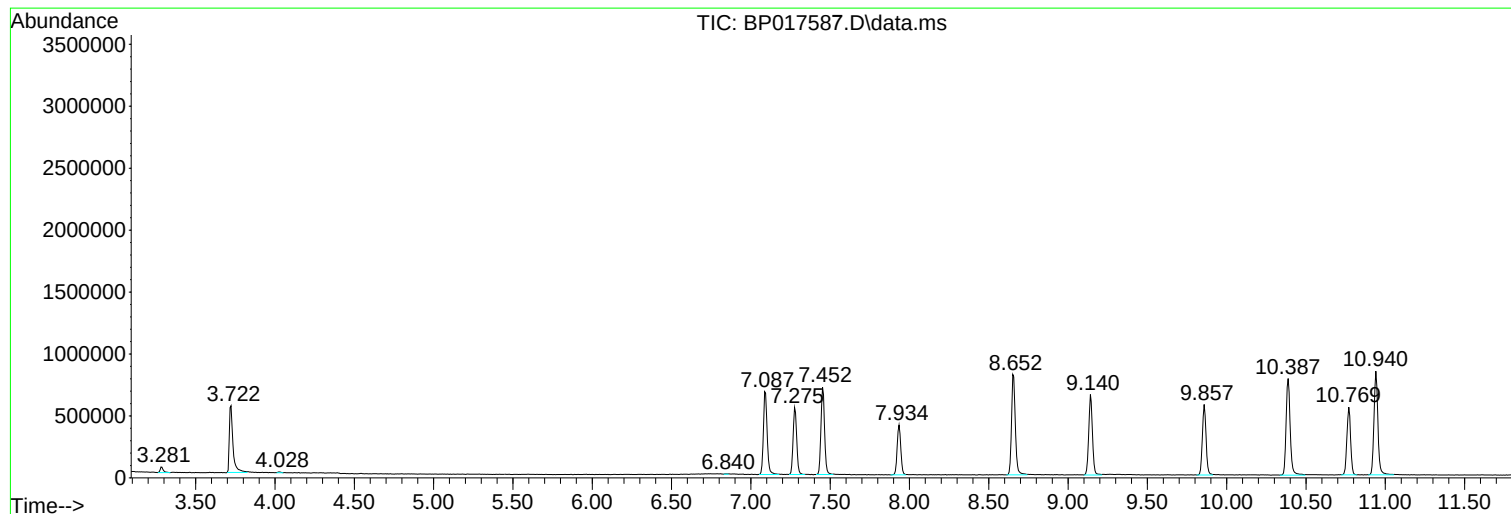

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017587.D
Acq On : 06 Oct 2023 04:27
Operator : MA/JU
Sample : PB155912BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017587.D
Acq On : 06 Oct 2023 04:27
Operator : MA/JU
Sample : PB155912BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc