

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017588.D
 Acq On : 06 Oct 2023 05:01
 Operator : MA/JU
 Sample : PB155932BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK932

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	42	rVB	37131	49449	1.43%	0.160%
2	3.722	105	108	123	rBV	417633	642732	18.58%	2.077%
3	4.028	156	160	163	rBV4	6381	7903	0.23%	0.026%
4	6.722	611	618	620	rBV8	2961	7116	0.21%	0.023%
5	7.093	674	681	695	rBV	493232	830532	24.01%	2.683%
6	7.275	706	712	726	rVB	407542	635997	18.39%	2.055%
7	7.451	735	742	754	rBV	524514	841484	24.33%	2.719%
8	7.934	816	824	836	rBV	350007	563671	16.30%	1.821%
9	8.657	937	947	962	rBV	581648	1009643	29.19%	3.262%
10	9.140	1020	1029	1037	rBV	479988	787815	22.78%	2.545%
11	9.751	1130	1133	1137	rVB5	3071	3873	0.11%	0.013%
12	9.857	1143	1151	1160	rBV	417792	679858	19.66%	2.197%
13	10.387	1233	1241	1257	rBV	597626	1053909	30.47%	3.405%
14	10.769	1299	1306	1317	rBV	468670	777616	22.48%	2.512%
15	10.940	1322	1335	1350	rBV	602632	1070687	30.96%	3.459%
16	11.834	1482	1487	1492	rVB8	2896	4944	0.14%	0.016%
17	12.363	1570	1577	1583	rVV5	8646	16832	0.49%	0.054%
18	13.457	1760	1763	1770	rBV7	5514	10497	0.30%	0.034%
19	13.575	1779	1783	1791	rBV10	4055	9019	0.26%	0.029%
20	13.728	1805	1809	1810	rBV4	2936	3594	0.10%	0.012%
21	14.039	1855	1862	1872	rBV	1123372	1570516	45.41%	5.074%
22	14.322	1904	1910	1926	rBV	1212416	1787927	51.70%	5.777%
23	14.628	1953	1962	1969	rBV	721401	1046899	30.27%	3.383%
24	14.869	1997	2003	2022	rBV	370638	745219	21.55%	2.408%
25	15.028	2028	2030	2034	rVB5	4858	6121	0.18%	0.020%
26	15.627	2126	2132	2140	rBV	1585601	2269281	65.61%	7.332%
27	15.769	2150	2156	2168	rBV	403761	587429	16.98%	1.898%
28	15.869	2170	2173	2179	rVB5	8126	13432	0.39%	0.043%
29	17.074	2376	2378	2385	rVB8	3459	5146	0.15%	0.017%
30	17.192	2397	2398	2404	rVB6	2861	3552	0.10%	0.011%
31	17.416	2429	2436	2446	rBV	942693	1321887	38.22%	4.271%
32	17.516	2446	2453	2465	rBV	1919902	2623002	75.84%	8.475%
33	18.045	2541	2543	2546	rVB4	3316	3985	0.12%	0.013%
34	18.274	2575	2582	2586	rBV10	5972	11672	0.34%	0.038%
35	18.939	2693	2695	2698	rBV4	3928	4853	0.14%	0.016%
36	19.339	2759	2763	2767	rBV2	25369	34462	1.00%	0.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017588.D
Acq On : 06 Oct 2023 05:01
Operator : MA/JU
Sample : PB155932BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK932

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION

37	19.410	2772	2775	2780	rVV3	19530	25655	0.74%	0.083%
38	19.768	2830	2836	2845	rBV	2535943	3201357	92.56%	10.344%
39	21.551	3134	3139	3145	rBV	1224753	1568165	45.34%	5.067%
40	23.956	3540	3548	3558	rVB2	1650533	3458518	100.00%	11.174%
41	24.121	3570	3576	3587	rVB	790427	1653991	47.82%	5.344%




Sum of corrected areas: 30950240

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017588.D
Acq On : 06 Oct 2023 05:01
Operator : MA/JU
Sample : PB155932BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK932

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

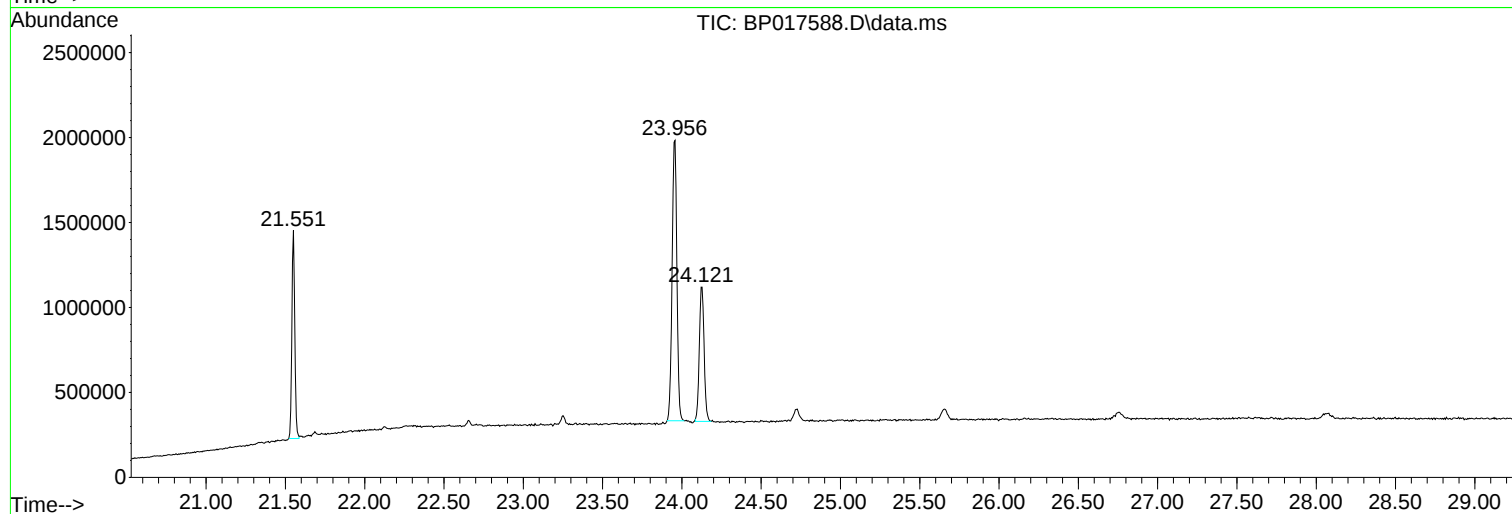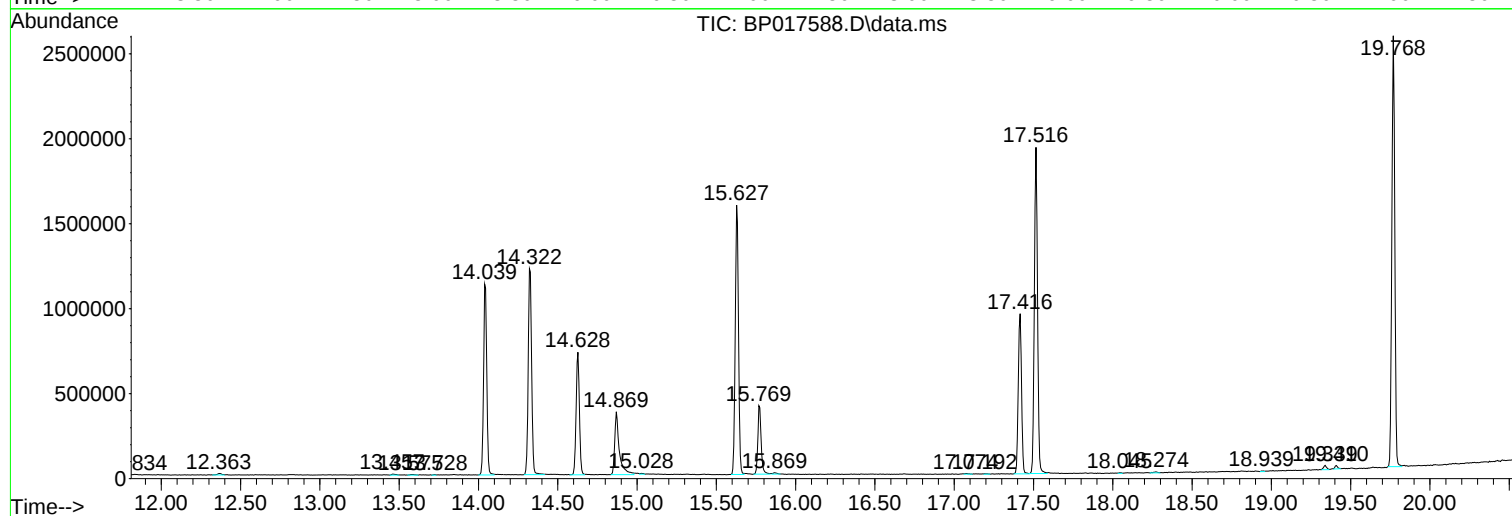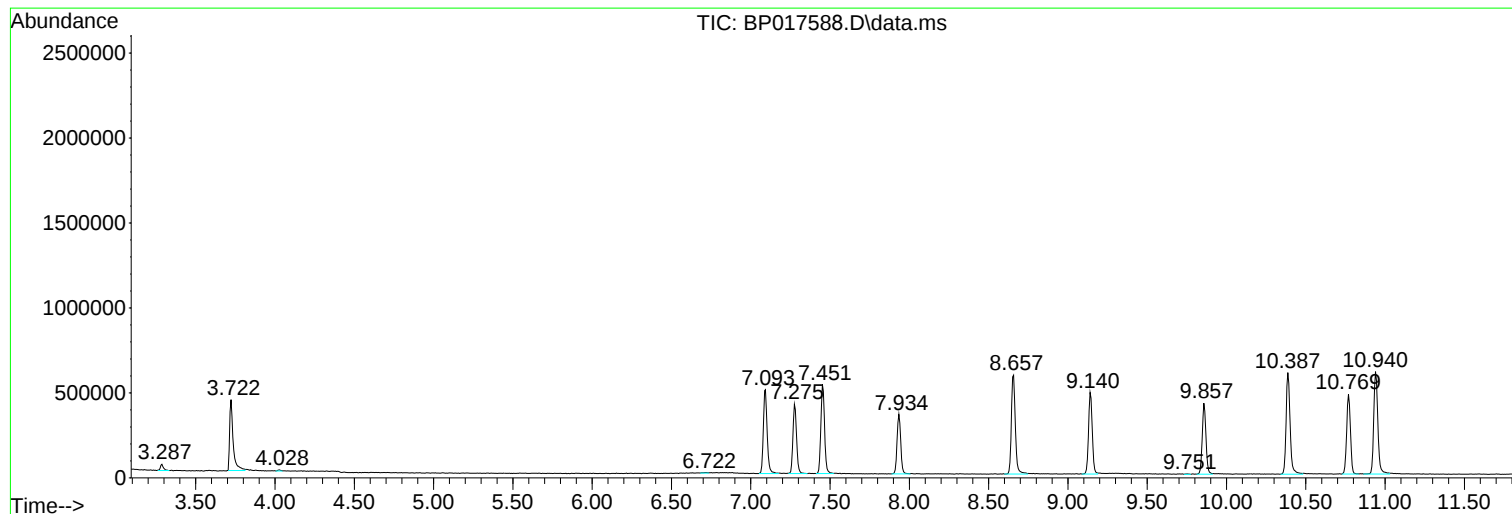

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017588.D
Acq On : 06 Oct 2023 05:01
Operator : MA/JU
Sample : PB155932BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK932

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017588.D
Acq On : 06 Oct 2023 05:01
Operator : MA/JU
Sample : PB155932BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK932

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------