

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017589.D
 Acq On : 06 Oct 2023 05:35
 Operator : MA/JU
 Sample : PB155937BL
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK937

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	39	rVB	33318	40699	1.17%	0.132%
2	3.722	104	108	130	rBV	432619	686490	19.70%	2.226%
3	4.028	157	160	163	rBV4	5258	6207	0.18%	0.020%
4	6.493	574	579	580	rBV5	2173	3864	0.11%	0.013%
5	6.887	644	646	654	rVB8	3227	5824	0.17%	0.019%
6	7.087	670	680	692	rBV	506519	848329	24.34%	2.751%
7	7.275	705	712	723	rBV	416083	644279	18.48%	2.090%
8	7.452	734	742	756	rBV	545758	859790	24.67%	2.789%
9	7.934	817	824	835	rBV	343140	549303	15.76%	1.782%
10	8.652	940	946	958	rBV	612073	1028715	29.51%	3.336%
11	9.140	1021	1029	1041	rBV	489768	809528	23.23%	2.626%
12	9.857	1144	1151	1164	rBV	418191	693314	19.89%	2.249%
13	10.387	1234	1241	1259	rBV	603189	1063091	30.50%	3.448%
14	10.769	1297	1306	1313	rBV	469244	764312	21.93%	2.479%
15	10.940	1326	1335	1352	rBV	617475	1075865	30.87%	3.489%
16	11.804	1474	1482	1485	rBV9	2715	7166	0.21%	0.023%
17	11.840	1485	1488	1494	rVV8	3999	8304	0.24%	0.027%
18	11.916	1498	1501	1508	rVB9	1656	3768	0.11%	0.012%
19	12.363	1572	1577	1582	rBV6	8694	16510	0.47%	0.054%
20	13.463	1761	1764	1772	rVB10	5053	8384	0.24%	0.027%
21	13.851	1822	1830	1832	rBV9	3475	5381	0.15%	0.017%
22	14.040	1856	1862	1872	rBV	1107573	1554981	44.61%	5.043%
23	14.322	1904	1910	1924	rBV	1215816	1790570	51.37%	5.807%
24	14.628	1955	1962	1971	rBV	682870	1011769	29.03%	3.281%
25	14.869	1997	2003	2021	rBV	353141	726794	20.85%	2.357%
26	15.145	2048	2050	2056	rBV7	2110	3647	0.10%	0.012%
27	15.263	2064	2070	2073	rBV8	2181	4497	0.13%	0.015%
28	15.628	2125	2132	2145	rBV	1598541	2312695	66.35%	7.501%
29	15.775	2150	2157	2170	rVV	399597	593446	17.03%	1.925%
30	15.875	2170	2174	2179	rVB8	8780	16163	0.46%	0.052%
31	16.422	2263	2267	2271	rBV6	4290	7465	0.21%	0.024%
32	17.075	2373	2378	2381	rBV7	2877	4935	0.14%	0.016%
33	17.204	2395	2400	2403	rBV7	2616	4775	0.14%	0.015%
34	17.416	2429	2436	2443	rBV	918633	1257487	36.08%	4.078%
35	17.516	2447	2453	2466	rVV	1877114	2574952	73.88%	8.351%
36	18.398	2601	2603	2609	rVB5	3722	4453	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017589.D
Acq On : 06 Oct 2023 05:35
Operator : MA/JU
Sample : PB155937BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK937

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION

37	19.339	2759	2763	2768	rVB2	23145	27755	0.80%	0.090%
38	19.410	2772	2775	2780	rVV2	19340	24590	0.71%	0.080%
39	19.769	2830	2836	2845	rBV	2469079	3173969	91.06%	10.294%
40	21.551	3134	3139	3145	rBV	1165314	1489620	42.74%	4.831%
41	23.951	3540	3547	3560	rVB2	1667402	3485434	100.00%	11.304%
42	24.127	3570	3577	3589	rVB	766696	1633667	46.87%	5.298%




Sum of corrected areas: 30832787

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017589.D
Acq On : 06 Oct 2023 05:35
Operator : MA/JU
Sample : PB155937BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK937

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

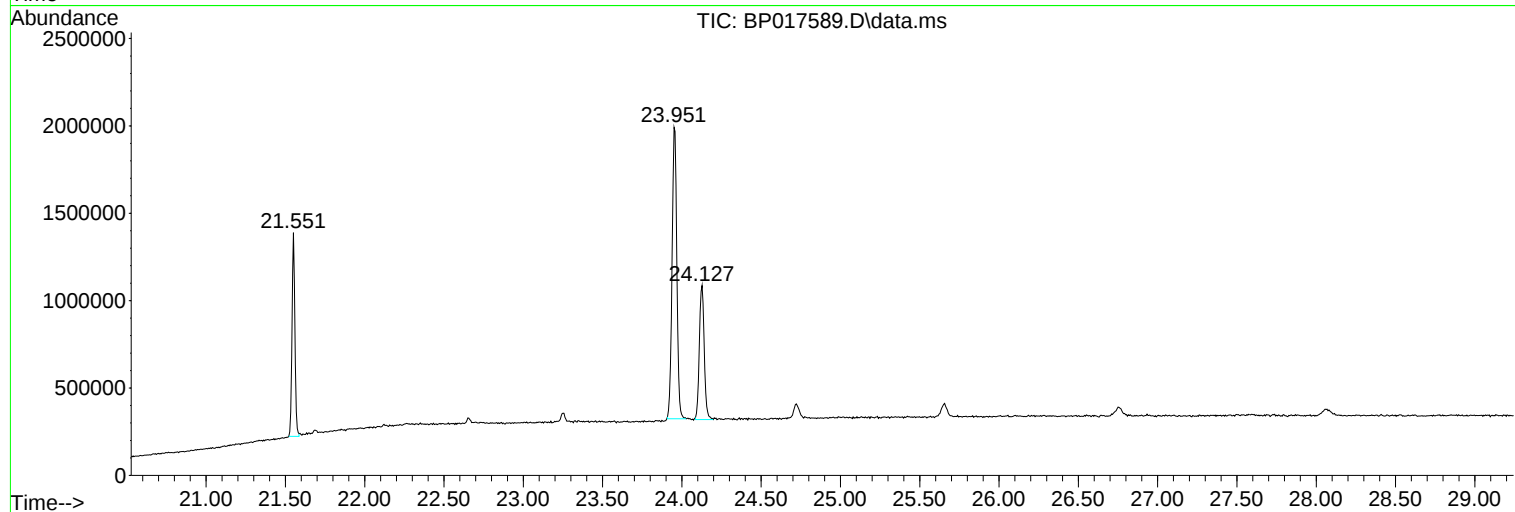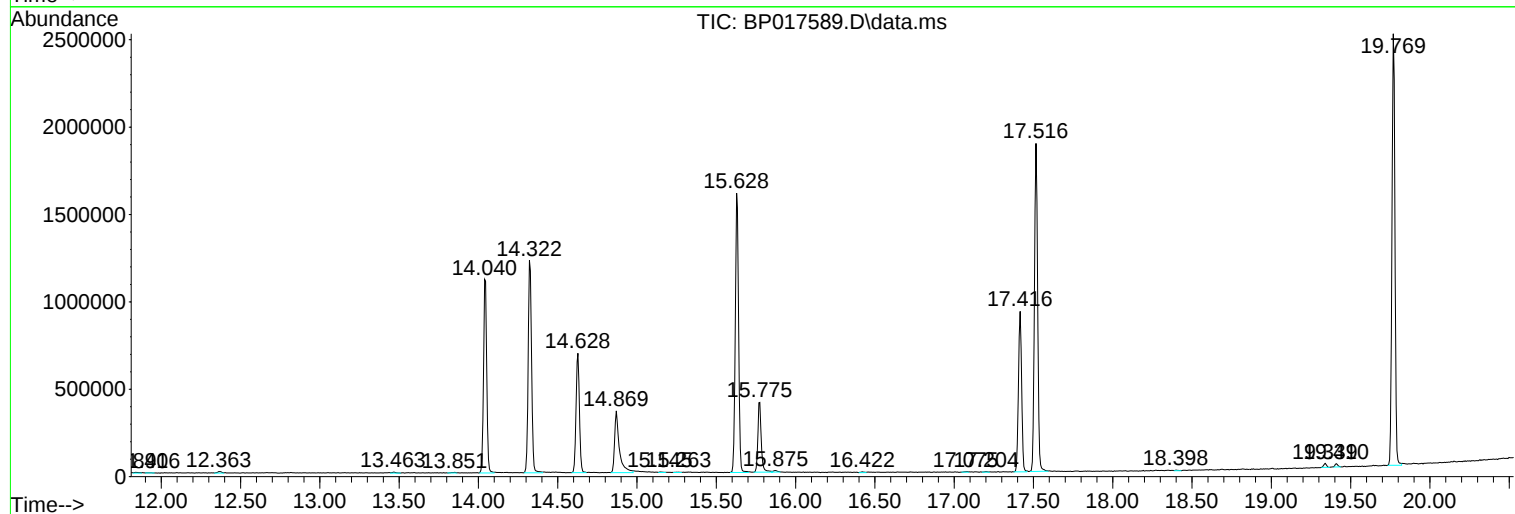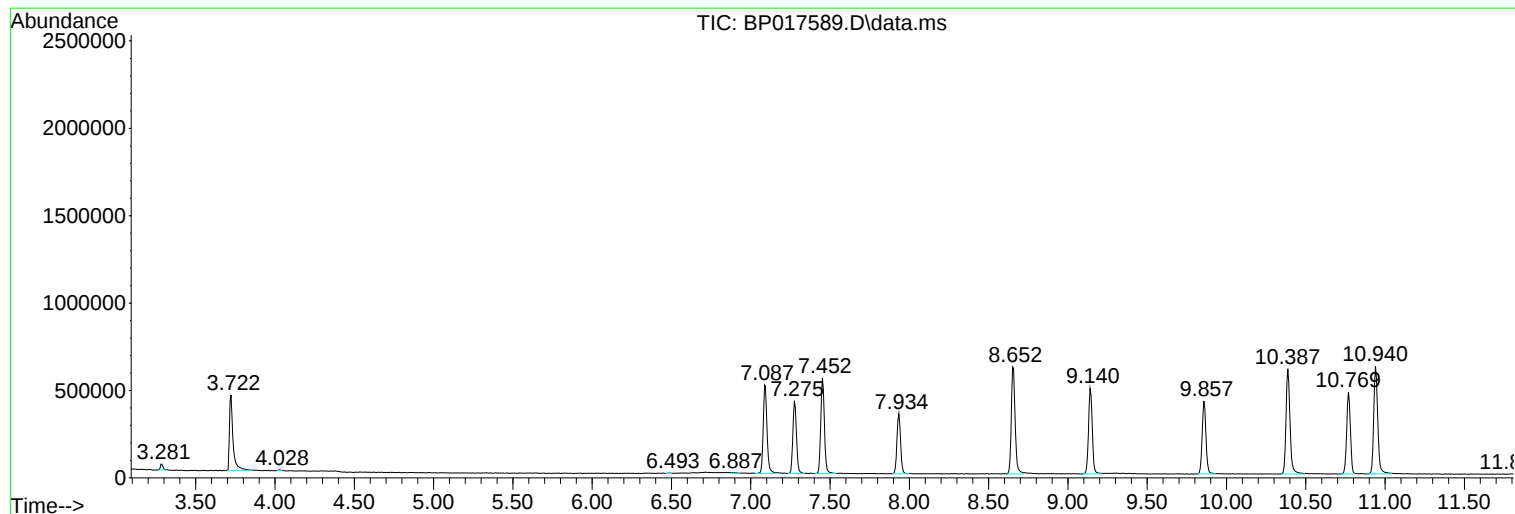

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017589.D
Acq On : 06 Oct 2023 05:35
Operator : MA/JU
Sample : PB155937BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK937

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017589.D
Acq On : 06 Oct 2023 05:35
Operator : MA/JU
Sample : PB155937BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK937

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc