

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017601.D
 Acq On : 06 Oct 2023 14:47
 Operator : MA/JU
 Sample : PB156032BL
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK032

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	39	rVB	34273	45034	1.27%	0.145%
2	3.722	104	108	125	rBV	411476	653134	18.48%	2.103%
3	4.022	156	159	166	rVB4	9438	15344	0.43%	0.049%
4	5.928	479	483	488	rVB8	2738	3863	0.11%	0.012%
5	7.087	673	680	694	rBV	493076	805084	22.78%	2.593%
6	7.275	705	712	724	rBV	393748	609403	17.24%	1.962%
7	7.452	735	742	752	rBV	516408	813714	23.03%	2.620%
8	7.934	817	824	835	rVV	361360	574451	16.26%	1.850%
9	8.652	938	946	962	rBV	597537	1001223	28.33%	3.224%
10	9.140	1022	1029	1038	rBV	452806	758267	21.46%	2.442%
11	9.857	1141	1151	1162	rBV	400928	660257	18.68%	2.126%
12	10.387	1232	1241	1259	rBV	572923	1018578	28.82%	3.280%
13	10.504	1259	1261	1267	rVB7	2793	4007	0.11%	0.013%
14	10.769	1299	1306	1313	rBV	484482	796028	22.53%	2.563%
15	10.940	1326	1335	1350	rBV	586409	1048593	29.67%	3.377%
16	11.057	1353	1355	1361	rVV7	4451	7889	0.22%	0.025%
17	11.816	1481	1484	1485	rBV3	3552	3938	0.11%	0.013%
18	12.369	1572	1578	1584	rBV7	7766	13664	0.39%	0.044%
19	12.745	1637	1642	1644	rBV6	2696	4120	0.12%	0.013%
20	13.463	1759	1764	1771	rVB4	8787	14659	0.41%	0.047%
21	13.845	1824	1829	1832	rVB7	3164	5854	0.17%	0.019%
22	14.040	1856	1862	1871	rBV	1080467	1508768	42.69%	4.859%
23	14.322	1904	1910	1923	rBV	1205718	1738445	49.19%	5.598%
24	14.628	1955	1962	1969	rBV	741754	1096374	31.03%	3.531%
25	14.869	1997	2003	2025	rBV	328651	725823	20.54%	2.337%
26	15.416	2092	2096	2101	rBV8	2878	5161	0.15%	0.017%
27	15.628	2125	2132	2144	rBV	1606359	2277130	64.44%	7.333%
28	15.769	2150	2156	2167	rBV	393256	584152	16.53%	1.881%
29	15.869	2170	2173	2177	rVB4	7853	11381	0.32%	0.037%
30	16.139	2217	2219	2224	rBV5	2240	3744	0.11%	0.012%
31	16.686	2309	2312	2318	rVB8	2440	4247	0.12%	0.014%
32	17.075	2376	2378	2383	rVB6	3017	4711	0.13%	0.015%
33	17.416	2429	2436	2447	rBV	971505	1381690	39.10%	4.449%
34	17.516	2447	2453	2468	rVV	1811117	2555223	72.31%	8.229%
35	17.769	2493	2496	2498	rBV3	3321	3932	0.11%	0.013%
36	19.339	2759	2763	2768	rBV3	23260	28997	0.82%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017601.D
Acq On : 06 Oct 2023 14:47
Operator : MA/JU
Sample : PB156032BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK032

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION

37	19.410	2772	2775	2778	rVB3	18920	21730	0.61%	0.070%
38	19.769	2831	2836	2844	rBV	2375375	3157537	89.35%	10.168%
39	21.551	3134	3139	3148	rBV	1256568	1656071	46.86%	5.333%
40	23.251	3425	3428	3436	rVB2	122552	190420	5.39%	0.613%
41	23.957	3540	3548	3559	rVB2	1604127	3533837	100.00%	11.380%
42	24.127	3571	3577	3589	rVB	814533	1706299	48.28%	5.495%




Sum of corrected areas: 31052776

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017601.D
Acq On : 06 Oct 2023 14:47
Operator : MA/JU
Sample : PB156032BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK032

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

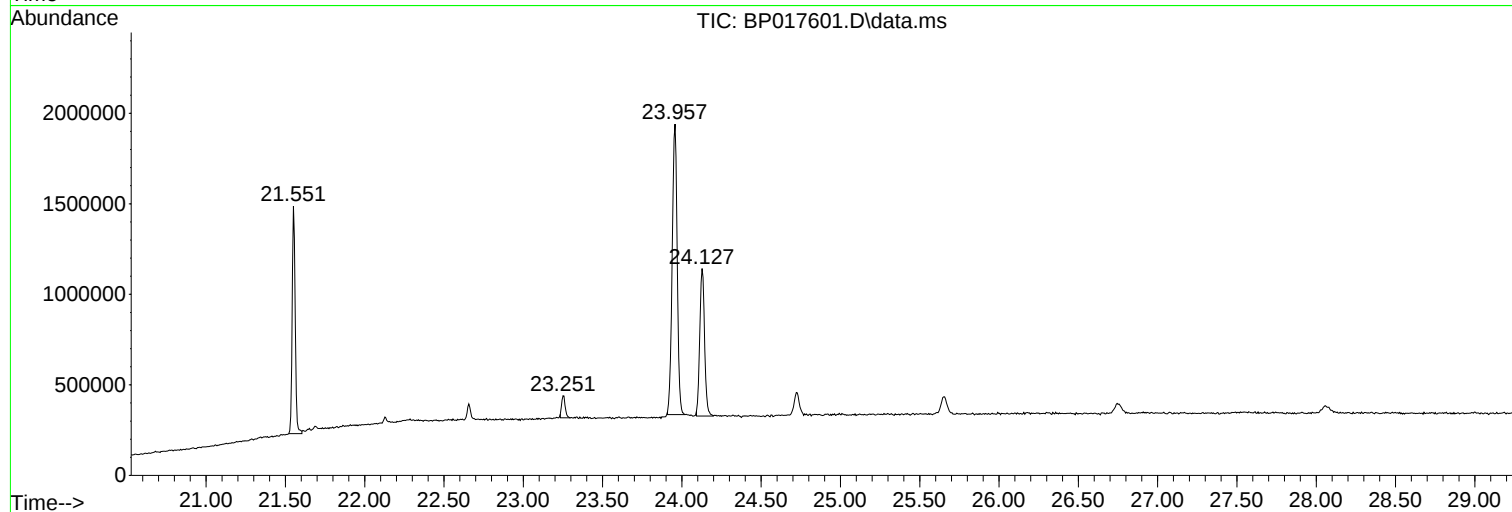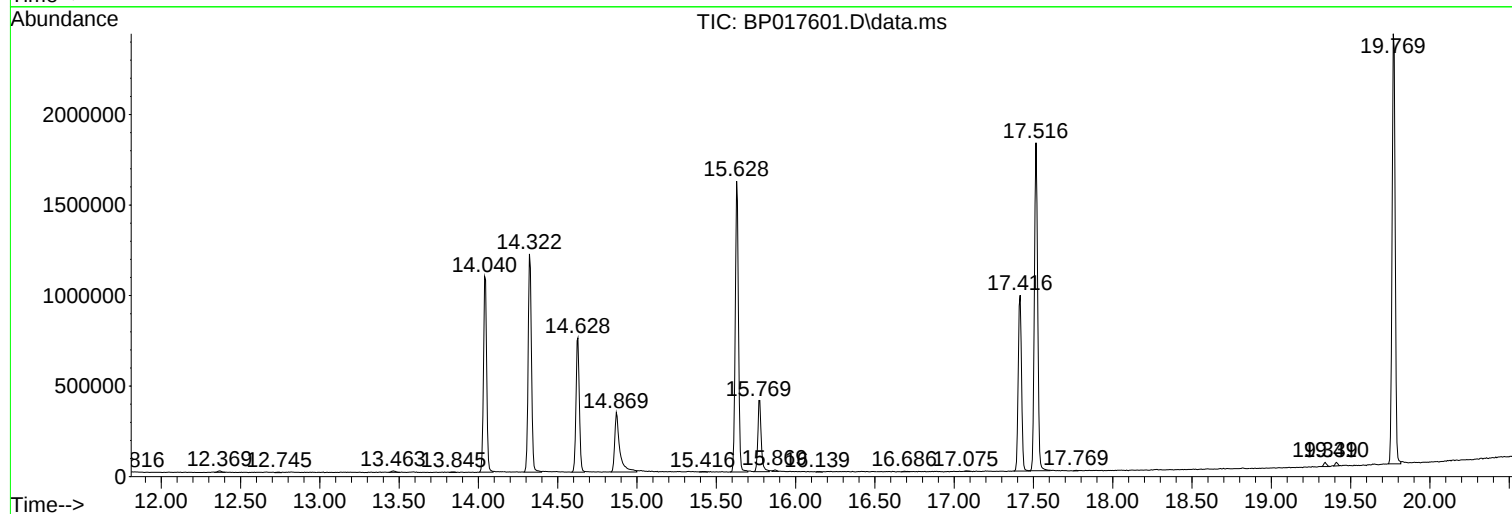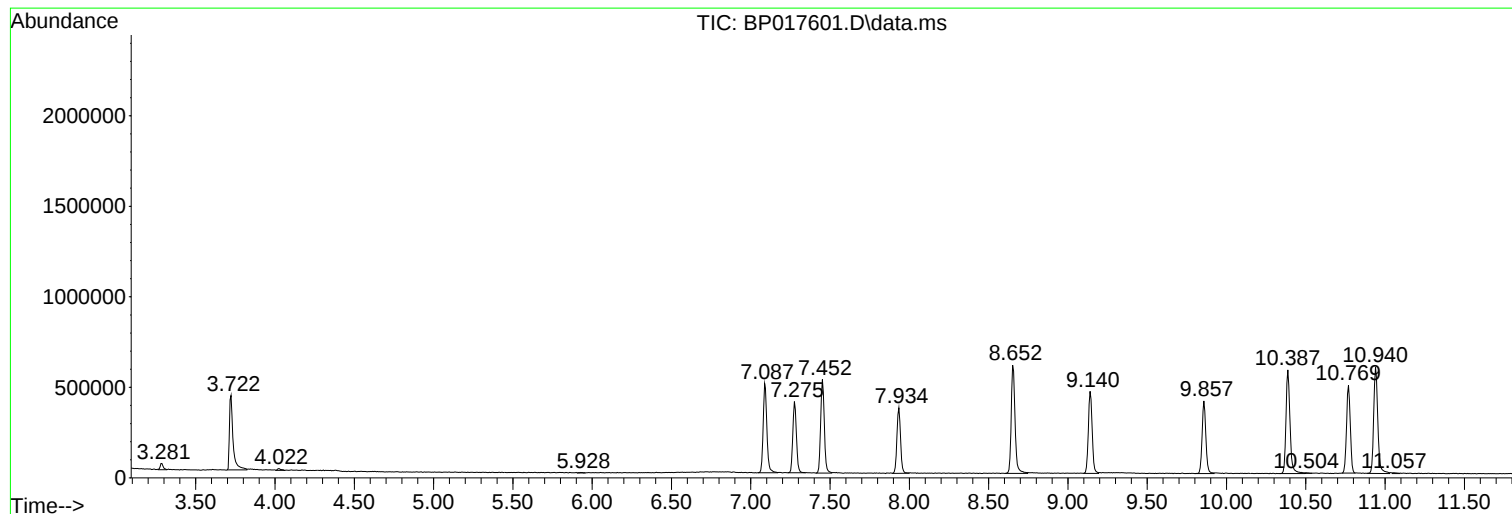

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017601.D
Acq On : 06 Oct 2023 14:47
Operator : MA/JU
Sample : PB156032BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK032










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.251	2.23 ng/ul	190420	Perylene-d12	24.127

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Nonadecane	268	C19H40	000629-92-5	94
2			Nonadecane	268	C19H40	000629-92-5	91
3			Docosane, 11-butyl-	366	C26H54	013475-76-8	91
4			Heneicosane, 11-pentyl-	366	C26H54	014739-72-1	91
5			Heneicosane	296	C21H44	000629-94-7	87

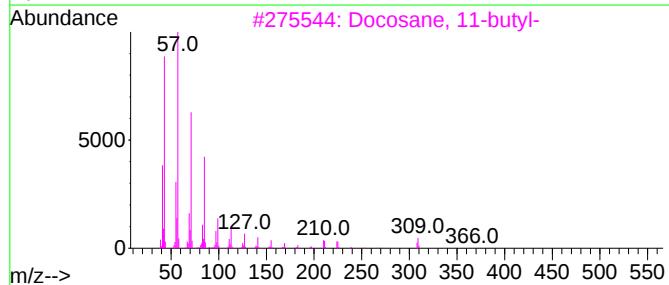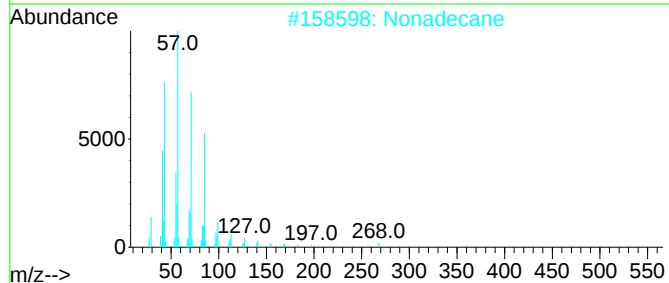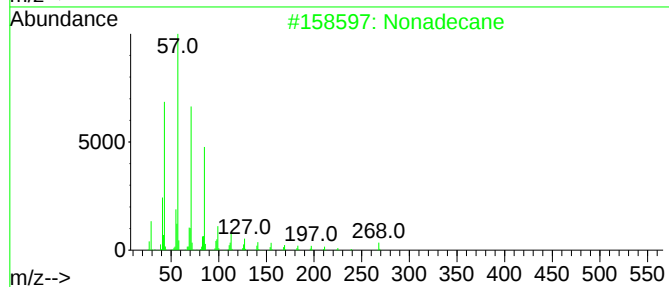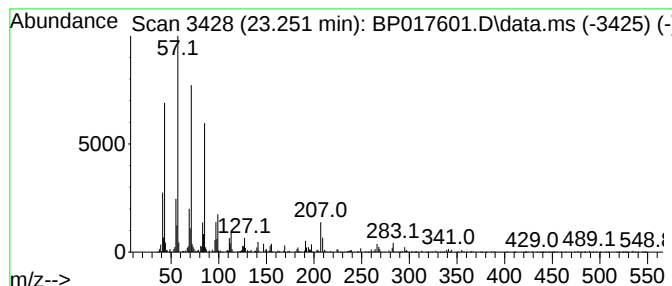

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017601.D
Acq On : 06 Oct 2023 14:47
Operator : MA/JU
Sample : PB156032BL
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK032

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	23.251	2.2	ng/u1	190420	6	24.127	1706300	20.0