

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017606.D
 Acq On : 06 Oct 2023 17:38
 Operator : MA/JU
 Sample : 04624-10
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	20	25	32	rBV	1254487	1714948	44.08%	5.705%
2	3.728	105	109	124	rBV	108891	190838	4.91%	0.635%
3	4.028	158	160	166	rVB4	8676	10139	0.26%	0.034%
4	4.546	244	248	259	rVB	31731	49417	1.27%	0.164%
5	7.093	675	681	691	rBV	100585	173385	4.46%	0.577%
6	7.275	703	712	723	rBV	367592	582477	14.97%	1.938%
7	7.452	735	742	751	rBV	379598	613539	15.77%	2.041%
8	7.934	816	824	836	rBV	302711	509135	13.09%	1.694%
9	8.652	938	946	961	rBV	295795	514178	13.22%	1.711%
10	9.140	1022	1029	1042	rBV	454804	757206	19.46%	2.519%
11	9.858	1141	1151	1160	rBV	371480	620612	15.95%	2.065%
12	10.387	1234	1241	1254	rBV	501923	909843	23.39%	3.027%
13	10.769	1298	1306	1314	rBV	428885	718878	18.48%	2.392%
14	10.940	1328	1335	1351	rBV	379055	694246	17.85%	2.310%
15	12.316	1564	1569	1571	rBV6	2523	4049	0.10%	0.013%
16	12.363	1571	1577	1585	rVB4	8318	17430	0.45%	0.058%
17	12.822	1650	1655	1659	rVB8	2750	5462	0.14%	0.018%
18	13.469	1760	1765	1770	rBV6	7643	14397	0.37%	0.048%
19	13.810	1817	1823	1824	rBV6	2720	4071	0.10%	0.014%
20	13.840	1824	1828	1833	rVV7	3630	6041	0.16%	0.020%
21	14.040	1854	1862	1880	rBV	1116154	1533487	39.42%	5.101%
22	14.322	1903	1910	1922	rBV	1182367	1702968	43.78%	5.665%
23	14.628	1955	1962	1973	rBV	654907	960777	24.70%	3.196%
24	14.881	1999	2005	2021	rBV2	50338	143018	3.68%	0.476%
25	15.628	2123	2132	2143	rBV	1637524	2301523	59.16%	7.657%
26	15.710	2144	2146	2151	rVV5	8701	11838	0.30%	0.039%
27	15.769	2151	2156	2168	rVV	444539	666601	17.14%	2.218%
28	15.869	2170	2173	2176	rVB4	7545	10283	0.26%	0.034%
29	17.081	2374	2379	2383	rVB8	5045	7744	0.20%	0.026%
30	17.416	2430	2436	2445	rBV	880094	1201286	30.88%	3.996%
31	17.516	2447	2453	2468	rVV	1944986	2757214	70.88%	9.172%
32	17.675	2478	2480	2485	rVB6	5031	5662	0.15%	0.019%
33	17.857	2509	2511	2516	rBV6	3162	5010	0.13%	0.017%
34	18.263	2575	2580	2587	rBV3	47044	74190	1.91%	0.247%
35	19.181	2734	2736	2740	rVB4	8963	8281	0.21%	0.028%
36	19.339	2759	2763	2767	rVB3	25694	29342	0.75%	0.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017606.D
Acq On : 06 Oct 2023 17:38
Operator : MA/JU
Sample : 04624-10
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHA1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION

37	19.410	2772	2775	2779	rVB2	24409	26543	0.68%	0.088%
38	19.504	2788	2791	2796	rBV3	37341	48683	1.25%	0.162%
39	19.769	2830	2836	2843	rBV	2639961	3479151	89.43%	11.574%
40	21.551	3134	3139	3146	rBV	1116718	1423746	36.60%	4.736%
41	23.251	3425	3428	3438	rVB2	100968	167189	4.30%	0.556%
42	23.957	3539	3548	3557	rBV2	1808888	3890210	100.00%	12.942%
43	24.127	3570	3577	3586	rVB	703037	1494625	38.42%	4.972%




Sum of corrected areas: 30059662

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017606.D
Acq On : 06 Oct 2023 17:38
Operator : MA/JU
Sample : 04624-10
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

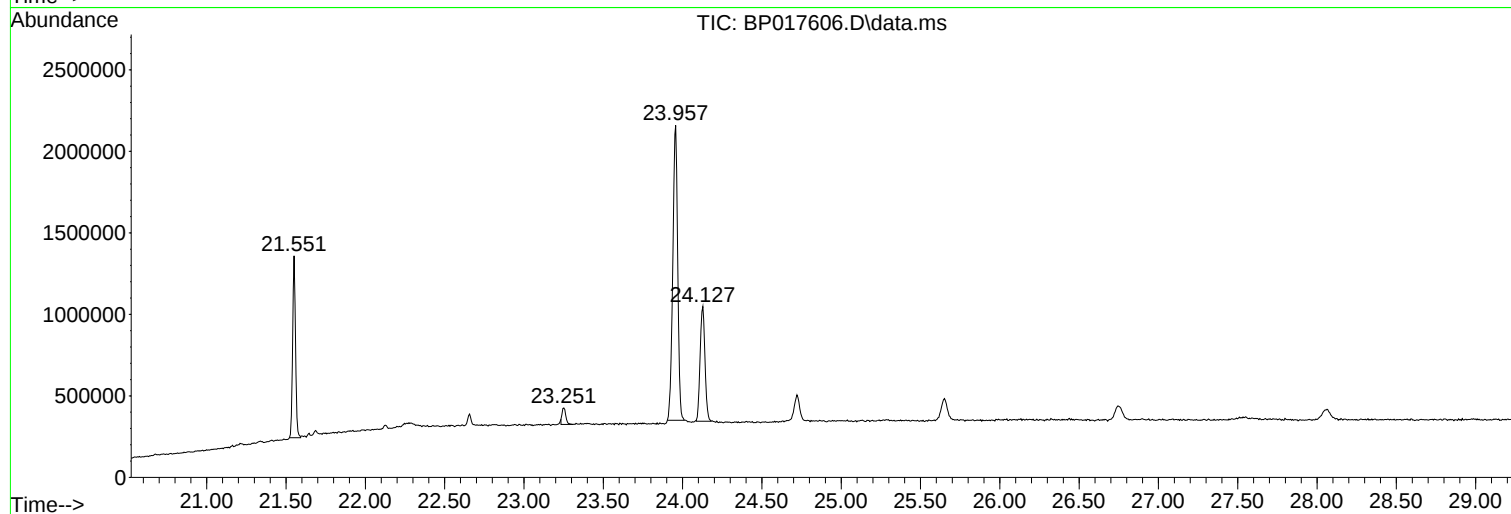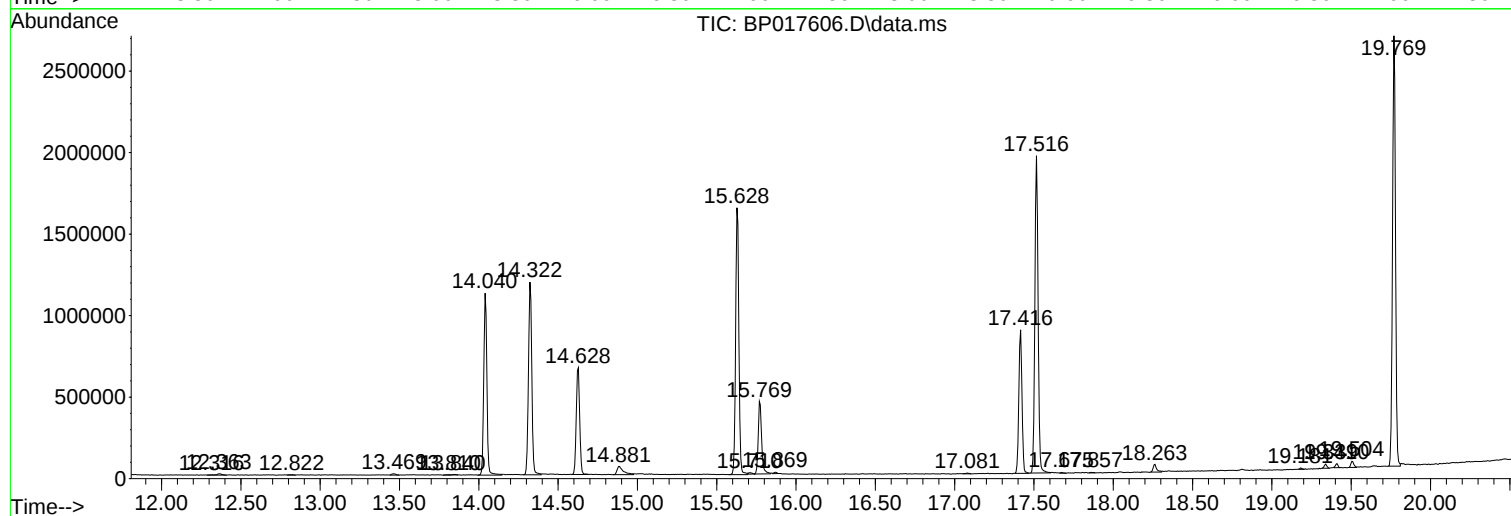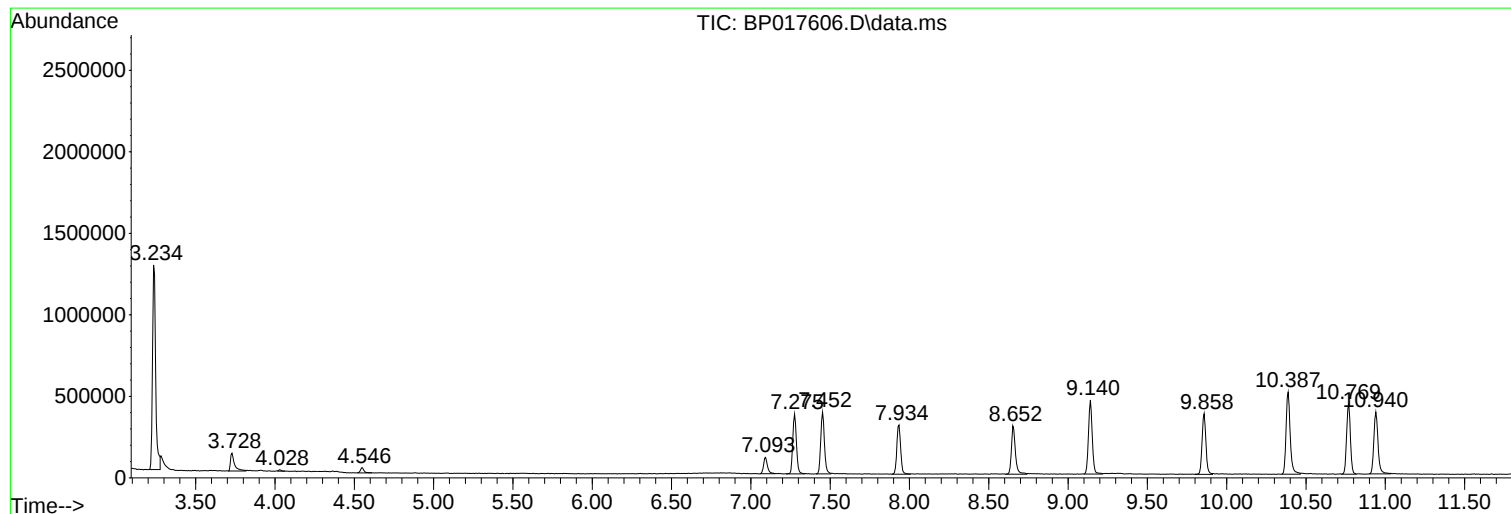

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017606.D
Acq On : 06 Oct 2023 17:38
Operator : MA/JU
Sample : 04624-10
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHA1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.251	2.24 ng/ul	167189	Perylene-d12	24.127

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Eicosane	282	C20H42	000112-95-8	95
2			Tridecane, 1-iodo-	310	C13H27I	035599-77-0	91
3			Nonadecane	268	C19H40	000629-92-5	87
4			Nonadecane	268	C19H40	000629-92-5	87
5			Borane, diethyl(decyloxy)-	226	C14H31BO	1000152-34-3	87

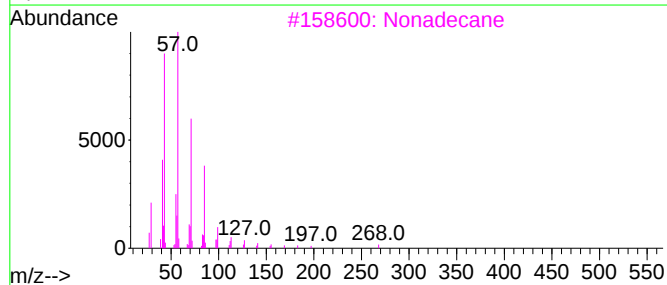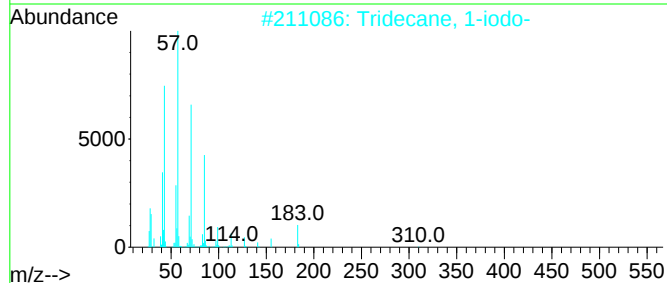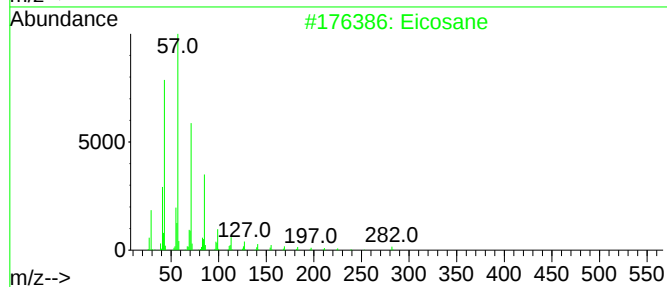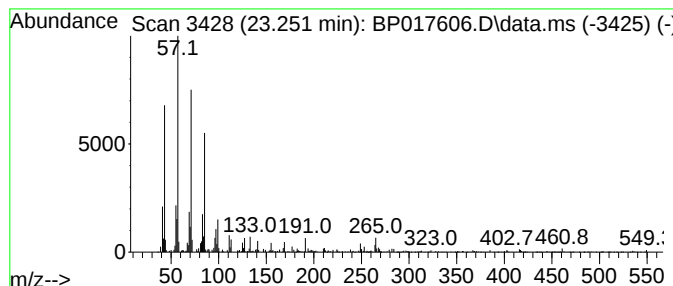

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017606.D
Acq On : 06 Oct 2023 17:38
Operator : MA/JU
Sample : 04624-10
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	23.251	2.2	ng/u1	167189	6	24.127	1494630	20.0