

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017612.D
 Acq On : 06 Oct 2023 21:03
 Operator : MA/JU
 Sample : 04624-15
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	20	25	52	rVB	6781577	9700448	100.00%	22.958%
2	3.722	105	108	123	rBV	141987	229738	2.37%	0.544%
3	4.546	243	248	258	rBV2	23400	38658	0.40%	0.091%
4	7.093	674	681	694	rBV	116630	209599	2.16%	0.496%
5	7.275	706	712	722	rVB	431967	659866	6.80%	1.562%
6	7.452	734	742	754	rBV	453286	716662	7.39%	1.696%
7	7.928	817	823	838	rVB	352587	579977	5.98%	1.373%
8	8.652	939	946	957	rBV	337090	572569	5.90%	1.355%
9	9.140	1021	1029	1042	rBV	504814	845005	8.71%	2.000%
10	9.857	1143	1151	1161	rBV	413664	698004	7.20%	1.652%
11	10.387	1234	1241	1255	rBV	567338	1025414	10.57%	2.427%
12	10.628	1276	1282	1287	rVB9	5374	10144	0.10%	0.024%
13	10.769	1293	1306	1314	rBV	489436	820465	8.46%	1.942%
14	10.940	1326	1335	1353	rBV	540523	968280	9.98%	2.292%
15	11.793	1474	1480	1491	rBV3	29421	81598	0.84%	0.193%
16	12.363	1571	1577	1581	rVB5	8204	12989	0.13%	0.031%
17	13.463	1760	1764	1769	rVB7	9180	15032	0.15%	0.036%
18	14.040	1856	1862	1877	rBV	1331176	1776038	18.31%	4.203%
19	14.322	1902	1910	1922	rBV	1368759	1956639	20.17%	4.631%
20	14.622	1951	1961	1968	rBV	733393	1092131	11.26%	2.585%
21	14.881	1997	2005	2018	rBV2	65178	169760	1.75%	0.402%
22	15.628	2124	2132	2142	rBV	1899806	2658810	27.41%	6.293%
23	15.704	2142	2145	2151	rVV7	16856	31543	0.33%	0.075%
24	15.769	2151	2156	2166	rVV	583189	822430	8.48%	1.946%
25	15.863	2170	2172	2178	rVV7	10133	17827	0.18%	0.042%
26	17.416	2429	2436	2442	rBV	962076	1371991	14.14%	3.247%
27	17.516	2447	2453	2465	rVV	2291758	3192843	32.91%	7.557%
28	18.045	2540	2543	2547	rBV6	6917	11029	0.11%	0.026%
29	18.263	2576	2580	2585	rBV4	37878	56653	0.58%	0.134%
30	19.339	2758	2763	2767	rBV2	30914	46776	0.48%	0.111%
31	19.410	2771	2775	2780	rVB	27399	39872	0.41%	0.094%
32	19.504	2788	2791	2796	rVB6	28239	36764	0.38%	0.087%
33	19.769	2830	2836	2844	rBV	3157954	4056360	41.82%	9.600%
34	21.551	3134	3139	3147	rBV	1255165	1671732	17.23%	3.957%
35	23.957	3540	3548	3561	rVB2	2141546	4325035	44.59%	10.236%
36	24.127	3570	3577	3587	rVB	836278	1734036	17.88%	4.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017612.D
Acq On : 06 Oct 2023 21:03
Operator : MA/JU
Sample : 04624-15
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHA3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 42252717

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017612.D
Acq On : 06 Oct 2023 21:03
Operator : MA/JU
Sample : 04624-15
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

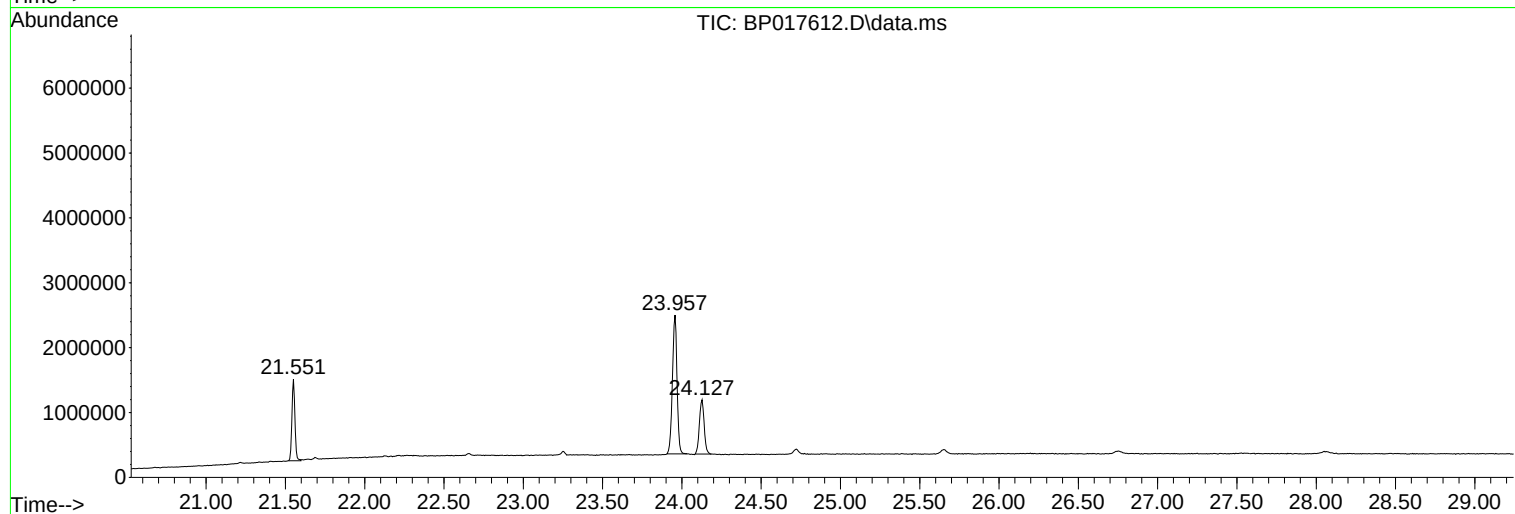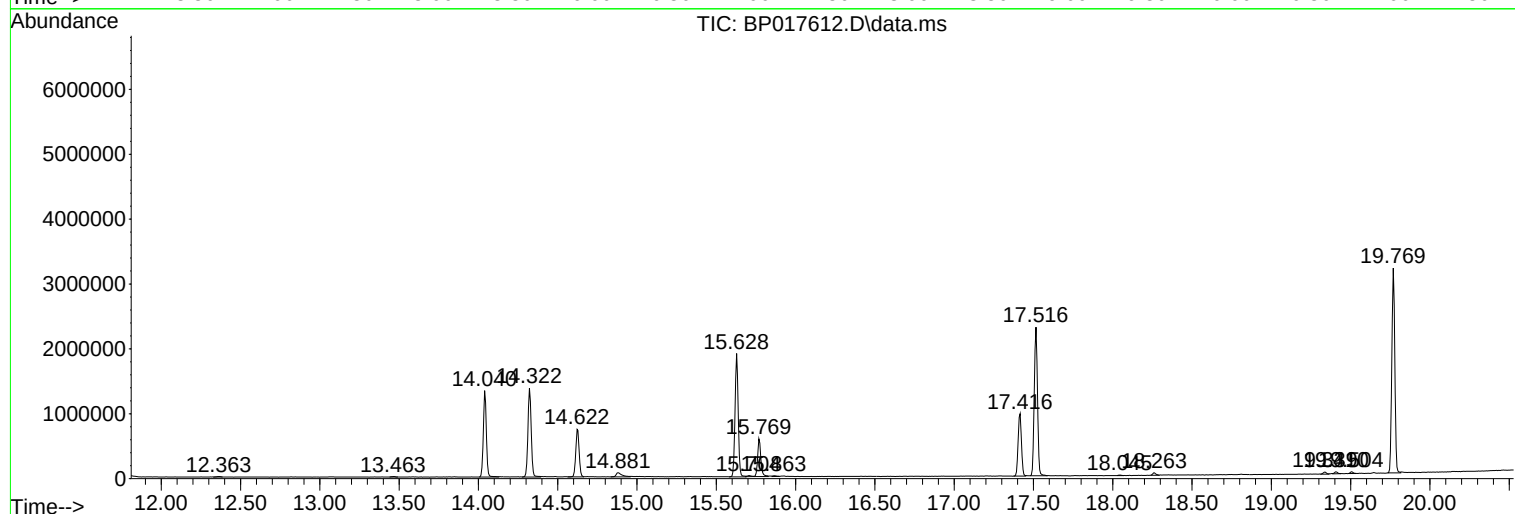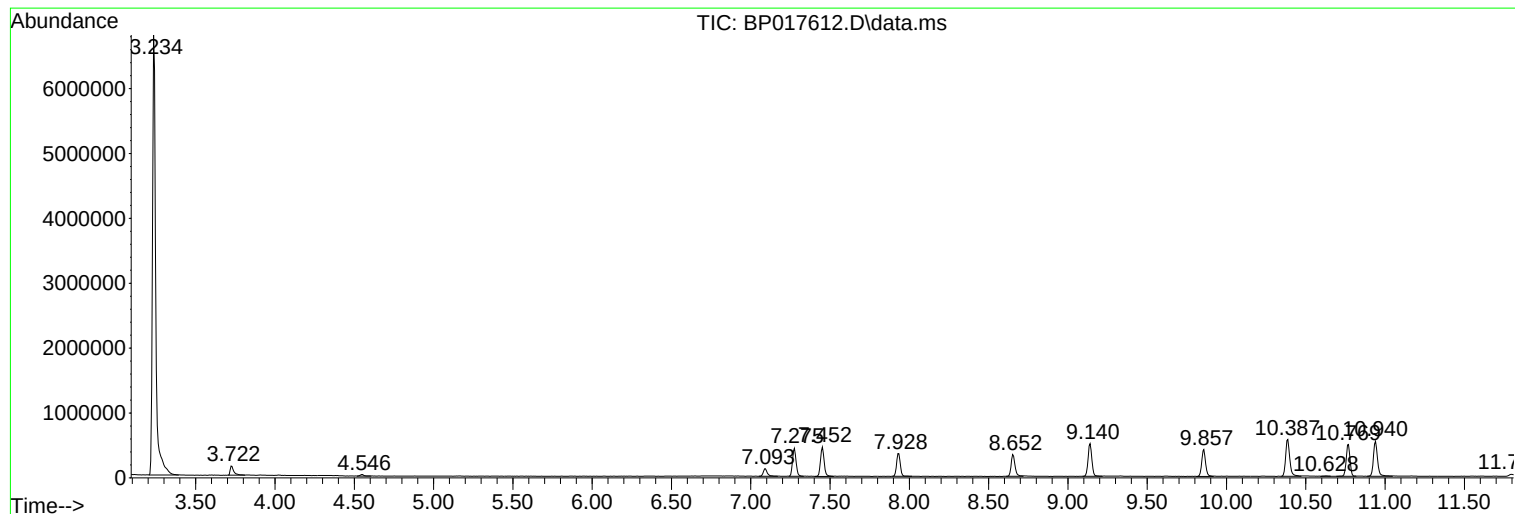

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017612.D
Acq On : 06 Oct 2023 21:03
Operator : MA/JU
Sample : 04624-15
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017612.D
Acq On : 06 Oct 2023 21:03
Operator : MA/JU
Sample : 04624-15
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------