

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017615.D
 Acq On : 06 Oct 2023 22:46
 Operator : MA/JU
 Sample : 04624-19
 Misc :
 ALS Vial : 95 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	30	rVB	19596	23486	0.56%	0.072%
2	3.281	30	33	38	rBV	21649	27087	0.64%	0.083%
3	3.728	106	109	119	rBV	146084	241339	5.71%	0.742%
4	4.028	157	160	165	rVB5	5757	7223	0.17%	0.022%
5	4.546	242	248	261	rBV	501976	761551	18.00%	2.342%
6	5.016	325	328	334	rVB8	2441	4461	0.11%	0.014%
7	5.616	428	430	436	rVB7	2679	5092	0.12%	0.016%
8	6.340	550	553	556	rBV4	3209	6078	0.14%	0.019%
9	7.093	675	681	694	rBV	134171	233256	5.51%	0.717%
10	7.275	705	712	720	rBV	441852	675335	15.96%	2.077%
11	7.452	735	742	753	rBV	472295	749517	17.72%	2.305%
12	7.934	817	824	836	rVB	317639	516378	12.21%	1.588%
13	8.652	939	946	960	rBV	376382	640630	15.14%	1.970%
14	9.140	1022	1029	1042	rBV	532176	858557	20.30%	2.641%
15	9.857	1144	1151	1165	rBV	430802	711976	16.83%	2.190%
16	10.387	1234	1241	1259	rBV	617128	1119217	26.46%	3.443%
17	10.769	1299	1306	1314	rVB	437335	722784	17.09%	2.223%
18	10.940	1327	1335	1351	rBV	554180	997158	23.57%	3.067%
19	11.081	1357	1359	1364	rVB6	3833	5248	0.12%	0.016%
20	11.822	1479	1485	1487	rBV7	2887	6306	0.15%	0.019%
21	12.363	1572	1577	1581	rBV2	8804	14662	0.35%	0.045%
22	12.928	1667	1673	1680	rBV6	13952	26757	0.63%	0.082%
23	12.998	1680	1685	1692	rBV	32268	64292	1.52%	0.198%
24	13.187	1714	1717	1720	rBV5	3586	5194	0.12%	0.016%
25	13.463	1759	1764	1768	rBV2	20512	29945	0.71%	0.092%
26	13.563	1773	1781	1786	rBV6	11019	21654	0.51%	0.067%
27	13.640	1790	1794	1800	rBV2	17391	33639	0.80%	0.103%
28	13.704	1800	1805	1814	rVB	16656	30539	0.72%	0.094%
29	13.839	1827	1828	1833	rVB5	3874	4682	0.11%	0.014%
30	14.039	1856	1862	1876	rBV	1303414	1770200	41.85%	5.445%
31	14.322	1903	1910	1920	rBV	1428806	2037100	48.16%	6.266%
32	14.628	1955	1962	1972	rBV	667866	975840	23.07%	3.002%
33	14.881	1999	2005	2017	rBV2	66592	168586	3.99%	0.519%
34	15.375	2086	2089	2092	rVB5	5351	6714	0.16%	0.021%
35	15.422	2092	2097	2098	rBV5	4190	7255	0.17%	0.022%
36	15.628	2125	2132	2143	rBV	1909080	2659023	62.86%	8.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017615.D
 Acq On : 06 Oct 2023 22:46
 Operator : MA/JU
 Sample : 04624-19
 Misc :
 ALS Vial : 95 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

37	15.769	2150	2156	2168	rBV	519731	745863	17.63%	2.294%
38	15.869	2170	2173	2180	rVB8	10472	16777	0.40%	0.052%
39	16.675	2308	2310	2315	rVB6	3903	5466	0.13%	0.017%
40	17.416	2429	2436	2446	rBV	875179	1239668	29.30%	3.813%
41	17.516	2446	2453	2464	rBV	2162534	2989787	70.68%	9.196%
42	18.263	2575	2580	2589	rBV2	61468	105098	2.48%	0.323%
43	19.333	2759	2762	2766	rVB4	25599	31839	0.75%	0.098%
44	19.404	2772	2774	2779	rVB	25207	30364	0.72%	0.093%
45	19.504	2788	2791	2797	rBV3	41838	57484	1.36%	0.177%
46	19.769	2830	2836	2843	rBV	2946137	3812922	90.14%	11.728%
47	21.551	3134	3139	3146	rBV	1179470	1516705	35.85%	4.665%
48	23.957	3539	3548	3559	rBV	1962123	4230231	100.00%	13.012%
49	24.127	3570	3577	3586	rVB	712381	1560395	36.89%	4.800%




Sum of corrected areas: 32511360

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017615.D
Acq On : 06 Oct 2023 22:46
Operator : MA/JU
Sample : 04624-19
Misc :
ALS Vial : 95 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

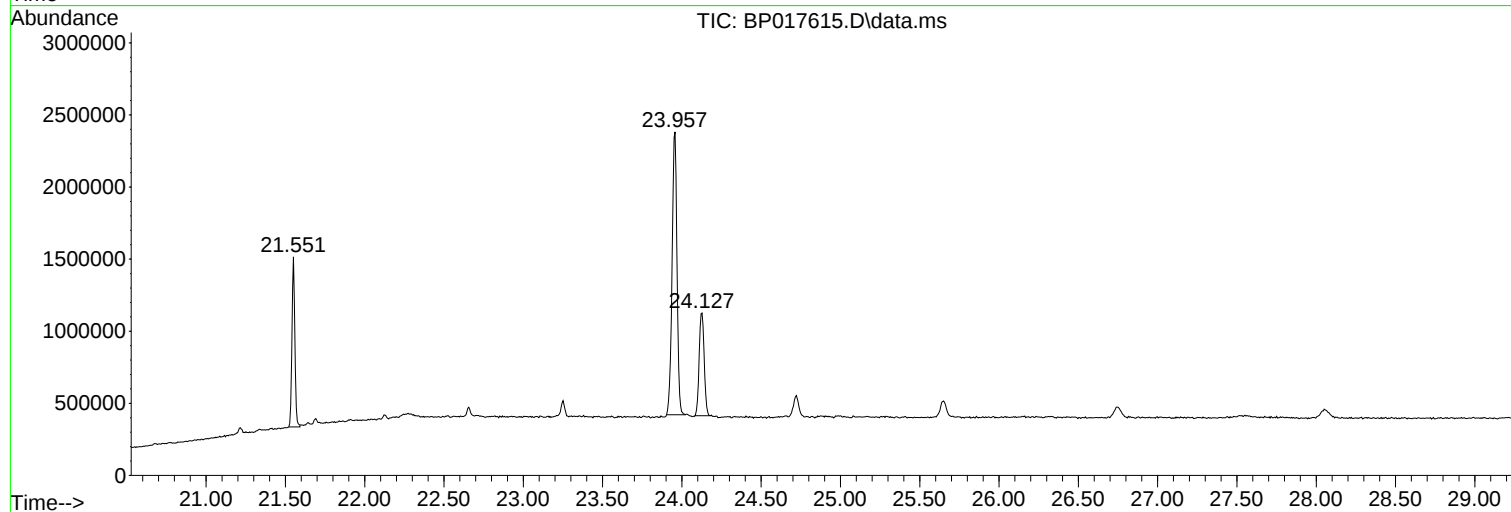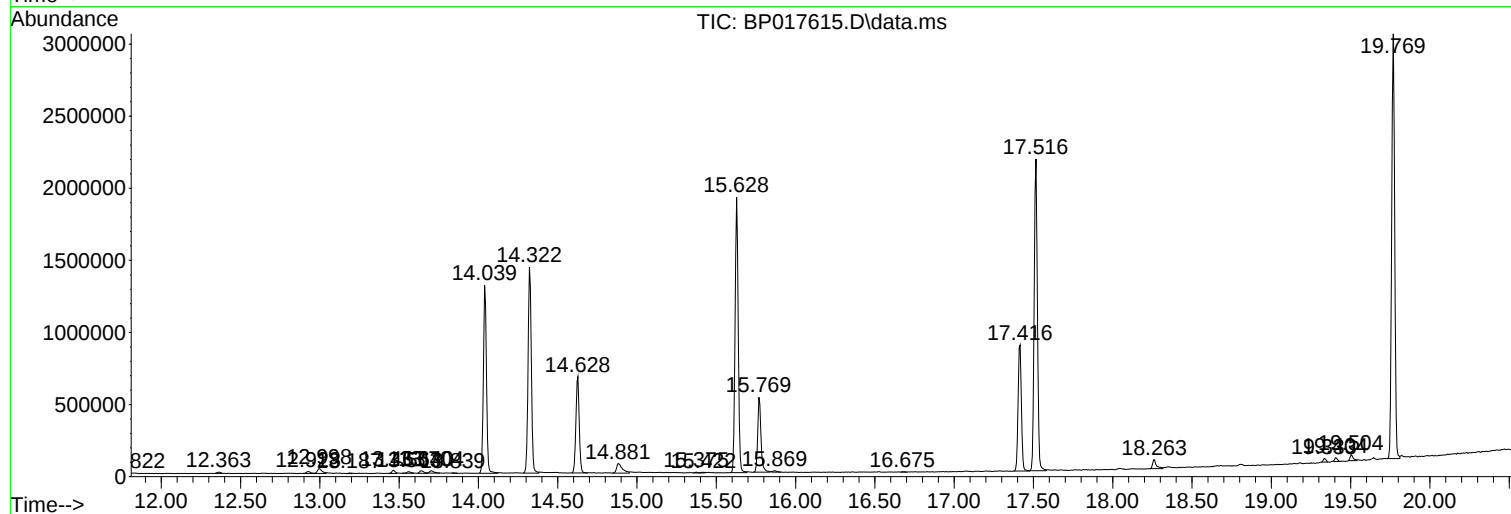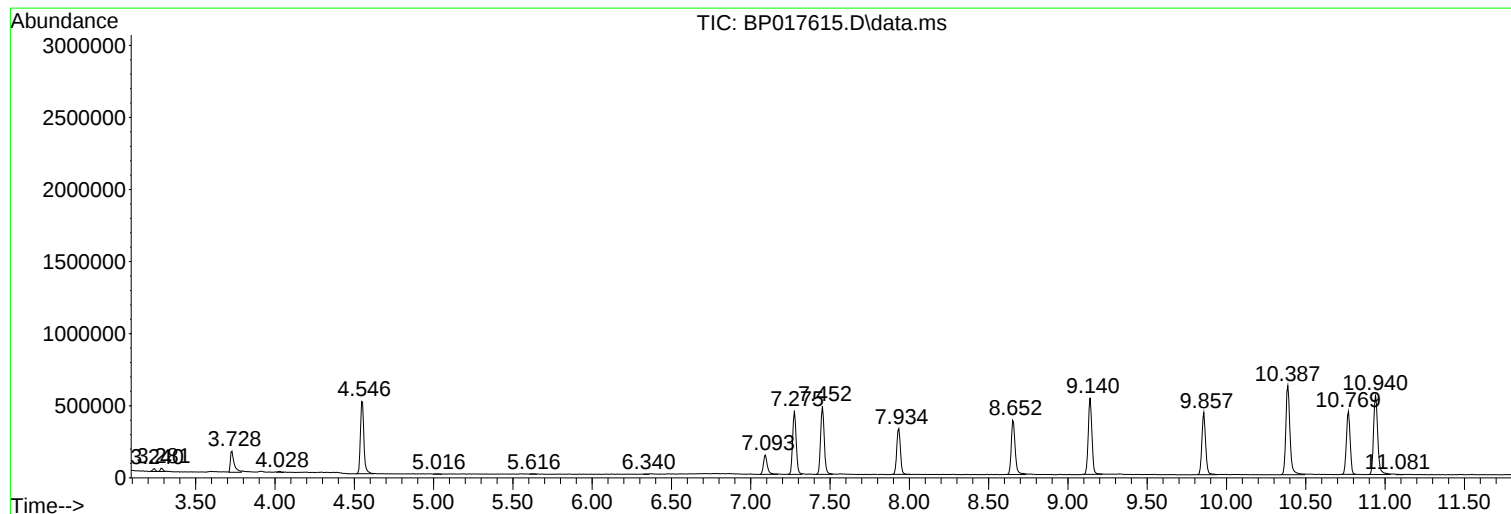

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017615.D
Acq On : 06 Oct 2023 22:46
Operator : MA/JU
Sample : 04624-19
Misc :
ALS Vial : 95 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHB3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.546	29.50 ng/ul	761551	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

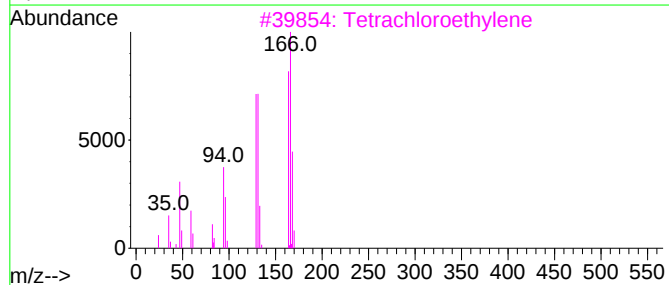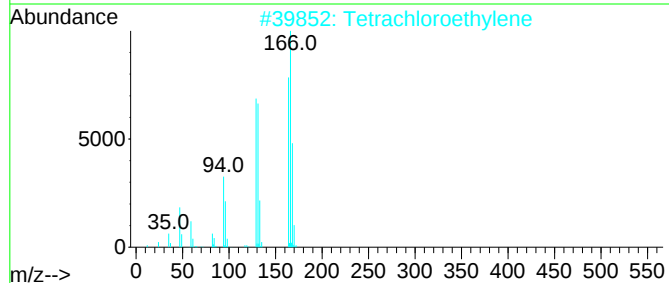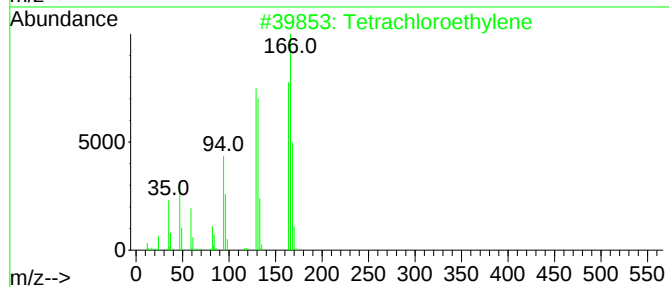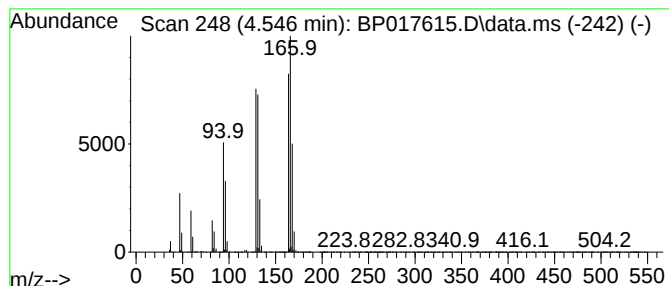

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017615.D
Acq On : 06 Oct 2023 22:46
Operator : MA/JU
Sample : 04624-19
Misc :
ALS Vial : 95 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.546	29.5	ng/u1	761551	1	7.934	516378	20.0