

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017616.D
 Acq On : 06 Oct 2023 23:21
 Operator : MA/JU
 Sample : 04624-20
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	38	rVB	20819	25913	0.65%	0.091%
2	3.728	106	109	123	rBV	69913	121545	3.06%	0.426%
3	3.911	136	140	148	rVB4	5714	11548	0.29%	0.040%
4	4.028	157	160	162	rVB4	5747	4456	0.11%	0.016%
5	4.546	243	248	257	rVB	115311	170271	4.28%	0.596%
6	7.093	675	681	693	rBV	109194	185527	4.67%	0.650%
7	7.275	702	712	725	rBV	392226	598881	15.07%	2.098%
8	7.452	735	742	753	rBV	389079	616017	15.50%	2.158%
9	7.934	816	824	834	rBV	317442	519868	13.08%	1.821%
10	8.216	865	872	879	rBV10	9478	23847	0.60%	0.084%
11	8.652	940	946	965	rBV	294839	512828	12.90%	1.796%
12	9.057	1012	1015	1019	rVB6	4384	5189	0.13%	0.018%
13	9.140	1022	1029	1036	rBV	482007	777732	19.57%	2.724%
14	9.257	1043	1049	1055	rVB	7772	12782	0.32%	0.045%
15	9.857	1144	1151	1161	rBV	321504	544136	13.69%	1.906%
16	10.387	1234	1241	1254	rBV	504987	908695	22.86%	3.183%
17	10.769	1298	1306	1319	rBV	434074	738443	18.58%	2.586%
18	10.899	1322	1328	1329	rBV6	2789	4704	0.12%	0.016%
19	10.940	1329	1335	1353	rVB	335370	618184	15.55%	2.165%
20	11.557	1435	1440	1441	rBV5	3506	5153	0.13%	0.018%
21	12.369	1574	1578	1585	rVB5	8359	14853	0.37%	0.052%
22	12.875	1660	1664	1668	rBV7	2656	4122	0.10%	0.014%
23	13.187	1713	1717	1721	rBV7	3625	4421	0.11%	0.015%
24	13.463	1759	1764	1769	rBV2	13223	20805	0.52%	0.073%
25	14.040	1856	1862	1876	rBV	1097350	1482794	37.30%	5.193%
26	14.322	1899	1910	1922	rBV	1207021	1757080	44.20%	6.154%
27	14.622	1951	1961	1969	rBV	695082	996220	25.06%	3.489%
28	14.887	2000	2006	2020	rBV3	33142	100841	2.54%	0.353%
29	15.304	2073	2077	2079	rBV5	4111	4652	0.12%	0.016%
30	15.369	2083	2088	2092	rBV8	2382	4702	0.12%	0.016%
31	15.628	2124	2132	2143	rBV	1624242	2326178	58.52%	8.147%
32	15.769	2150	2156	2167	rBV	330514	486216	12.23%	1.703%
33	15.869	2170	2173	2182	rVV10	9555	19861	0.50%	0.070%
34	15.934	2182	2184	2190	rVB5	2695	4087	0.10%	0.014%
35	16.428	2262	2268	2273	rBV10	3395	5999	0.15%	0.021%
36	17.075	2376	2378	2382	rBV5	3434	4192	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
 Data File : BP017616.D
 Acq On : 06 Oct 2023 23:21
 Operator : MA/JU
 Sample : 04624-20
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
 Title : SVOA CALIBRATION

37	17.410	2429	2435	2446	rBV	898165	1260850	31.72%	4.416%
38	17.510	2446	2452	2466	rBV	2005364	2919555	73.45%	10.226%
39	17.675	2477	2480	2485	rVB7	4122	5880	0.15%	0.021%
40	18.045	2538	2543	2548	rBV5	28207	37801	0.95%	0.132%
41	18.257	2575	2579	2589	rVV6	23923	38828	0.98%	0.136%
42	19.333	2759	2762	2766	rVB3	24354	31654	0.80%	0.111%
43	19.404	2771	2774	2780	rVB	25714	33344	0.84%	0.117%
44	19.504	2788	2791	2794	rBV4	18338	22548	0.57%	0.079%
45	19.769	2830	2836	2843	rBV	2831576	3572836	89.88%	12.514%
46	21.545	3134	3138	3147	rVB	1117707	1449081	36.45%	5.075%
47	23.951	3538	3547	3560	rVB	1855887	3975109	100.00%	13.923%
48	24.121	3570	3576	3590	rVB	739616	1561278	39.28%	5.468%




Sum of corrected areas: 28551506

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017616.D
Acq On : 06 Oct 2023 23:21
Operator : MA/JU
Sample : 04624-20
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

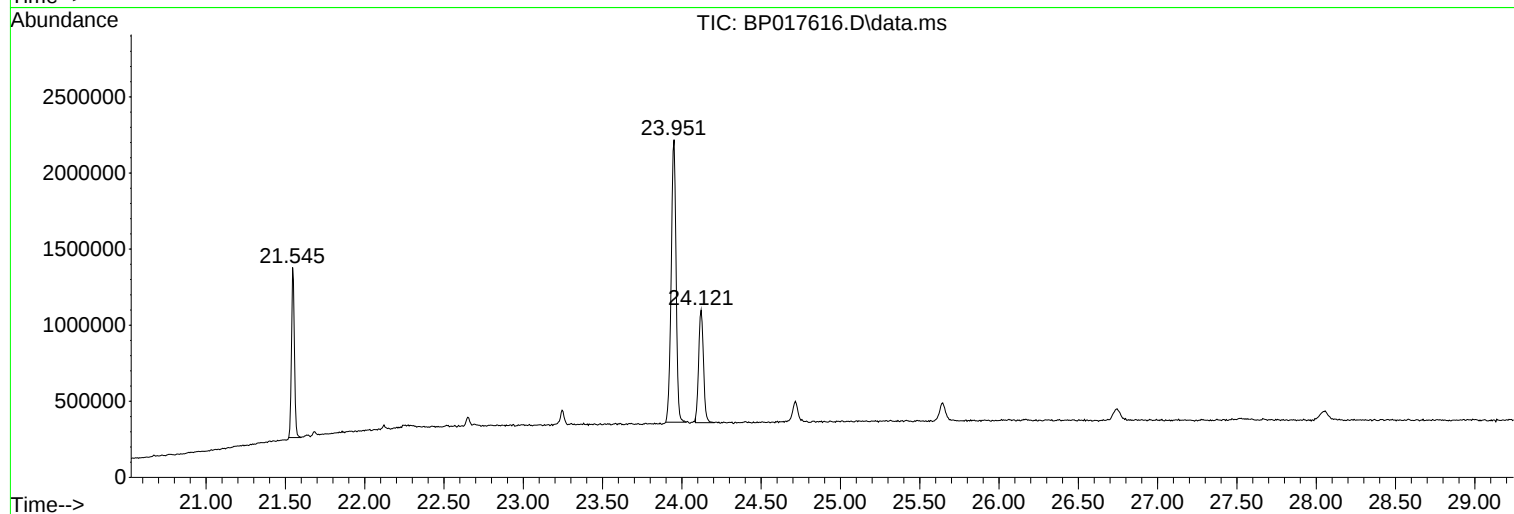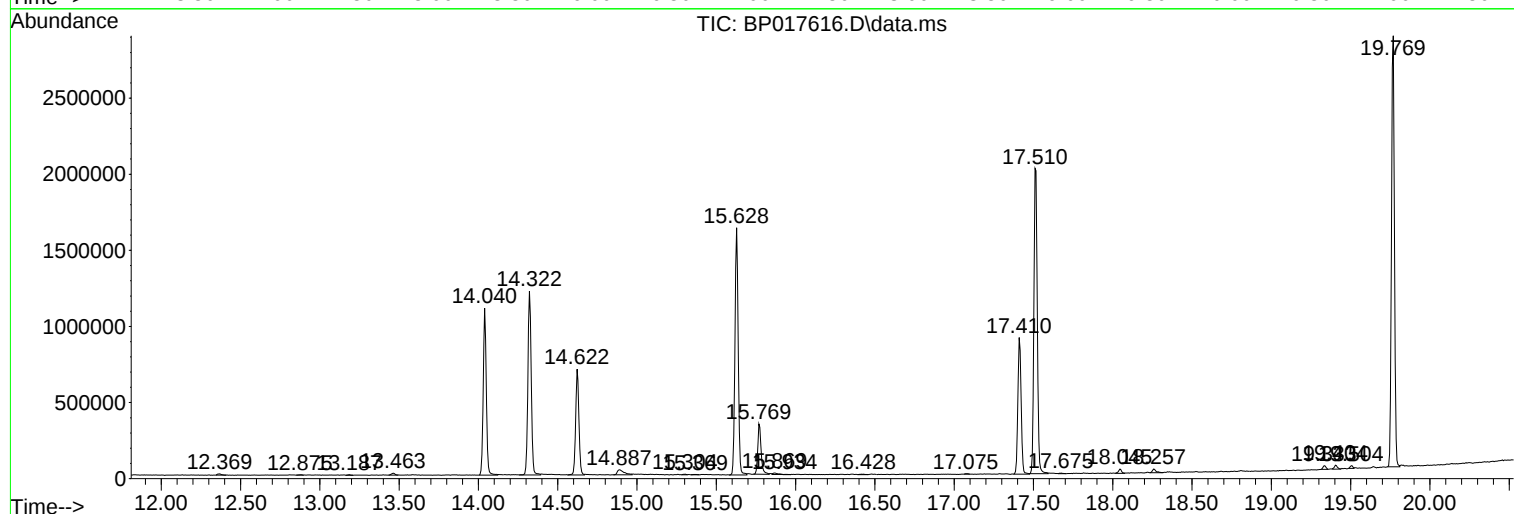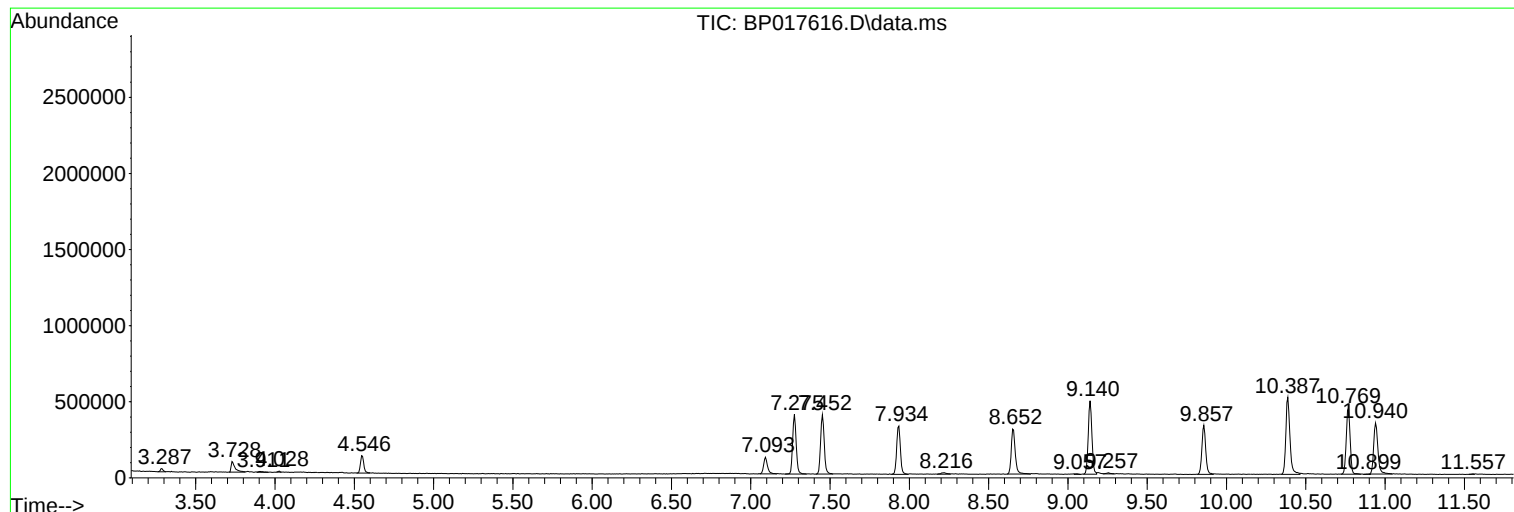

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017616.D
Acq On : 06 Oct 2023 23:21
Operator : MA/JU
Sample : 04624-20
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK86










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.546	6.55 ng/ul	170271	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	43

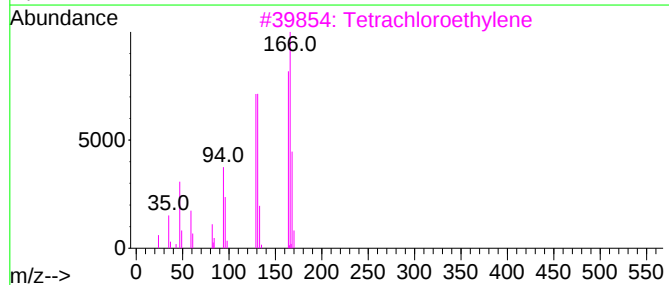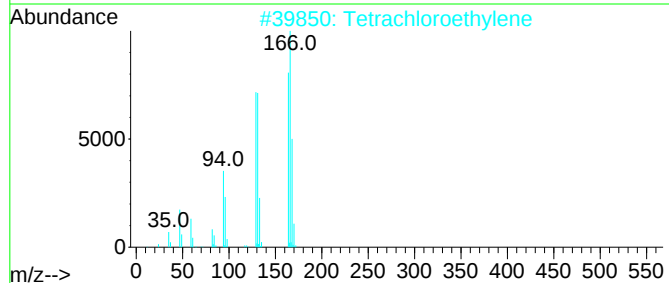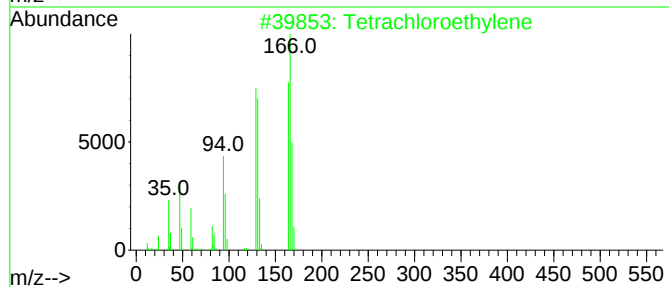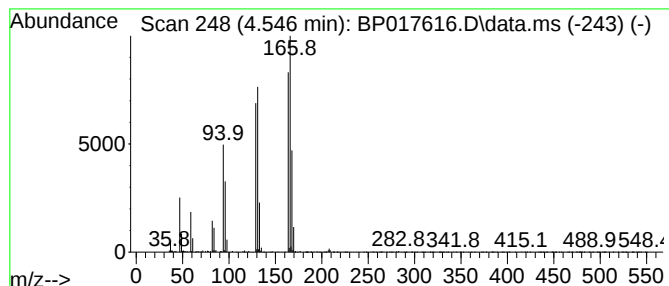

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100423\
Data File : BP017616.D
Acq On : 06 Oct 2023 23:21
Operator : MA/JU
Sample : 04624-20
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.546	6.5	ng/u1	170271	1	7.934	519868	20.0