




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011934.D
 Acq On : 05 Oct 2022 17:22
 Operator : CG/JU
 Sample : N4890-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0E3

Manual Integrations APPROVED

Quant Time: Oct 05 23:23:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay
 10/06/2022
 Supervised By :mohammad
 ahmed
 10/10/2022

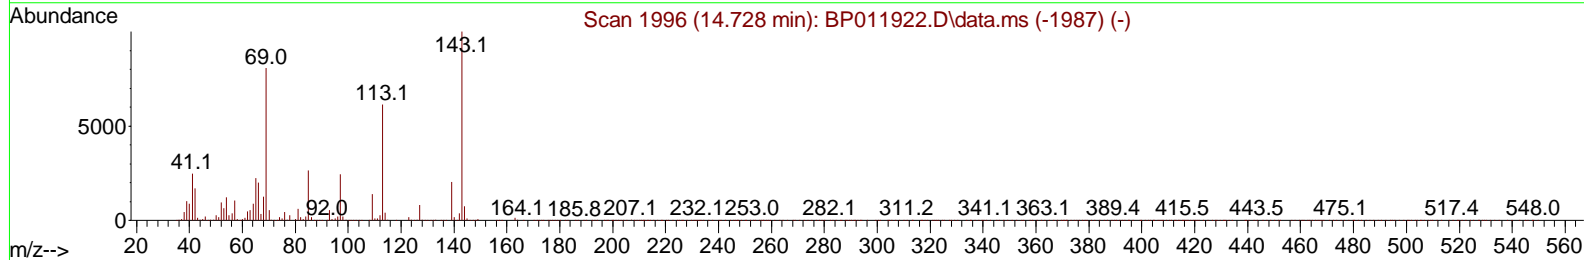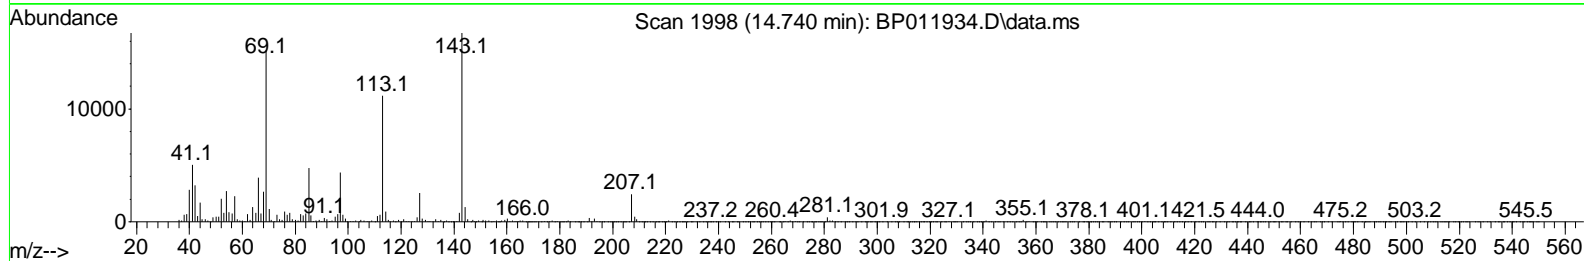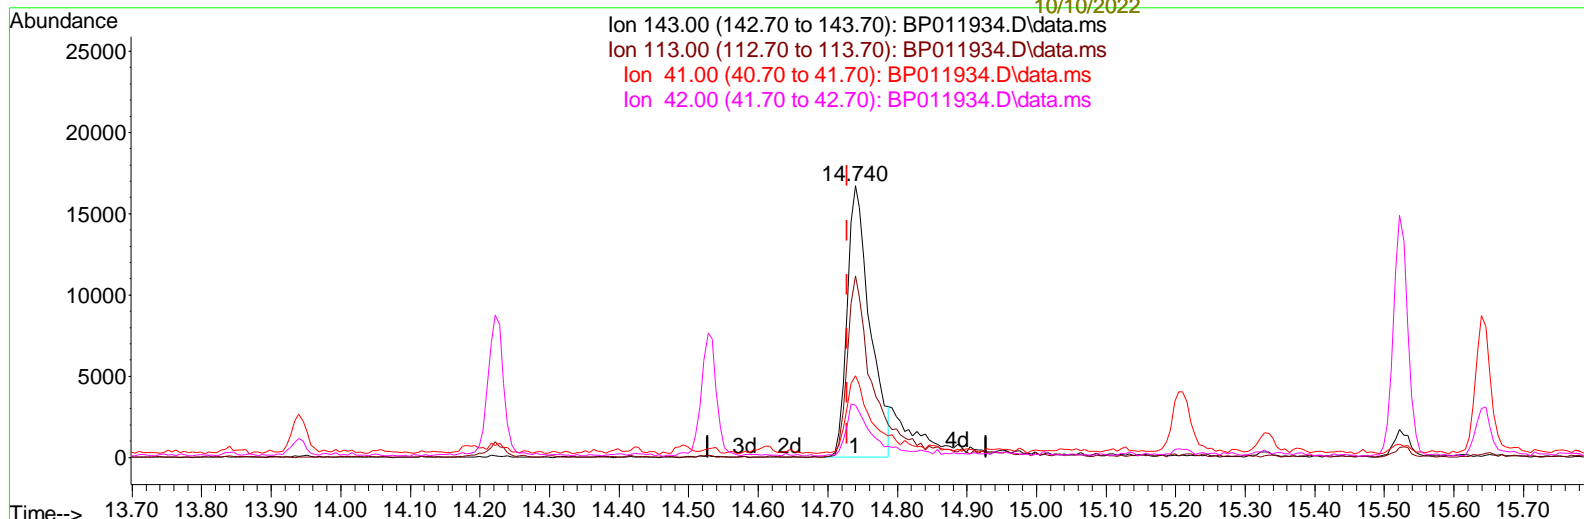

TIC: BP011934.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.740min (+ 0.012) 4.19 ng/ul

response 37873

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.80	66.84
41.00	24.20	30.12#
42.00	16.40	19.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011934.D
 Acq On : 05 Oct 2022 17:22
 Operator : CG/JU
 Sample : N4890-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1


Instrument :
 BNA_P
ClientSampleId :
 EY0E3

Manual Integrations APPROVED



Quant Time: Oct 05 23:23:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay
 10/06/2022

Supervised By :mohammad
 ahmed
 10/10/2022

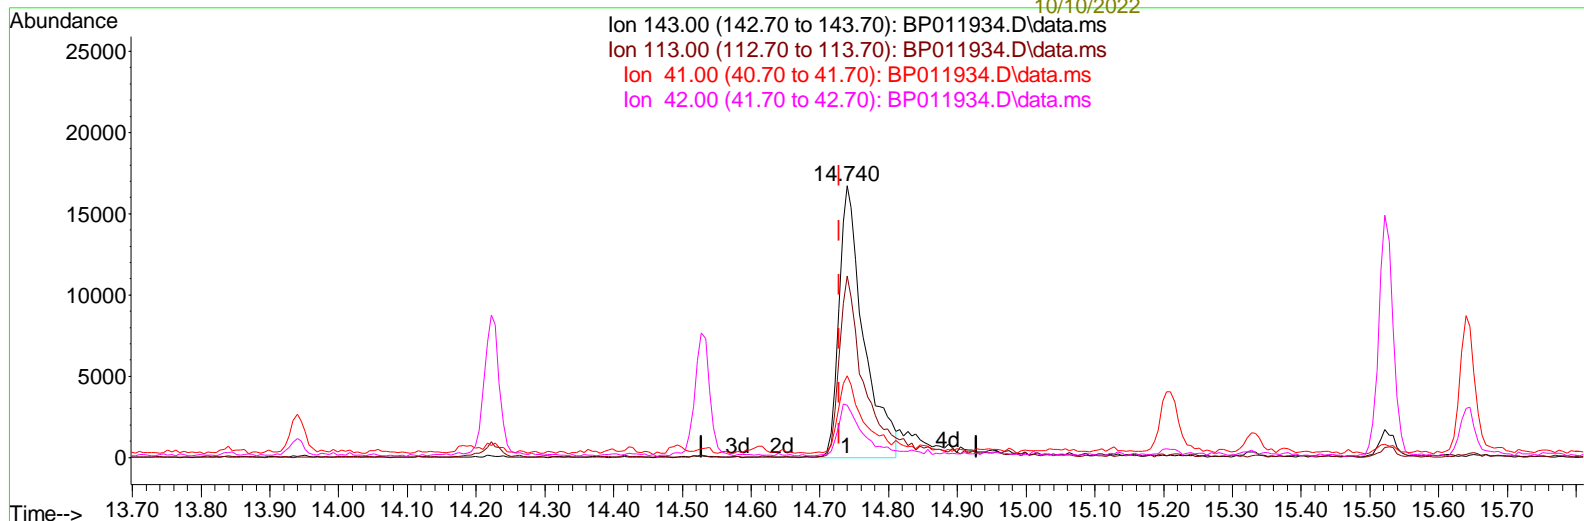

Ion 143.00 (142.70 to 143.70): BP011934.D\data.ms
 Ion 113.00 (112.70 to 113.70): BP011934.D\data.ms
 Ion 41.00 (40.70 to 41.70): BP011934.D\data.ms
 Ion 42.00 (41.70 to 42.70): BP011934.D\data.ms

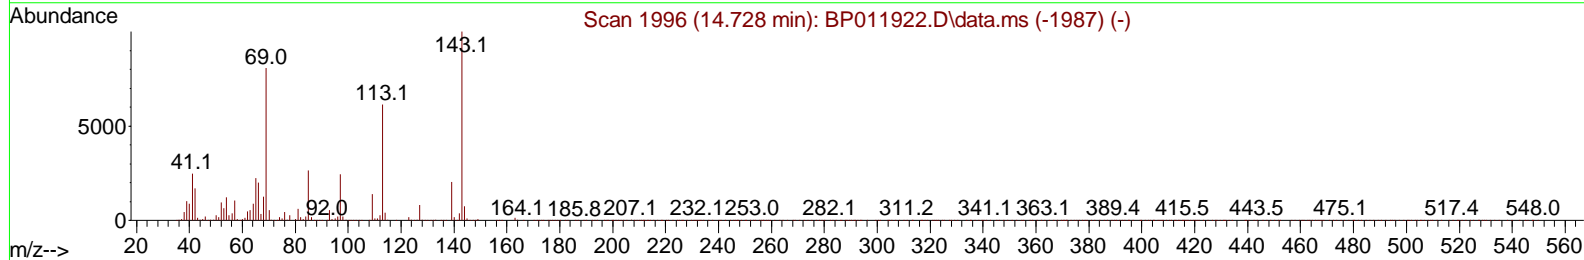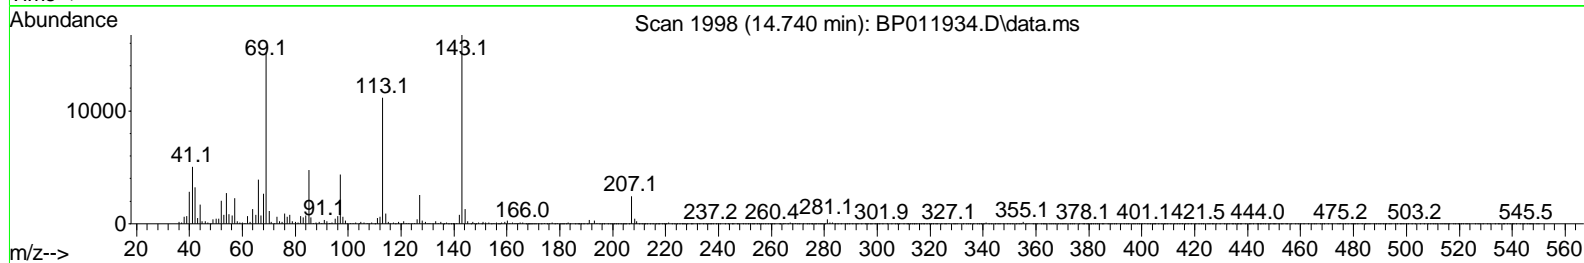

TIC: BP011934.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.740min (+ 0.012) 4.57 ng/ul m

response 41301

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.80	66.84
41.00	24.20	30.12#
42.00	16.40	19.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011934.D
 Acq On : 05 Oct 2022 17:22
 Operator : CG/JU
 Sample : N4890-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 EY0E3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut
 Upadhyay
 10/06/2022

Supervised By :mohammad
 ahmed
 10/10/2022

Quant Time: Oct 05 23:23:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Compound	R. T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	247856	20.000	ng/ul	0.00
20) Naphthalene-d8	10.693	136	1019588	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	610222	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1283304	20.000	ng/ul	0.00
79) Chrysene-d12	21.374	240	1288619	20.000	ng/ul	0.00
88) Perylene-d12	23.804	264	1305518	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	28487	5.069	ng/uL	0.00
4) Pyridine-d5	3.734	84	68206	4.143	ng/ul	0.01
7) Phenol-d5	7.046	99	145617	6.805	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	389424	32.834	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	440887	26.102	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	274077	15.495	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	269452	34.696	ng/ul	0.00
24) 2-Nitrophenol-d4	9.775	143	275151	33.115	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.310	165	480809	31.285	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	412969	17.626	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	1546150	35.432	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	1789395	35.970	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	41301m	4.571	ng/ul	0.01
60) Fluorene-d10	15.522	176	1428593	37.697	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	206720	26.614	ng/ul	0.00
73) Anthracene-d10	17.386	188	2299690	39.340	ng/ul	0.00
81) Pyrene-d10	19.622	212	2726502	41.778	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.651	264	2643816	40.455	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011934.D
 Acq On : 05 Oct 2022 17:22
 Operator : CG/JU
 Sample : N4890-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 EY0E3

Quant Time: Oct 05 23:23:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay
 10/06/2022

Supervised By : mohammad ahmed
 10/10/2022

