




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011935.D
 Acq On : 05 Oct 2022 17:56
 Operator : CG/JU
 Sample : N4819-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Q0

Manual IntegrationsAPPROVED

Quant Time: Oct 05 23:23:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/06/2022
 Supervised By :mohammad ahmed 10/10/2022

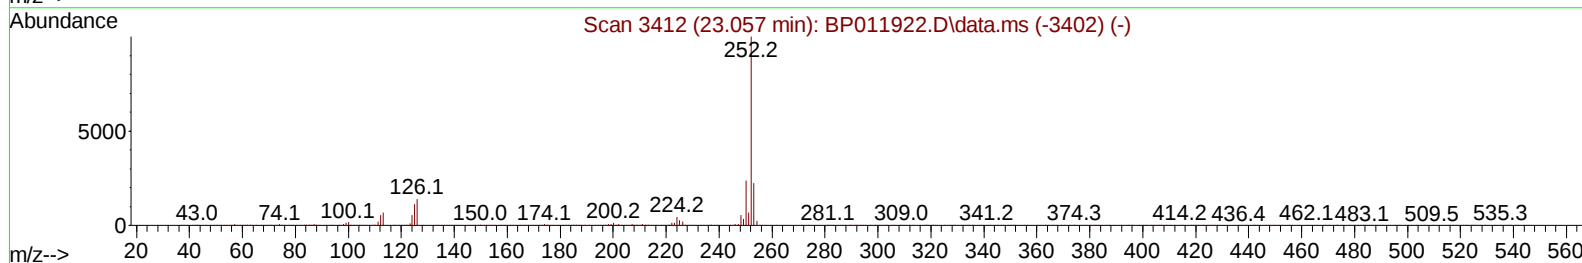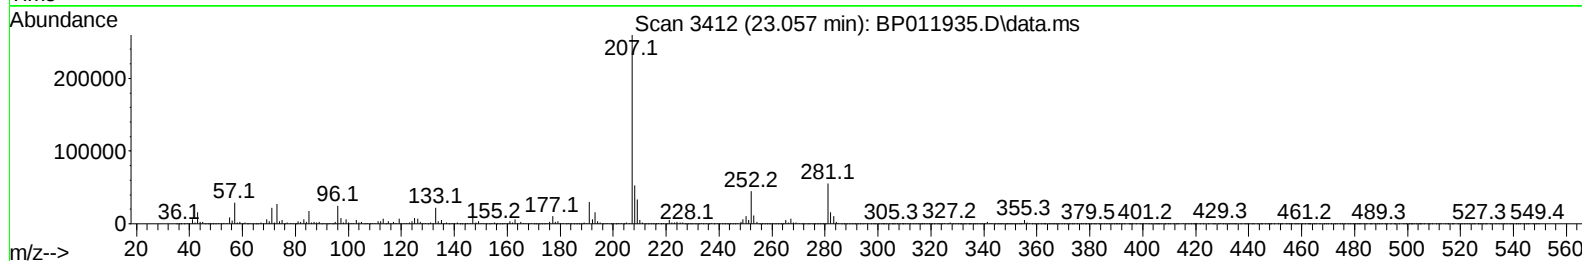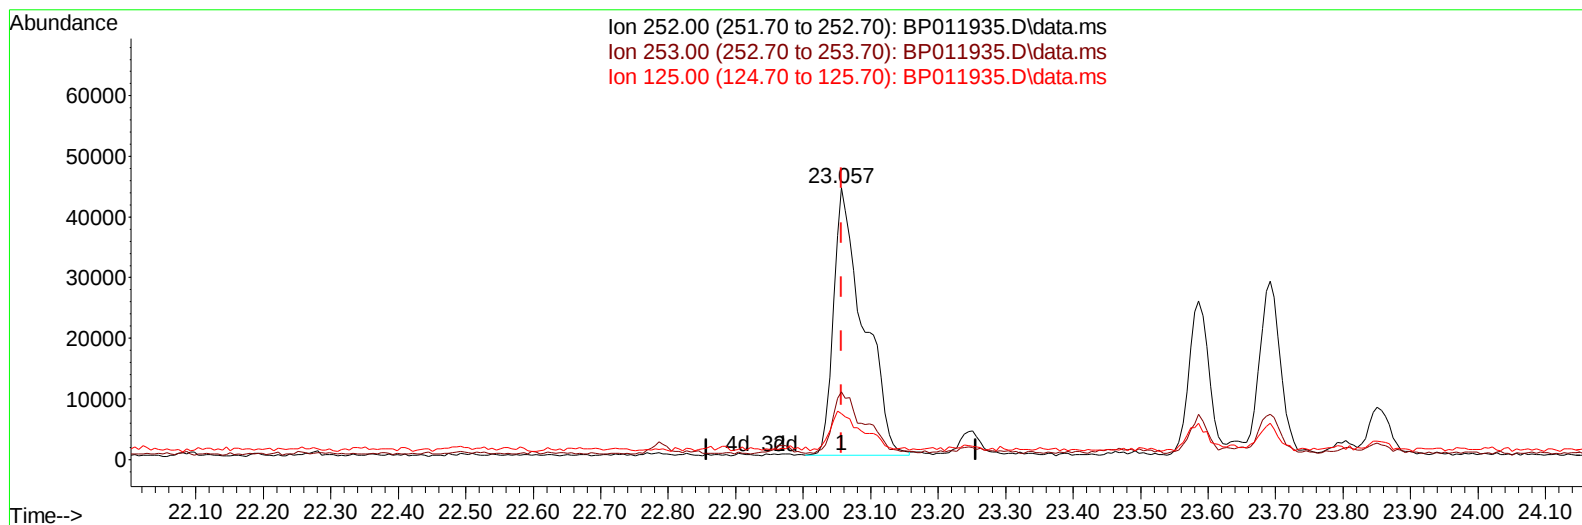

TIC: BP011935.D\data.ms

(90) Benzo(b)fluoranthene

23.057min (+ 0.000) 1.76 ng/u1

response 135510

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.30	24.82
125.00	11.50	16.80#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011935.D
 Acq On : 05 Oct 2022 17:56
 Operator : CG/JU
 Sample : N4819-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Q0

Manual IntegrationsAPPROVED

Quant Time: Oct 05 23:23:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/06/2022
 Supervised By :mohammad ahmed 10/10/2022

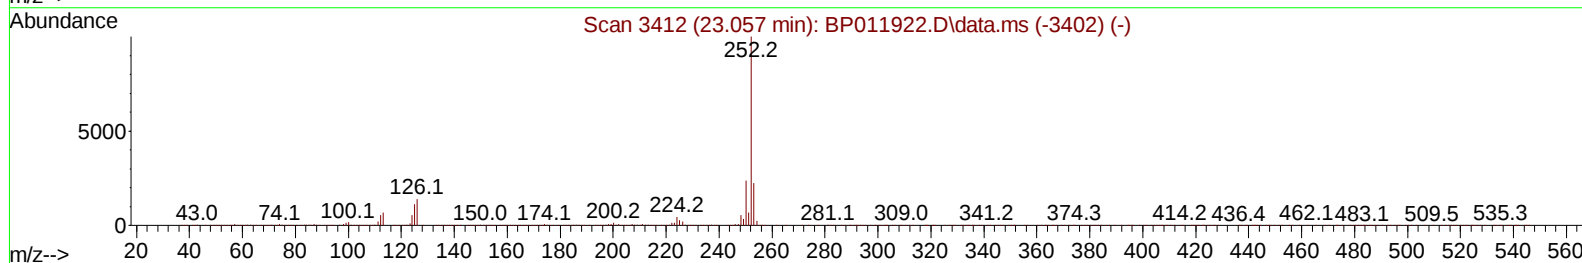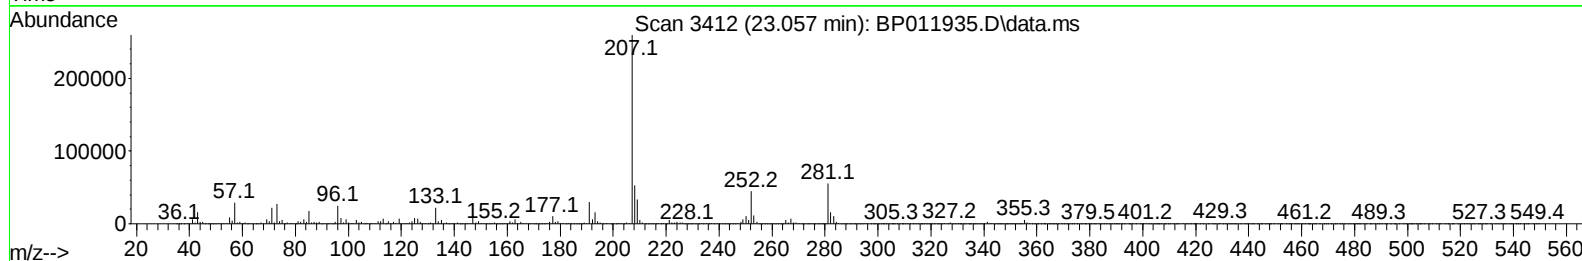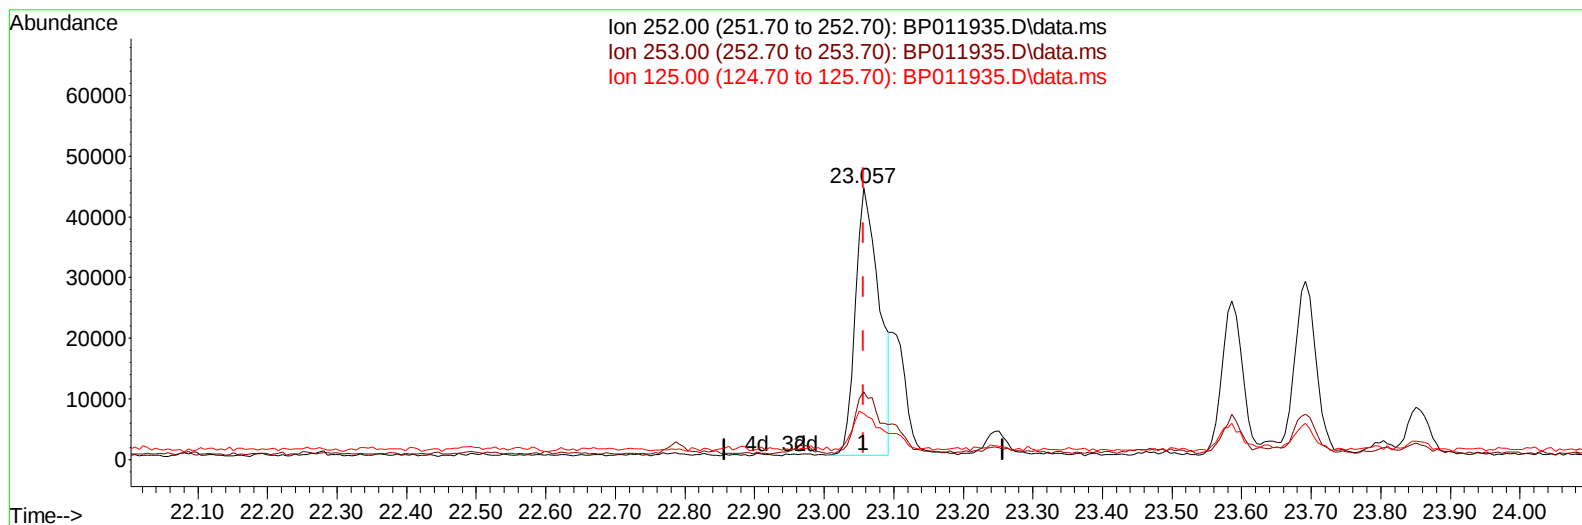

TIC: BP011935.D\data.ms

(90) Benzo(b)fluoranthene

23.057min (+ 0.000) 1.37 ng/u1 m

response 105339

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.30	24.82
125.00	11.50	16.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011935.D
 Acq On : 05 Oct 2022 17:56
 Operator : CG/JU
 Sample : N4819-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Q0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/06/2022
 Supervised By :mohammad ahmed 10/10/2022

Quant Time: Oct 05 23:23:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	224673	20.000	ng/ul	0.00
20) Naphthalene-d8	10.693	136	916104	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	550945	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1157160	20.000	ng/ul	0.00
79) Chrysene-d12	21.369	240	1186492	20.000	ng/ul	0.00
88) Perylene-d12	23.804	264	1208580	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	17270	3.390	ng/uL	0.00
4) Pyridine-d5	3.740	84	30637	2.053	ng/ul	0.02
7) Phenol-d5	7.046	99	301063	15.522	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	178036	16.560	ng/ul	0.00
11) 2-Chlorophenol-d4	7.411	132	254623	16.630	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	212396	13.247	ng/ul	0.00
21) Nitrobenzene-d5	9.046	128	112063	16.060	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	112139	15.021	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.310	165	217629	15.760	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	278101	13.210	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	669390	16.990	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	757751	16.871	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	92399	11.325	ng/ul	0.00
60) Fluorene-d10	15.522	176	635143	18.563	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.640	200	67107	9.581	ng/ul	0.00
73) Anthracene-d10	17.386	188	1001435	18.999	ng/ul	0.00
81) Pyrene-d10	19.616	212	1275662	21.229	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	1255150	20.746	ng/ul	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.292	202	108258	1.472	ng/ul	97
82) Pyrene	19.645	202	106884	1.396	ng/ul	99
87) Chrysene	21.410	228	75197	1.033	ng/ul	96
90) Benzo(b)fluoranthene	23.057	252	105339m	1.366	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011935.D
Acq On : 05 Oct 2022 17:56
Operator : CG/JU
Sample : N4819-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Q0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/06/2022
Supervised By :mohammad ahmed 10/10/2022

Quant Time: Oct 05 23:23:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 05 23:18:55 2022
Response via : Initial Calibration

