




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011952.D
 Acq On : 06 Oct 2022 04:14
 Operator : CG/JU
 Sample : N4847-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8S5

Manual IntegrationsAPPROVED

Quant Time: Oct 06 04:56:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/06/2022
 Supervised By :mohammad ahmed 10/10/2022

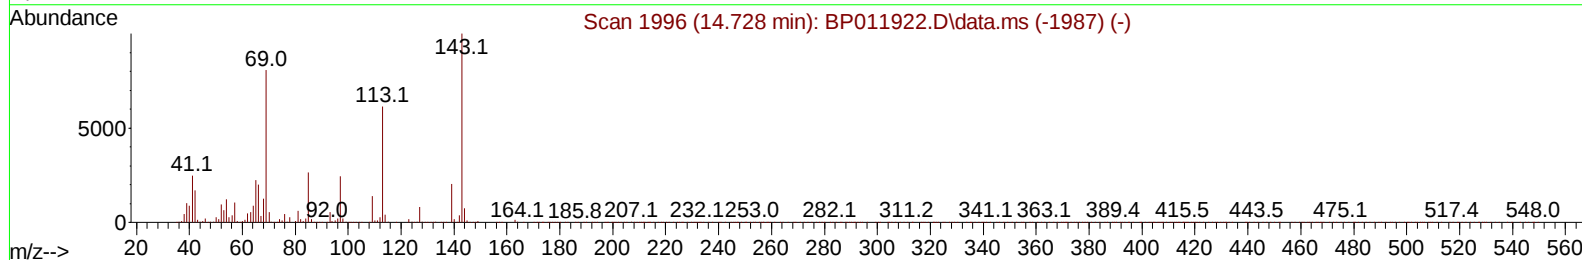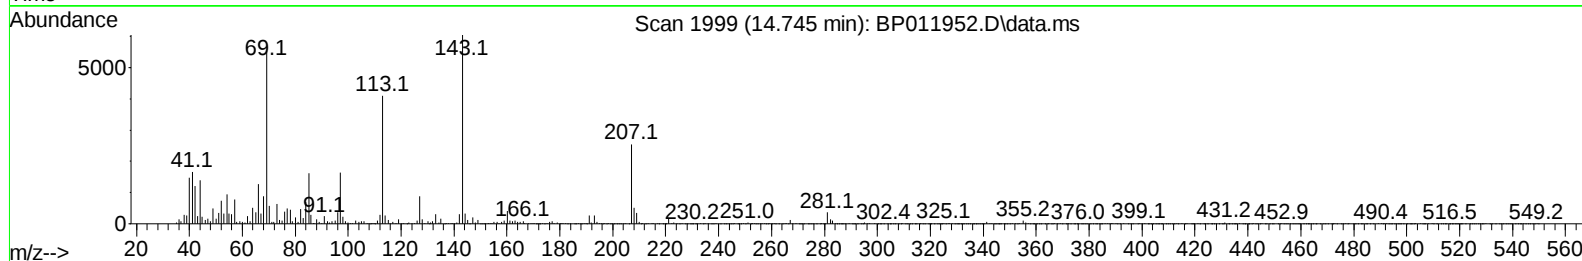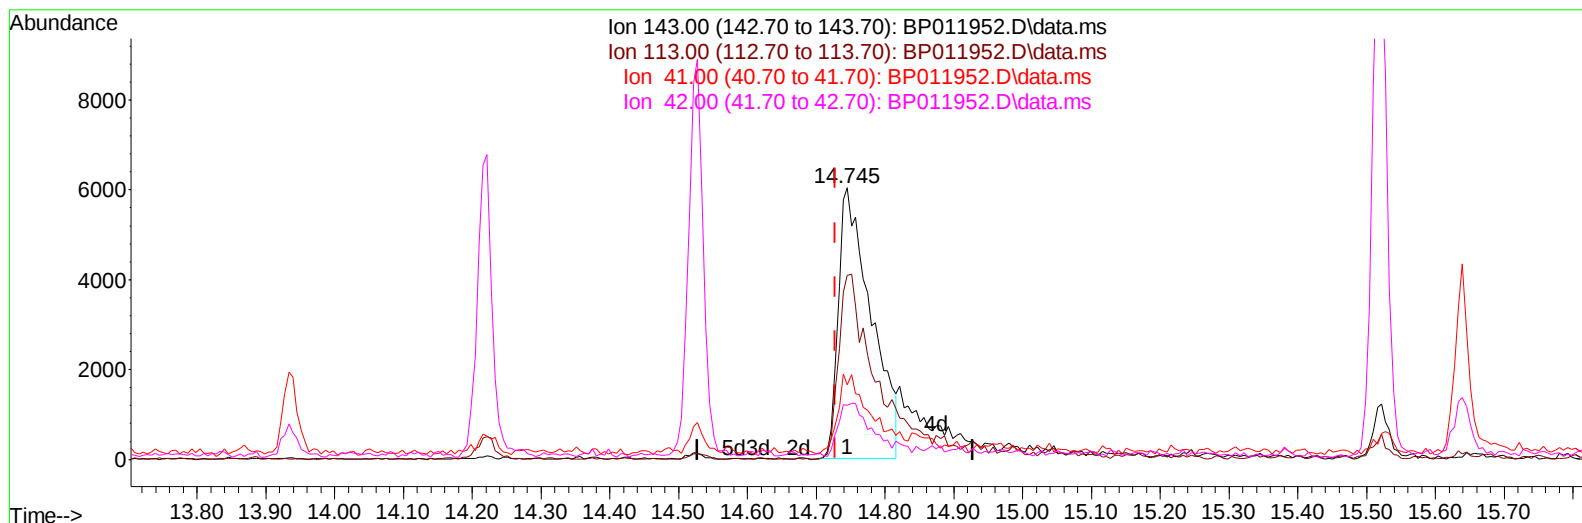

TIC: BP011952.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (+ 0.017) 1.96 ng/ul

response 19989

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.80	67.91
41.00	24.20	27.50
42.00	16.40	19.97#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011952.D
Acq On : 06 Oct 2022 04:14
Operator : CG/JU
Sample : N4847-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8S5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/06/2022
Supervised By :mohammad ahmed 10/10/2022

Quant Time: Oct 06 04:56:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 05 23:18:55 2022
Response via : Initial Calibration

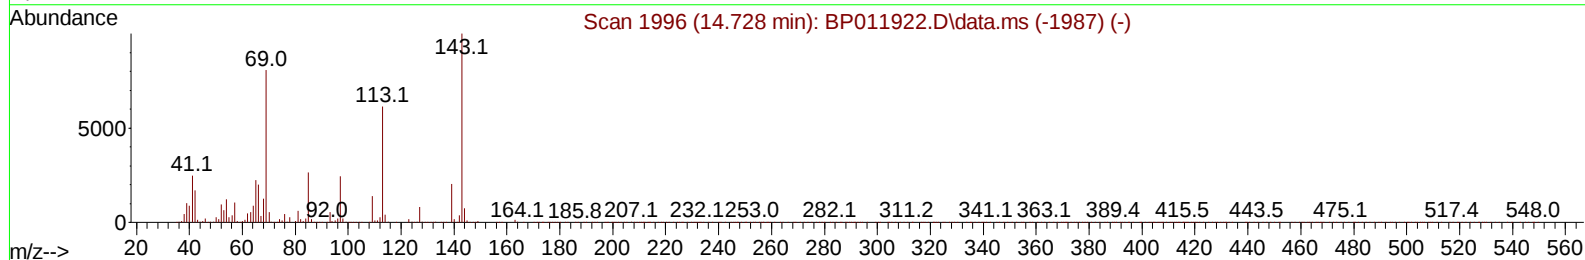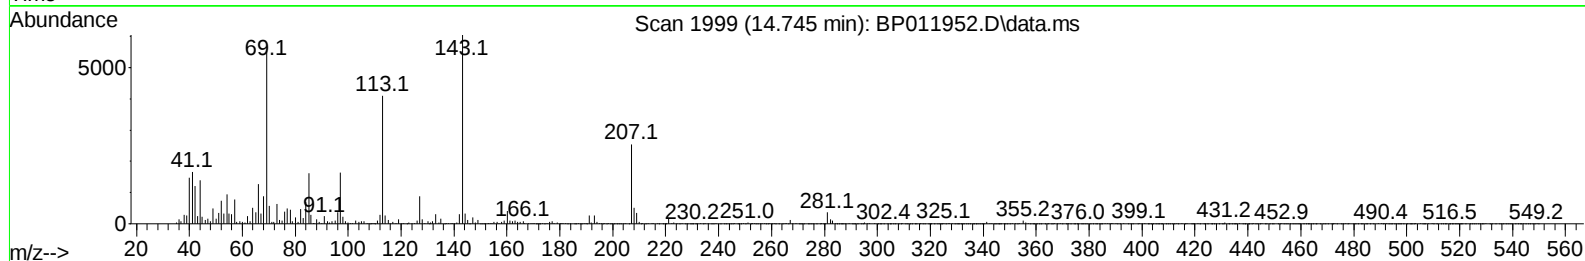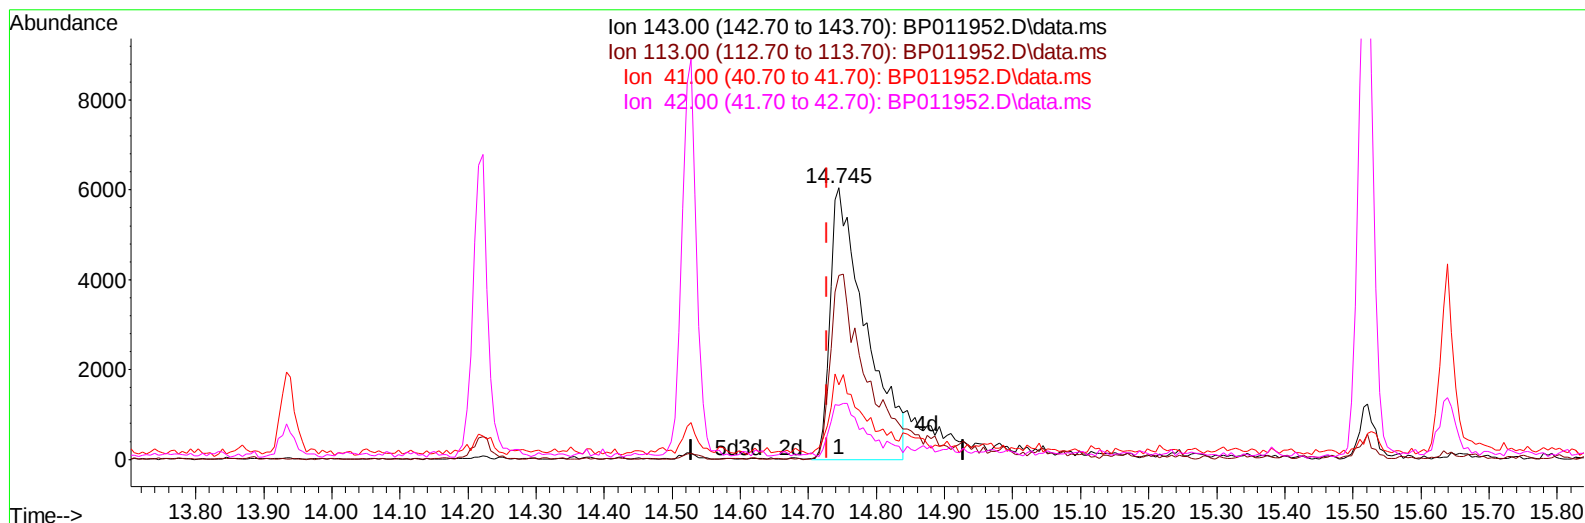

TIC: BP011952.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (+ 0.017) 2.14 ng/ul m

response 21881

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.80	67.91
41.00	24.20	27.50
42.00	16.40	19.97#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011952.D
 Acq On : 06 Oct 2022 04:14
 Operator : CG/JU
 Sample : N4847-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8S5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/06/2022
 Supervised By :mohammad ahmed 10/10/2022

Quant Time: Oct 06 04:56:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	270619	20.000	ng/ul	0.00
20) Naphthalene-d8	10.686	136	1128650	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.527	164	689882	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188	1460186	20.000	ng/ul	0.00
79) Chrysene-d12	21.368	240	1392668	20.000	ng/ul	0.00
88) Perylene-d12	23.798	264	1392135	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	24861	4.052	ng/uL	0.00
4) Pyridine-d5	3.734	84	41839	2.328	ng/ul	0.01
7) Phenol-d5	7.045	99	111300	4.764	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	285208	22.024	ng/ul	0.00
11) 2-Chlorophenol-d4	7.410	132	319621	17.331	ng/ul	0.00
15) 4-Methylphenol-d8	8.587	113	199623	10.336	ng/ul	-0.01
21) Nitrobenzene-d5	9.045	128	190185	22.123	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	146142	15.889	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	323499	19.015	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	501883	19.351	ng/ul	0.00
46) Dimethylphthalate-d6	13.939	166	1180670	23.932	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	1320218	23.474	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	21881m	2.142	ng/ul	0.02
60) Fluorene-d10	15.521	176	1094438	25.545	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	88633	10.029	ng/ul	0.00
73) Anthracene-d10	17.380	188	1919243	28.855	ng/ul	0.00
81) Pyrene-d10	19.615	212	2176793	30.863	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	2053657	29.469	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011952.D
Acq On : 06 Oct 2022 04:14
Operator : CG/JU
Sample : N4847-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8S5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/06/2022
Supervised By :mohammad ahmed 10/10/2022

Quant Time: Oct 06 04:56:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 05 23:18:55 2022
Response via : Initial Calibration

