




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP012019.D
 Acq On : 07 Oct 2022 21:23
 Operator : CG/JU
 Sample : N4951-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8T4

Manual IntegrationsAPPROVED

Quant Time: Oct 07 23:11:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 03:22:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/10/2022
 Supervised By :mohammad ahmed 10/10/2022

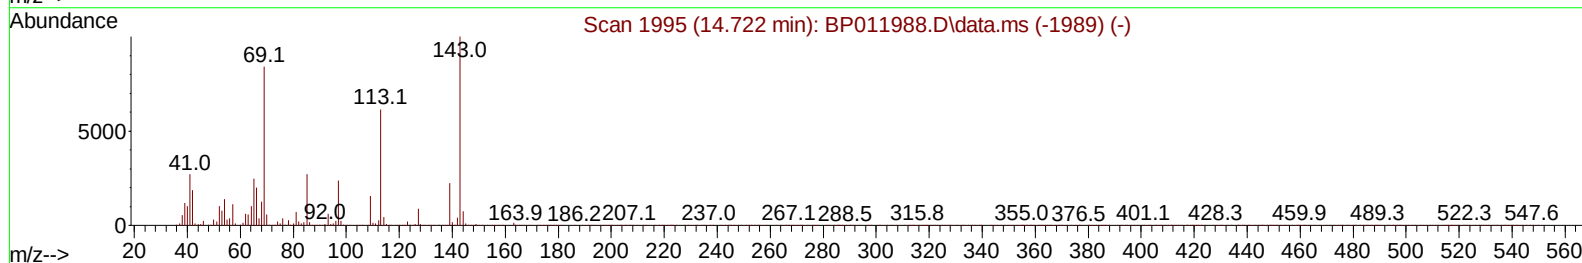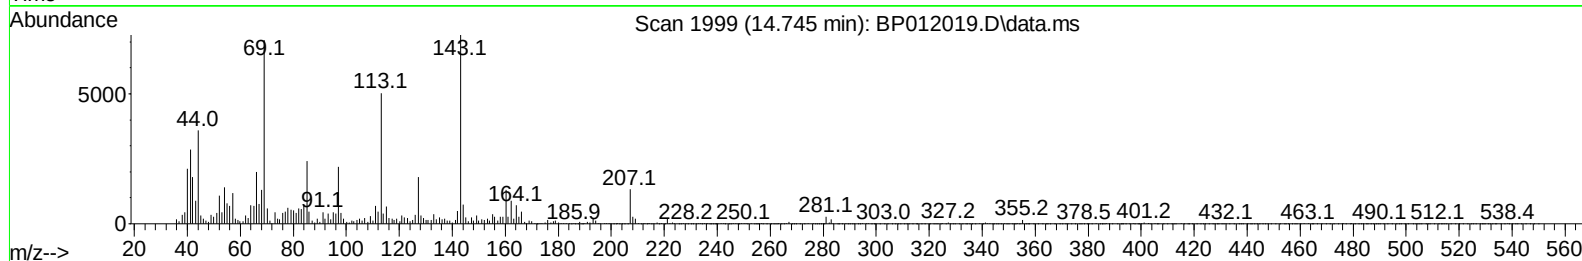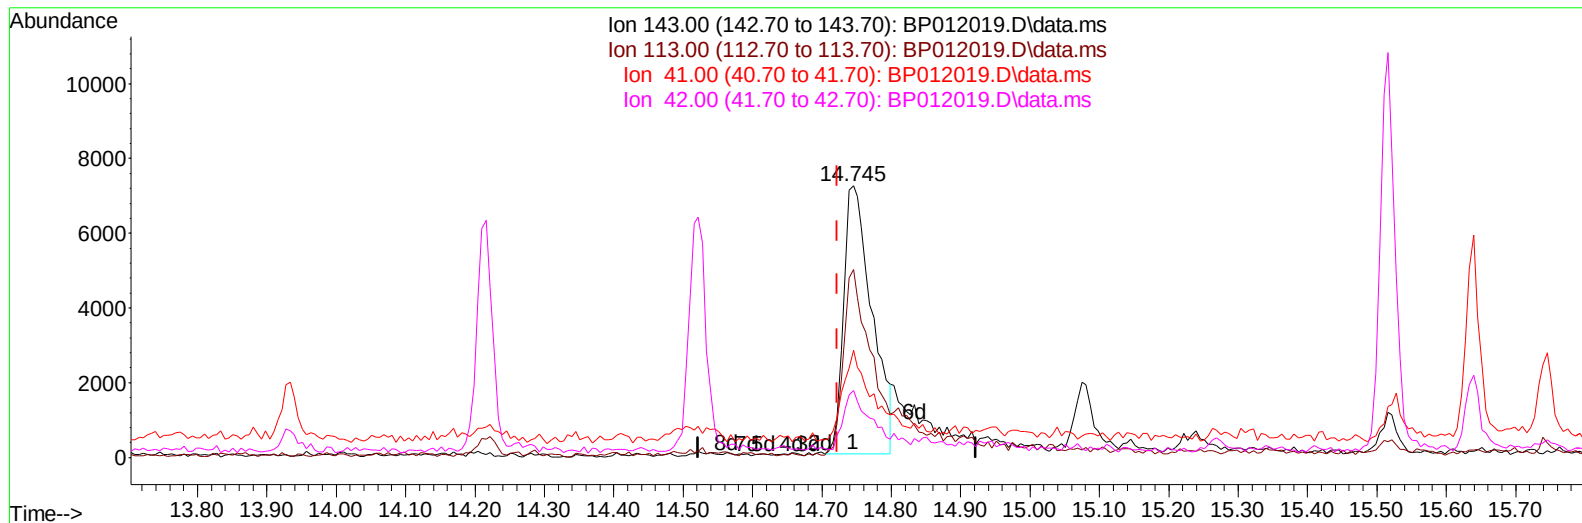

TIC: BP012019.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (+ 0.023) 2.44 ng/ul

response 20397

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.80	69.17
41.00	24.20	39.39#
42.00	16.40	24.66#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP012019.D
 Acq On : 07 Oct 2022 21:23
 Operator : CG/JU
 Sample : N4951-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8T4

Manual IntegrationsAPPROVED

Quant Time: Oct 07 23:11:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 03:22:44 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/10/2022
 Supervised By :mohammad ahmed 10/10/2022

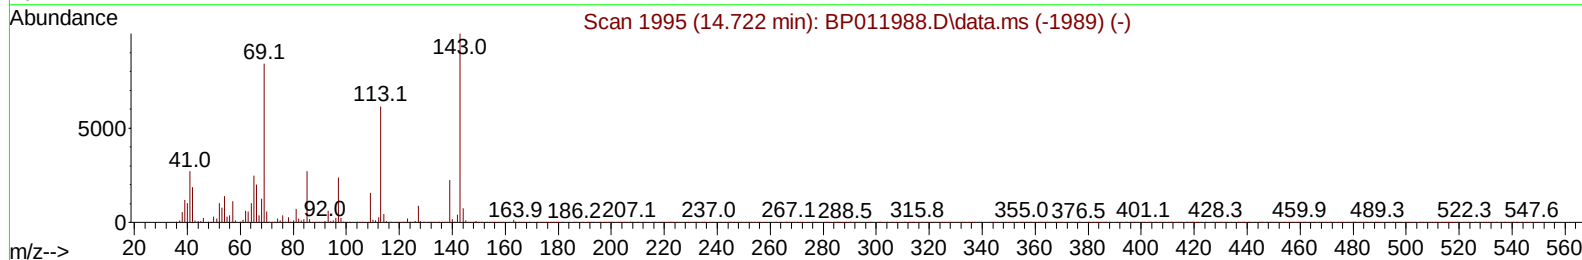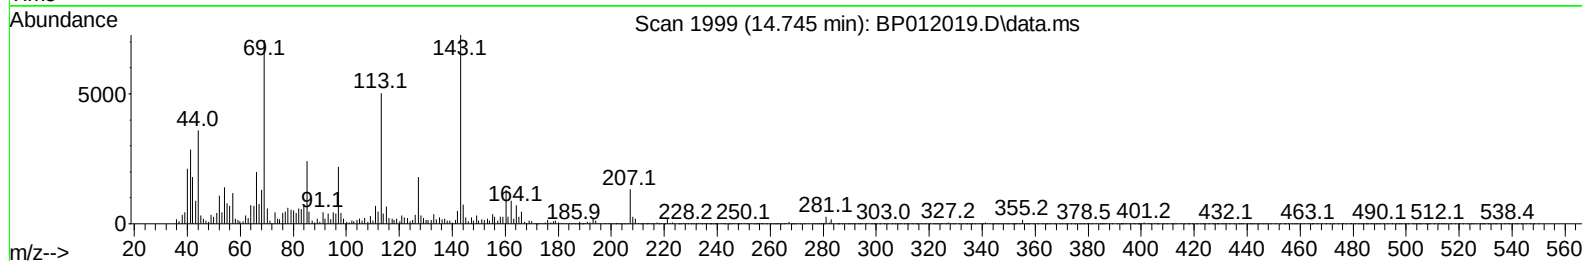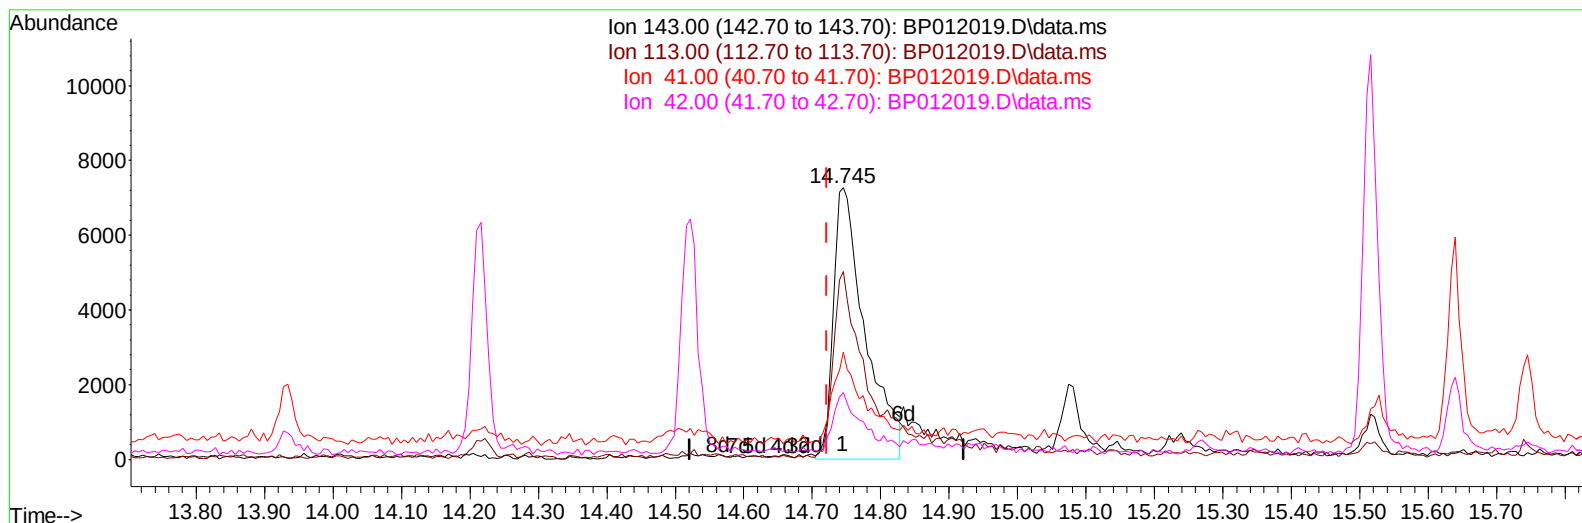

TIC: BP012019.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (+ 0.023) 2.80 ng/ul m

response 23428

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.80	69.17
41.00	24.20	39.39#
42.00	16.40	24.66#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP012019.D
 Acq On : 07 Oct 2022 21:23
 Operator : CG/JU
 Sample : N4951-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8T4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/10/2022
 Supervised By :mohammad ahmed 10/10/2022

Quant Time: Oct 07 23:11:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 03:22:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	229407	20.000	ng/ul	0.00
20) Naphthalene-d8	10.681	136	961280	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	564076	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188	1231498	20.000	ng/ul	0.00
79) Chrysene-d12	21.368	240	1214422	20.000	ng/ul	0.00
88) Perylene-d12	23.798	264	1248178	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	15142	2.911	ng/uL	0.00
4) Pyridine-d5	3.728	84	95096	6.241	ng/ul	0.01
7) Phenol-d5	7.040	99	83983	4.241	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	249326	22.712	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	264454	16.915	ng/ul	0.00
15) 4-Methylphenol-d8	8.587	113	158765	9.698	ng/ul	0.00
21) Nitrobenzene-d5	9.046	128	172211	23.520	ng/ul	0.00
24) 2-Nitrophenol-d4	9.763	143	166942	21.311	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	289880	20.006	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	409630	18.544	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	1047250	25.962	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	1242229	27.014	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	23428m	2.805	ng/ul	0.02
60) Fluorene-d10	15.516	176	976021	27.862	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	115439	15.487	ng/ul	0.00
73) Anthracene-d10	17.380	188	1658546	29.566	ng/ul	0.00
81) Pyrene-d10	19.616	212	1973213	32.083	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	1944602	31.122	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP012019.D
Acq On : 07 Oct 2022 21:23
Operator : CG/JU
Sample : N4951-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8T4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/10/2022
Supervised By :mohammad ahmed 10/10/2022

Quant Time: Oct 07 23:11:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 03:22:44 2022
Response via : Initial Calibration

