

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011967.D
 Acq On : 06 Oct 2022 13:21
 Operator : CG/JU
 Sample : N4956-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8W5

Quant Time: Oct 06 23:05:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	240665	20.000	ng/u1	0.00
20) Naphthalene-d8	10.687	136	970363	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.528	164	567310	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.281	188	1213898	20.000	ng/u1	0.00
79) Chrysene-d12	21.369	240	1293209	20.000	ng/u1	0.00
88) Perylene-d12	23.798	264	1353553	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	22541	4.131	ng/uL	0.00
4) Pyridine-d5	3.723	84	134739	8.430	ng/u1	0.00
7) Phenol-d5	7.046	99	112682	5.424	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	314185	27.282	ng/u1	0.00
11) 2-Chlorophenol-d4	7.411	132	361722	22.055	ng/u1	0.00
15) 4-Methylphenol-d8	8.593	113	209219	12.182	ng/u1	0.00
21) Nitrobenzene-d5	9.046	128	226760	30.680	ng/u1	0.00
24) 2-Nitrophenol-d4	9.769	143	230498	29.149	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.310	165	388539	26.564	ng/u1	0.00
31) 4-Chloroaniline-d4	10.828	131	467745	20.977	ng/u1	0.00
46) Dimethylphthalate-d6	13.940	166	1306021	32.193	ng/u1	0.00
49) Acenaphthylene-d8	14.222	160	1461300	31.597	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	37851	4.506	ng/u1	0.01
60) Fluorene-d10	15.522	176	1175378	33.361	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.640	200	194860	26.521	ng/u1	0.00
73) Anthracene-d10	17.381	188	1992176	36.028	ng/u1	0.00
81) Pyrene-d10	19.616	212	2465386	37.643	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.645	264	2540071	37.488	ng/u1	0.00
Target Compounds						
59) Diethylphthalate	15.351	149	85772	2.014	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011967.D
Acq On : 06 Oct 2022 13:21
Operator : CG/JU
Sample : N4956-13
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8W5

Quant Time: Oct 06 23:05:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 05 23:18:55 2022
Response via : Initial Calibration

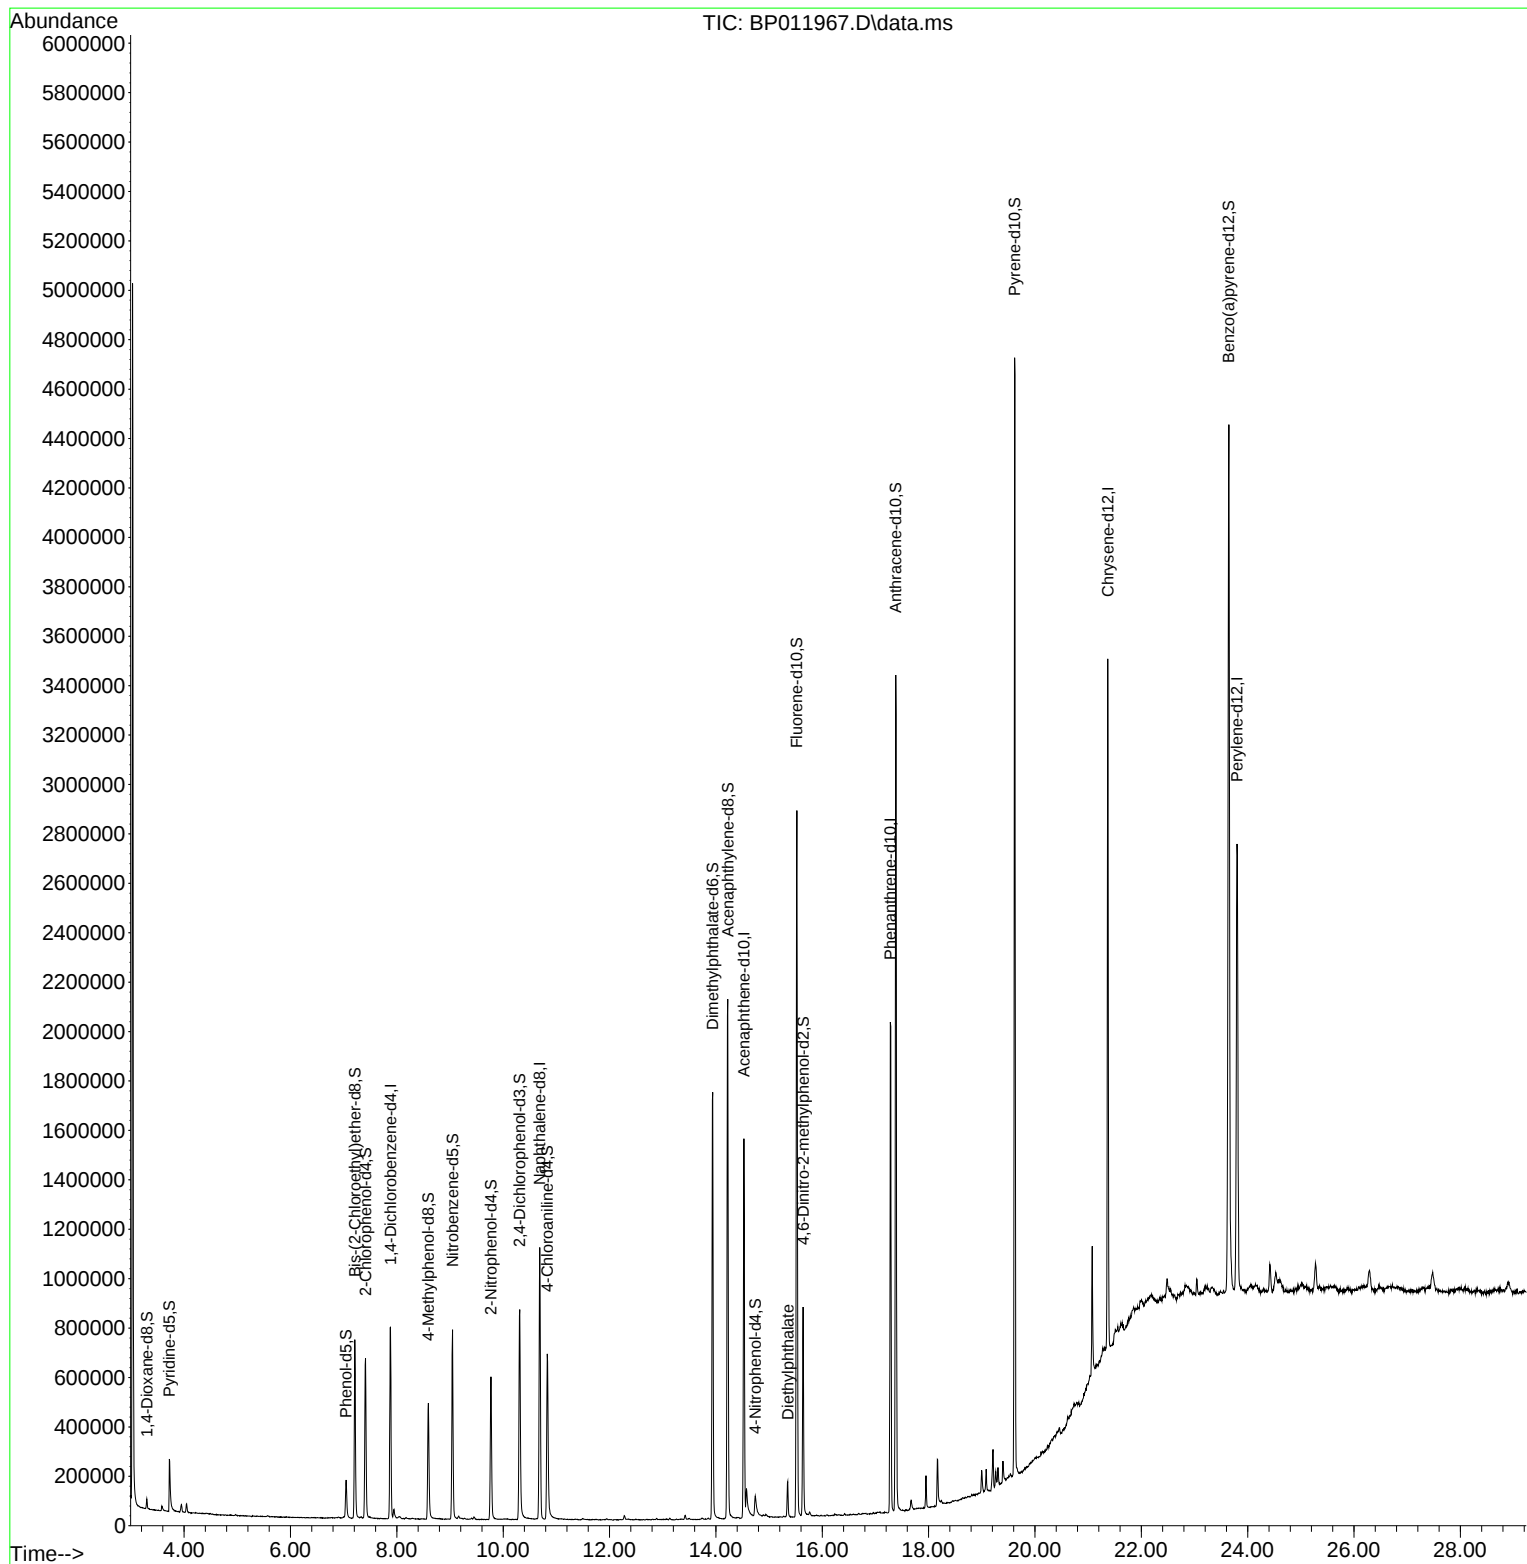

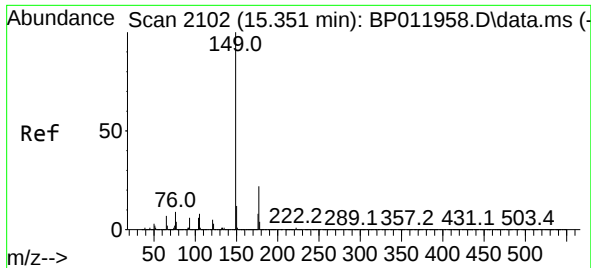

#59
 Diethylphthalate
 Concen: 2.014 ng/ul
 RT: 15.351 min Scan# 2102
 Delta R.T. 0.000 min
 Lab File: BP011967.D
 Acq: 06 Oct 2022 13:21

Instrument :
 BNA_P
 ClientSampleId :
 CB8W5

Tgt Ion:	149	Resp:	85772
Ion	Ratio	Lower	Upper
149	100		
177	22.5	17.8	26.8
150	12.2	9.9	14.9

