

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011976.D
 Acq On : 06 Oct 2022 18:34
 Operator : CG/JU
 Sample : N4923-13
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10055

Quant Time: Oct 06 23:08:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 05 23:18:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	259880	20.000	ng/u1	0.00
20) Naphthalene-d8	10.687	136	1034470	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.522	164	579089	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.281	188	1204220	20.000	ng/u1	0.00
79) Chrysene-d12	21.369	240	1259560	20.000	ng/u1	0.00
88) Perylene-d12	23.798	264	1317063	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	26029	4.417	ng/uL	0.00
4) Pyridine-d5	3.740	84	96920	5.615	ng/u1	0.02
7) Phenol-d5	7.046	99	112178	5.000	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	329520	26.498	ng/u1	0.00
11) 2-Chlorophenol-d4	7.411	132	357345	20.177	ng/u1	0.00
15) 4-Methylphenol-d8	8.593	113	203836	10.991	ng/u1	0.00
21) Nitrobenzene-d5	9.046	128	223808	28.404	ng/u1	0.00
24) 2-Nitrophenol-d4	9.769	143	222337	26.374	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.305	165	359570	23.060	ng/u1	0.00
31) 4-Chloroaniline-d4	10.828	131	485138	20.408	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	1233395	29.784	ng/u1	0.00
49) Acenaphthylene-d8	14.216	160	1382722	29.290	ng/u1	0.00
54) 4-Nitrophenol-d4	14.746	143	30604	3.569	ng/u1	0.02
60) Fluorene-d10	15.522	176	1111899	30.918	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.640	200	155915	21.391	ng/u1	0.00
73) Anthracene-d10	17.381	188	1826800	33.303	ng/u1	0.00
81) Pyrene-d10	19.616	212	2209274	34.634	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.639	264	2286255	34.677	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.734	128	74407	1.339	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011976.D
Acq On : 06 Oct 2022 18:34
Operator : CG/JU
Sample : N4923-13
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10055

Quant Time: Oct 06 23:08:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 05 23:18:55 2022
Response via : Initial Calibration

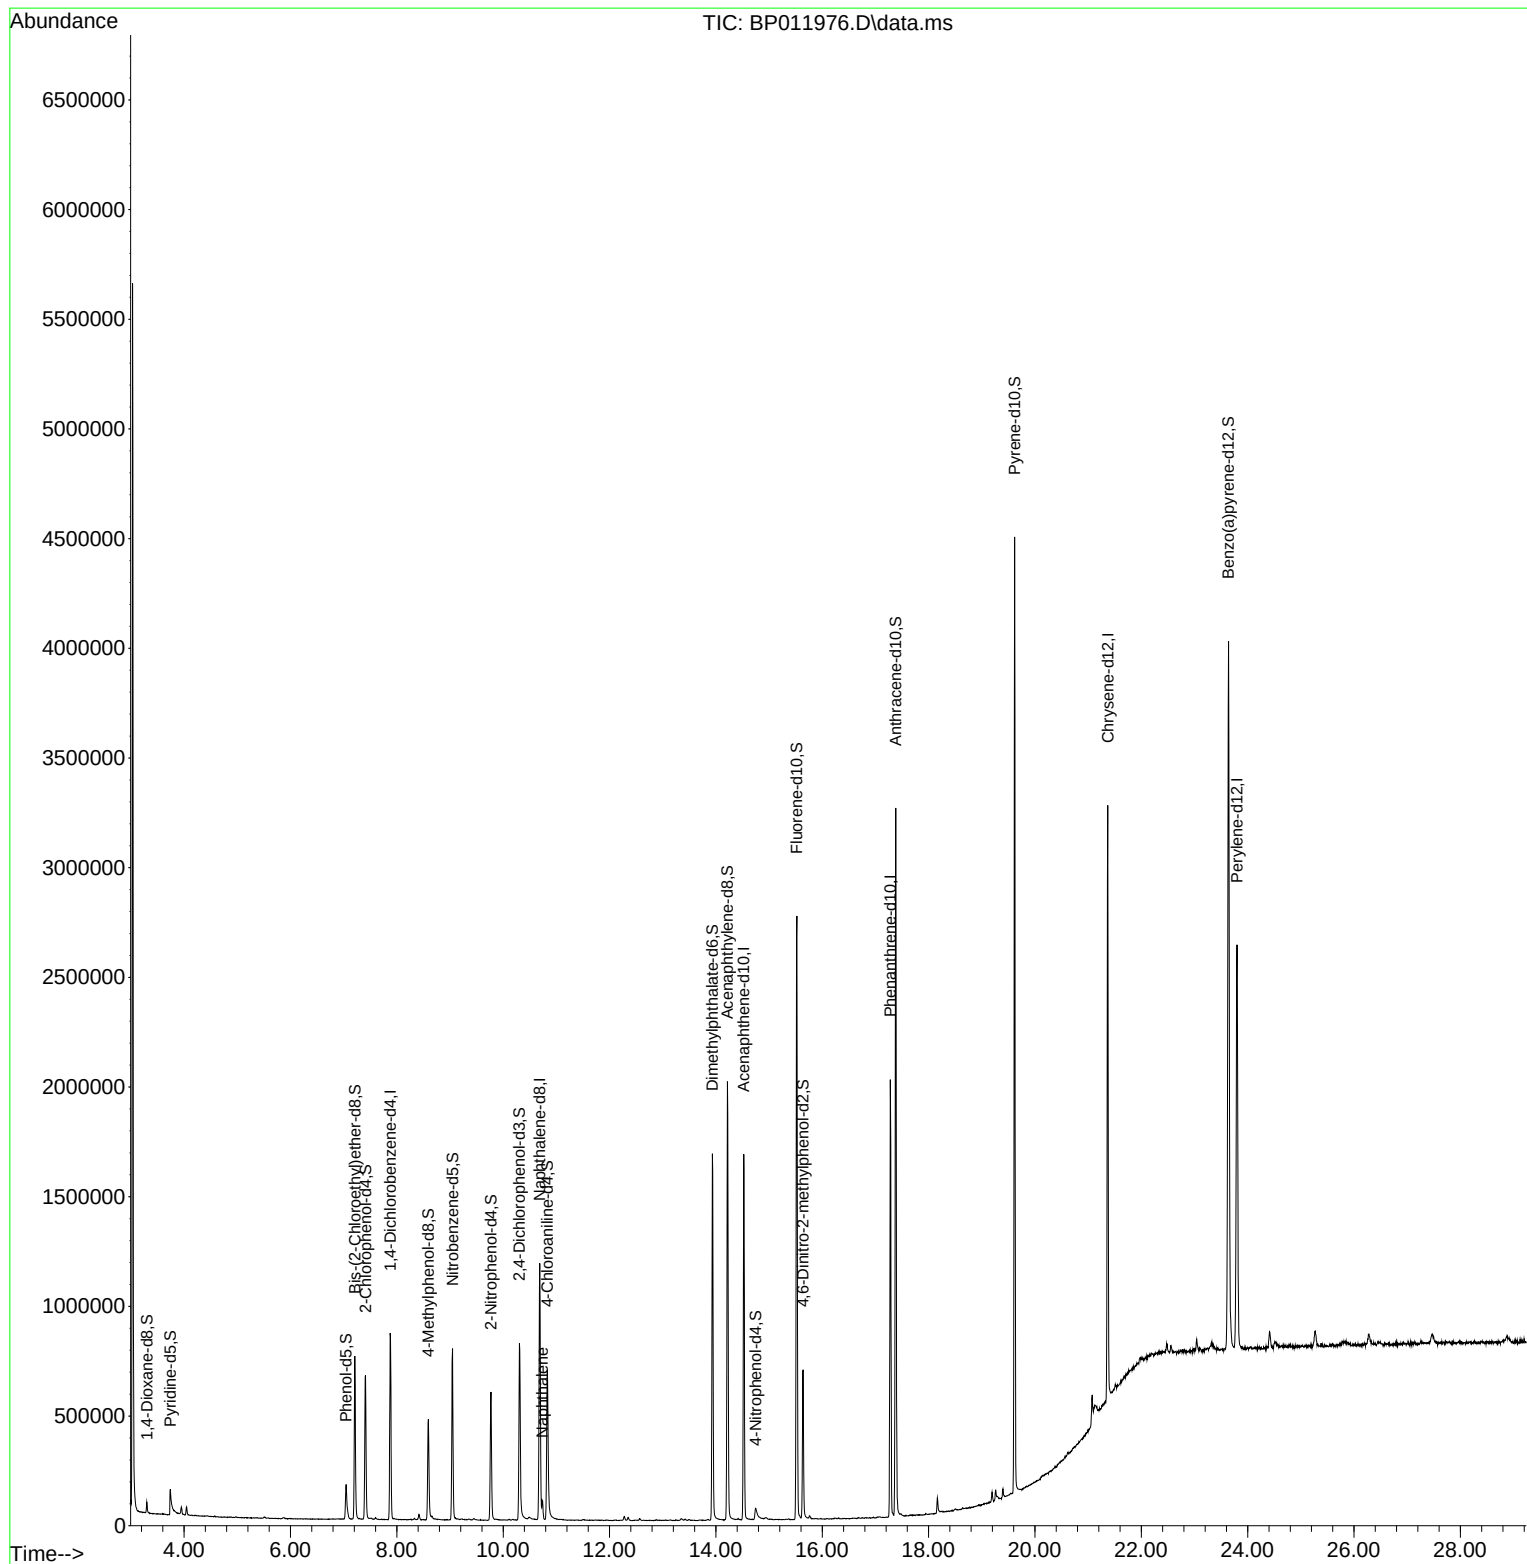

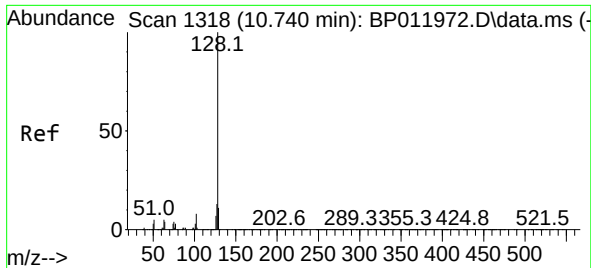

#30

Naphthalene

Concen: 1.339 ng/ul

RT: 10.734 min Scan# 11

Delta R.T. -0.012 min

Lab File: BP011976.D


Acq: 06 Oct 2022 18:34

Instrument :

BNA_P

ClientSampleId :

E10055

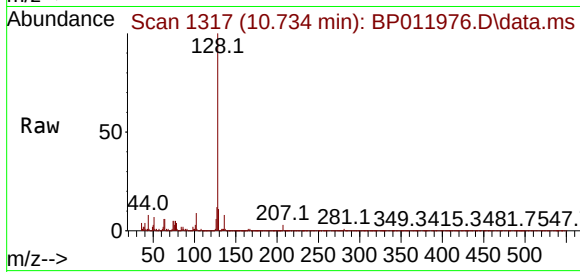

Tgt Ion:128 Resp: 74407

Ion Ratio Lower Upper

128 100

129 11.2 8.9 13.3

127 12.0 10.5 15.7

