

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011925.D
 Acq On : 05 Oct 2022 12:13
 Operator : CG/JU
 Sample : N4890-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0D9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	33	rVB	5516867	7078644	88.58%	10.468%
2	3.299	50	53	58	rVB	48918	57447	0.72%	0.085%
3	3.728	123	126	144	rBV	195183	305873	3.83%	0.452%
4	3.952	159	164	175	rVB	32827	55212	0.69%	0.082%
5	4.046	177	180	188	rVB	17734	23237	0.29%	0.034%
6	4.581	267	271	277	rBV3	13270	17808	0.22%	0.026%
7	7.046	684	690	702	rVB	199995	344407	4.31%	0.509%
8	7.211	712	718	733	rBV	796746	1315052	16.46%	1.945%
9	7.411	744	752	765	rBV	772580	1288946	16.13%	1.906%
10	7.881	823	832	842	rBV	790609	1298410	16.25%	1.920%
11	7.952	842	844	853	rVB10	5936	9614	0.12%	0.014%
12	8.593	945	953	972	rBV	608671	1025965	12.84%	1.517%
13	9.052	1023	1031	1045	rBV	825055	1434884	17.95%	2.122%
14	9.458	1094	1100	1105	rBV2	12892	22162	0.28%	0.033%
15	9.769	1146	1153	1164	rBV	623523	1091610	13.66%	1.614%
16	10.310	1237	1245	1269	rBV	1026280	1831592	22.92%	2.709%
17	10.493	1271	1276	1282	rBV6	9126	23914	0.30%	0.035%
18	10.693	1302	1310	1324	rVB	1092692	1846845	23.11%	2.731%
19	10.834	1326	1334	1351	rBV	843649	1575543	19.71%	2.330%
20	11.957	1517	1525	1530	rVB2	11667	19542	0.24%	0.029%
21	12.287	1574	1581	1587	rBV	18940	35073	0.44%	0.052%
22	13.146	1719	1727	1730	rBV8	4415	9058	0.11%	0.013%
23	13.428	1769	1775	1780	rVV6	8837	15409	0.19%	0.023%
24	13.504	1782	1788	1792	rVB5	4332	8084	0.10%	0.012%
25	13.940	1855	1862	1878	rBV	1959713	2786081	34.86%	4.120%
26	14.222	1898	1910	1929	rBV	2362807	3608276	45.15%	5.336%
27	14.528	1955	1962	1976	rVV	1582647	2369592	29.65%	3.504%
28	14.740	1992	1998	2018	rBV	83906	246075	3.08%	0.364%
29	14.946	2028	2033	2041	rVV	6840	17776	0.22%	0.026%
30	15.034	2045	2048	2057	rVB	3548	8724	0.11%	0.013%
31	15.522	2122	2131	2145	rBV	3242262	4754617	59.50%	7.031%
32	15.640	2145	2151	2166	rVV	881334	1232771	15.43%	1.823%
33	15.763	2168	2172	2180	rVB5	16036	29947	0.37%	0.044%
34	16.310	2261	2265	2271	rBV8	5589	9133	0.11%	0.014%
35	17.287	2424	2431	2441	rBV	2071634	2933002	36.70%	4.337%
36	17.387	2441	2448	2468	rVV	3784891	5482756	68.61%	8.108%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011925.D
 Acq On : 05 Oct 2022 12:13
 Operator : CG/JU
 Sample : N4890-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0D9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	18.169	2577	2581	2586	rBV2	82418	125575	1.57%	0.186%
38	19.198	2752	2756	2760	rBV2	49987	68123	0.85%	0.101%
39	19.263	2764	2767	2774	rVV	55484	82753	1.04%	0.122%
40	19.398	2787	2790	2797	rBV	69309	96691	1.21%	0.143%
41	19.622	2822	2828	2834	rBV	5314666	7120359	89.10%	10.530%
42	21.075	3073	3075	3081	rBV2	121212	158373	1.98%	0.234%
43	21.369	3121	3125	3136	rBV	2847115	3780840	47.31%	5.591%
44	23.645	3505	3512	3527	rVB2	3814464	7991609	100.00%	11.818%
45	23.804	3533	3539	3552	rVB2	1988405	3983114	49.84%	5.890%




Sum of corrected areas: 67620518

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011925.D
Acq On : 05 Oct 2022 12:13
Operator : CG/JU
Sample : N4890-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0D9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

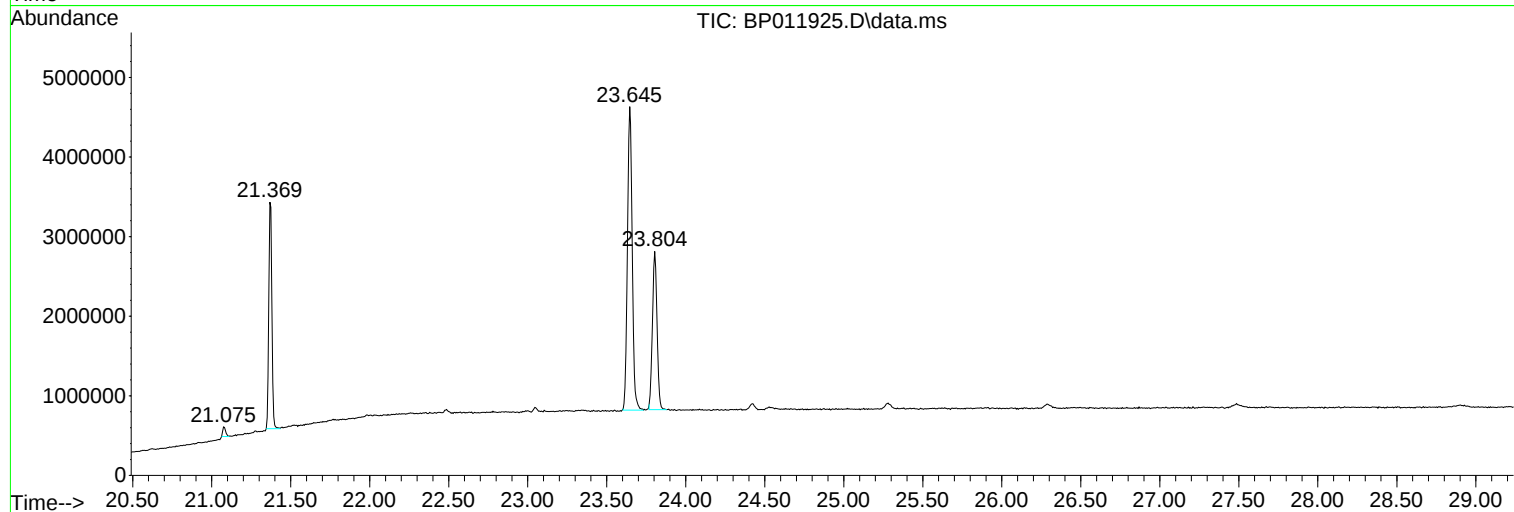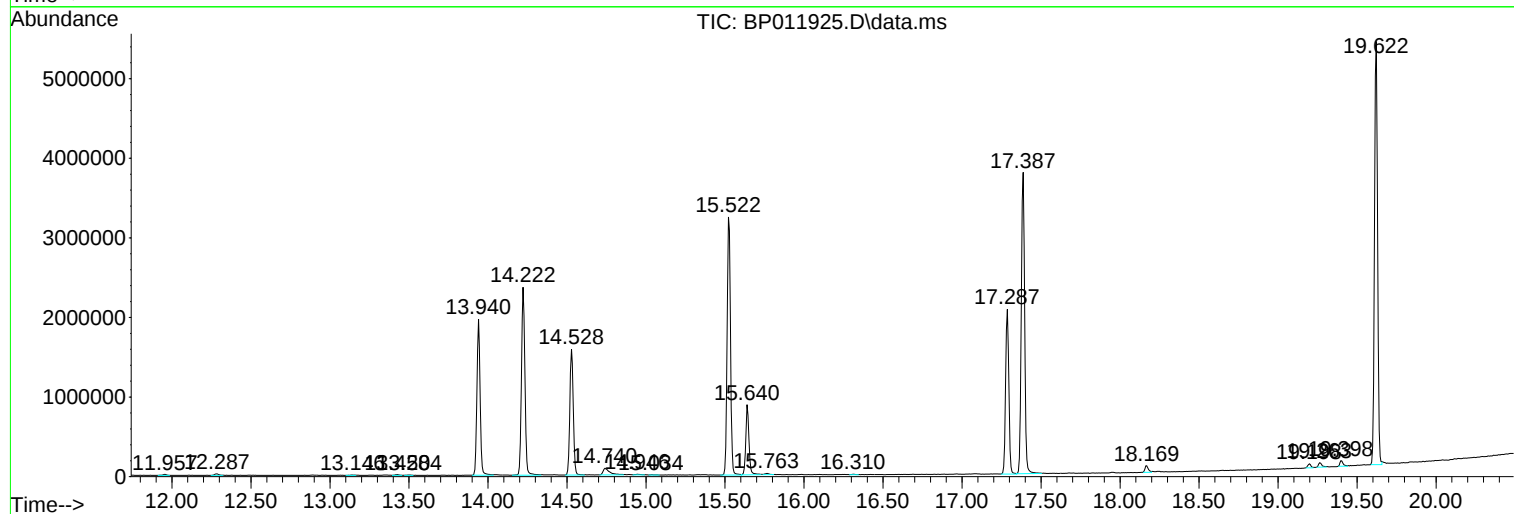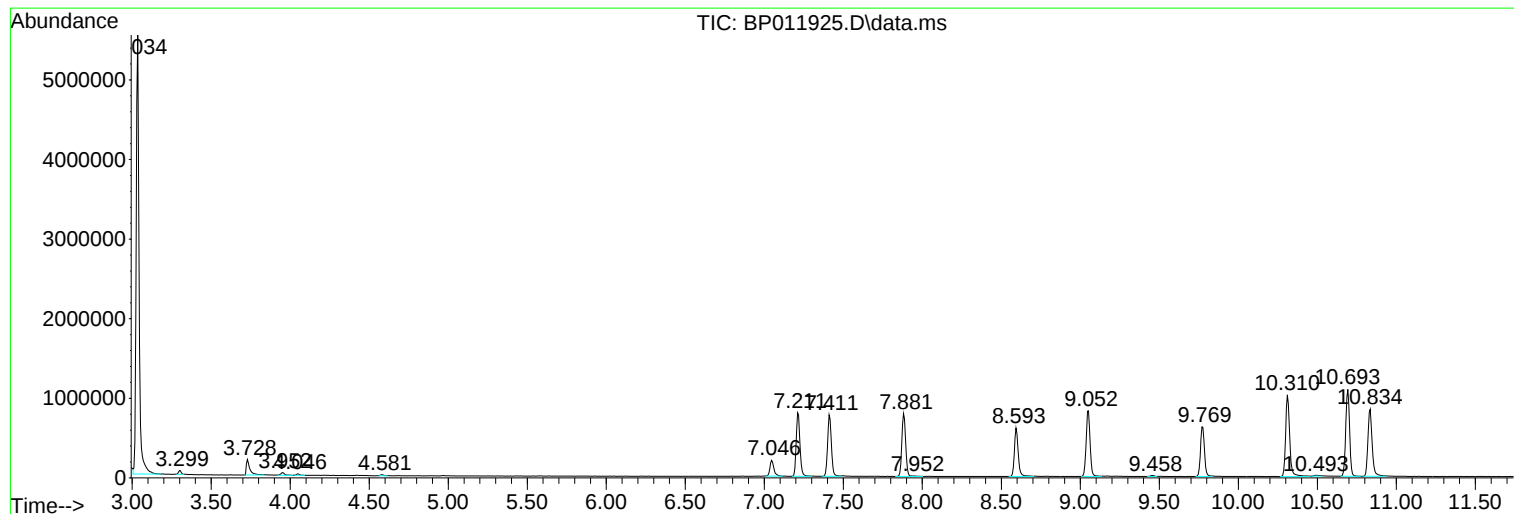

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011925.D
Acq On : 05 Oct 2022 12:13
Operator : CG/JU
Sample : N4890-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0D9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	109.04 ng/ul	7078640	1,4-Dichlorobenzene-d4	7.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

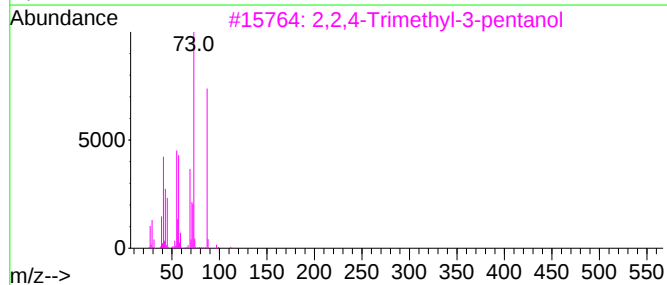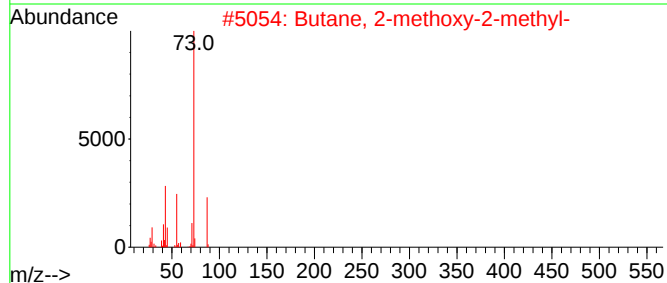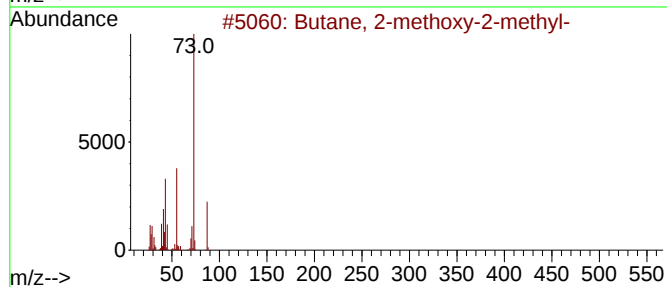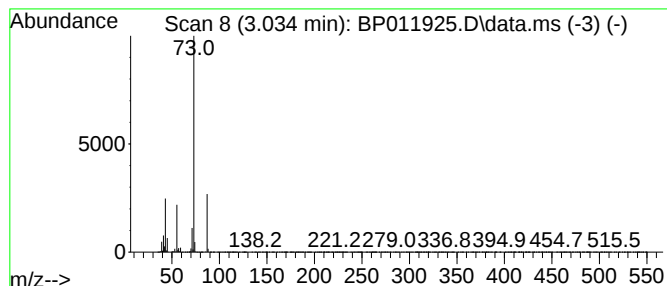

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011925.D
Acq On : 05 Oct 2022 12:13
Operator : CG/JU
Sample : N4890-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0D9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	109.0	ng/ul	7078640	1	7.881	1298410	20.0