

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011932.D
 Acq On : 05 Oct 2022 16:13
 Operator : CG/JU
 Sample : N4890-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0E0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	28	rVB	5097363	6655970	95.50%	10.705%
2	3.299	49	53	59	rBV	48320	59128	0.85%	0.095%
3	3.734	125	127	134	rBV	60425	93993	1.35%	0.151%
4	3.952	159	164	170	rVB	32238	48235	0.69%	0.078%
5	4.046	177	180	188	rVB	16637	23203	0.33%	0.037%
6	7.046	684	690	705	rVB	184137	328381	4.71%	0.528%
7	7.210	712	718	734	rBV	751550	1248848	17.92%	2.009%
8	7.410	745	752	764	rBV	725200	1179751	16.93%	1.897%
9	7.499	764	767	772	rVB7	5310	7586	0.11%	0.012%
10	7.881	825	832	840	rBV	753457	1196253	17.16%	1.924%
11	7.946	840	843	849	rVB6	4305	7842	0.11%	0.013%
12	8.593	944	953	972	rBV	557238	957875	13.74%	1.541%
13	9.046	1022	1030	1045	rBV	798472	1379545	19.79%	2.219%
14	9.457	1093	1100	1106	rVB	12341	20304	0.29%	0.033%
15	9.769	1144	1153	1173	rBV	586312	1045291	15.00%	1.681%
16	10.310	1237	1245	1264	rBV	948274	1695609	24.33%	2.727%
17	10.504	1274	1278	1291	rVB10	7186	23013	0.33%	0.037%
18	10.693	1302	1310	1323	rBV	1009541	1742605	25.00%	2.803%
19	10.834	1327	1334	1348	rBV	370616	705050	10.12%	1.134%
20	11.951	1517	1524	1531	rBV2	18597	32090	0.46%	0.052%
21	12.281	1574	1580	1589	rBV2	19741	39142	0.56%	0.063%
22	13.139	1721	1726	1731	rBV6	4443	9671	0.14%	0.016%
23	13.422	1768	1774	1780	rVV2	24506	40945	0.59%	0.066%
24	13.492	1784	1786	1793	rVB8	4246	7518	0.11%	0.012%
25	13.939	1853	1862	1878	rBV	1977154	2753670	39.51%	4.429%
26	14.222	1896	1910	1927	rBV	2347448	3486287	50.02%	5.607%
27	14.528	1955	1962	1977	rBV	1588109	2304298	33.06%	3.706%
28	14.739	1992	1998	2014	rBV2	76505	218216	3.13%	0.351%
29	14.957	2029	2035	2040	rVB10	6069	13523	0.19%	0.022%
30	15.522	2124	2131	2145	rBV	3287092	4693767	67.34%	7.549%
31	15.639	2145	2151	2165	rVV	859075	1225708	17.59%	1.971%
32	15.763	2168	2172	2182	rVB3	17104	34411	0.49%	0.055%
33	16.304	2261	2264	2271	rVB8	4972	8518	0.12%	0.014%
34	16.957	2372	2375	2383	rBV10	4214	8885	0.13%	0.014%
35	17.286	2424	2431	2441	rBV	1941534	2765008	39.67%	4.447%
36	17.386	2441	2448	2461	rBV	3920864	5587115	80.16%	8.986%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011932.D
 Acq On : 05 Oct 2022 16:13
 Operator : CG/JU
 Sample : N4890-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0E0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	17.951	2542	2544	2549	rVB4	9024	9698	0.14%	0.016%
38	18.163	2576	2580	2589	rBV	74401	134694	1.93%	0.217%
39	19.198	2752	2756	2762	rVB2	49653	65414	0.94%	0.105%
40	19.263	2763	2767	2771	rBV	57042	81230	1.17%	0.131%
41	19.398	2787	2790	2797	rBV3	50304	81283	1.17%	0.131%
42	19.616	2822	2827	2840	rBV	4951042	6739622	96.70%	10.840%
43	21.368	3120	3125	3135	rBV	2544573	3262524	46.81%	5.247%
44	23.639	3505	3511	3527	rVB2	3415413	6969929	100.00%	11.210%
45	23.804	3533	3539	3549	rVB2	1541480	3184716	45.69%	5.122%




Sum of corrected areas: 62176364

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011932.D
Acq On : 05 Oct 2022 16:13
Operator : CG/JU
Sample : N4890-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0E0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

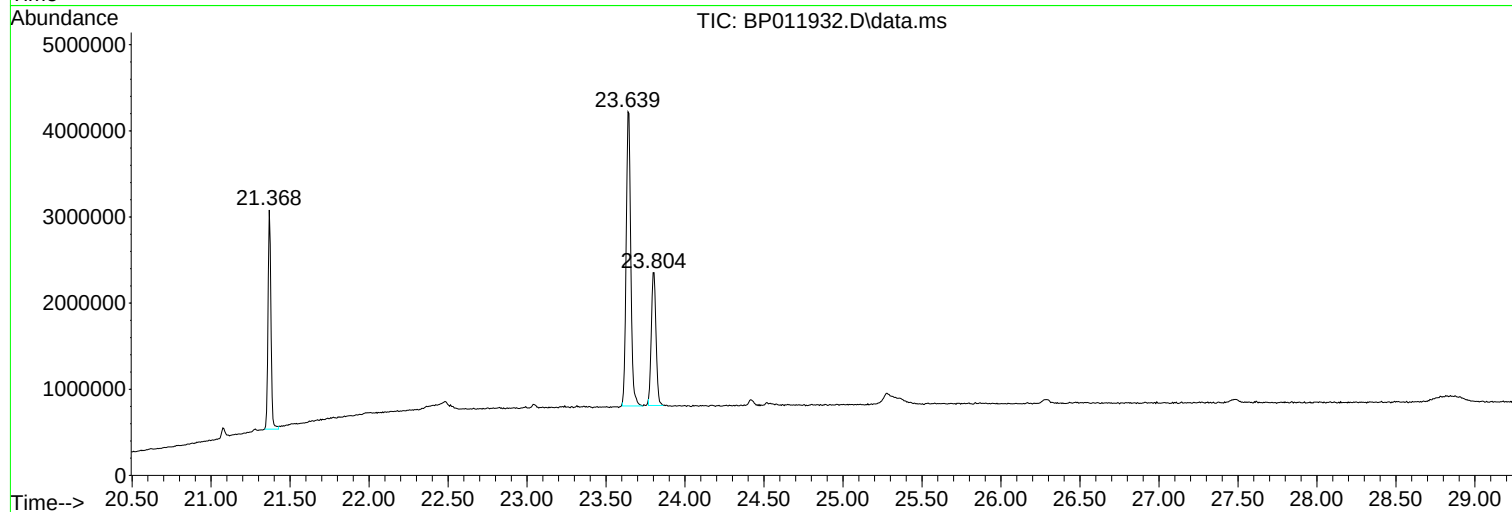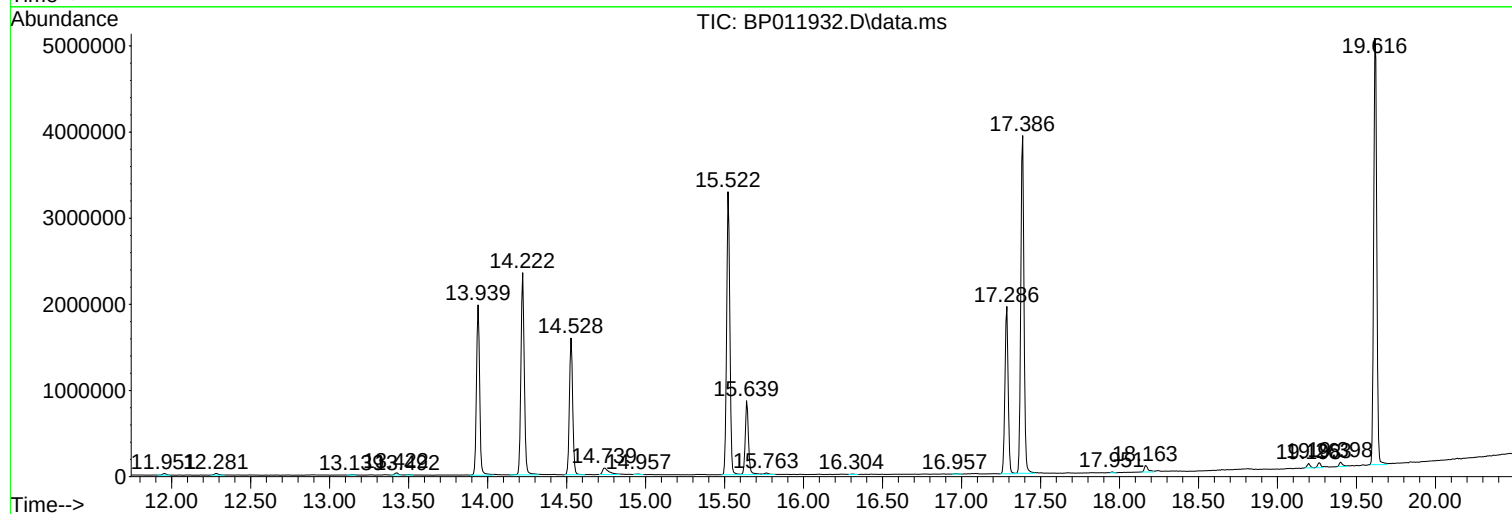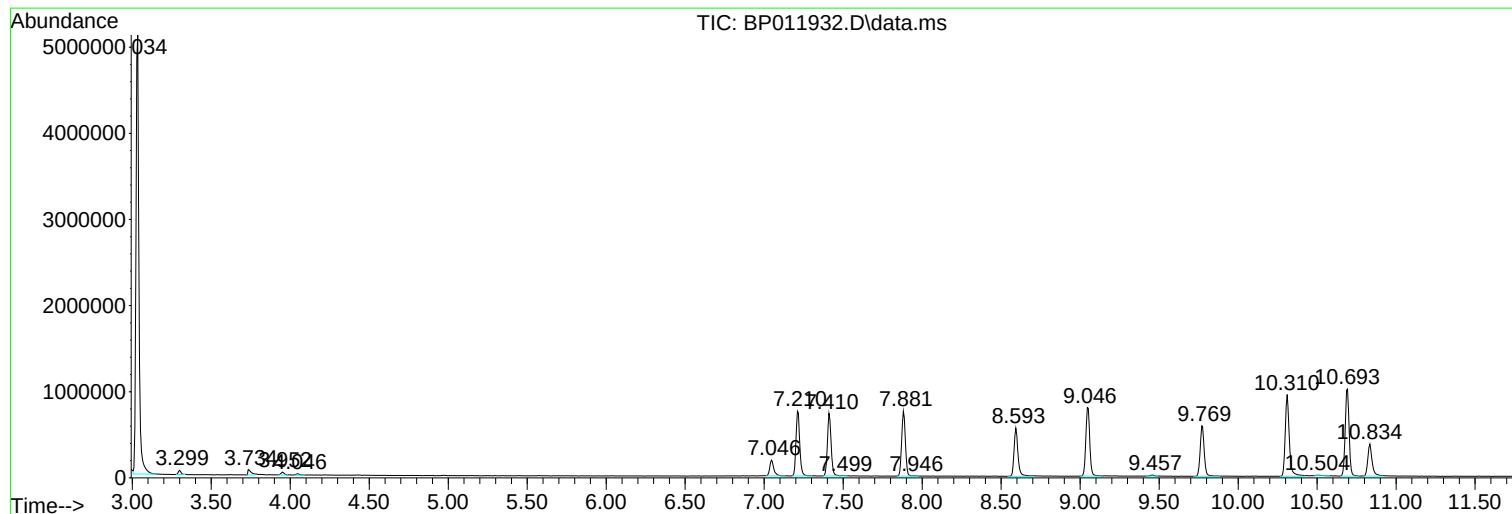

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011932.D
Acq On : 05 Oct 2022 16:13
Operator : CG/JU
Sample : N4890-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0E0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	111.28 ng/ul	6655970	1,4-Dichlorobenzene-d4	7.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
4	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		
5	N-Ethylformamide	73	C3H7NO	000627-45-2	9		

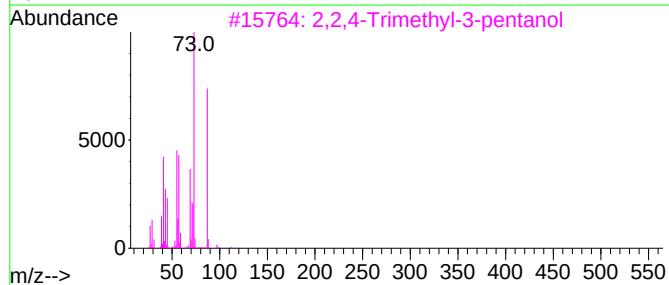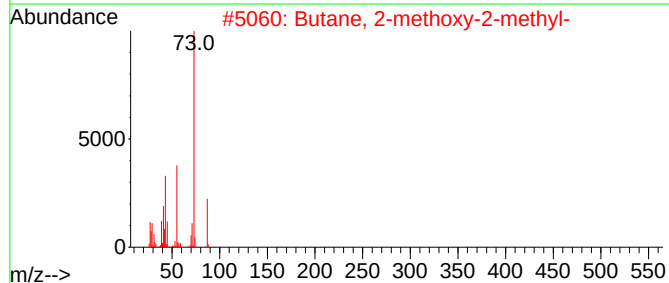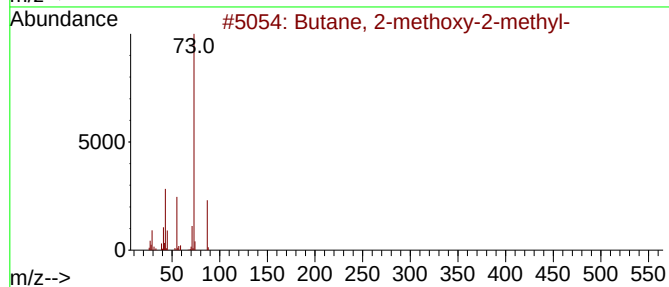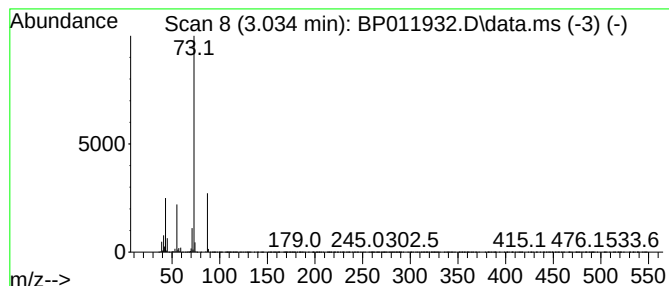

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011932.D
Acq On : 05 Oct 2022 16:13
Operator : CG/JU
Sample : N4890-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0E0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	111.3	ng/ul	6655970	1	7.881	1196250	20.0