

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011933.D
 Acq On : 05 Oct 2022 16:47
 Operator : CG/JU
 Sample : N4890-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY0E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	27	rVB	5115457	6570383	93.16%	10.332%
2	3.270	43	48	51	rBV	222079	272933	3.87%	0.429%
3	3.299	51	53	58	rVB	58147	62082	0.88%	0.098%
4	3.728	124	126	139	rBV	144976	239487	3.40%	0.377%
5	3.952	159	164	173	rVB	30915	52259	0.74%	0.082%
6	4.046	176	180	187	rVB	19249	27044	0.38%	0.043%
7	7.046	684	690	702	rVB	173300	299909	4.25%	0.472%
8	7.211	712	718	731	rBV	812082	1329666	18.85%	2.091%
9	7.411	745	752	764	rBV	755624	1228070	17.41%	1.931%
10	7.881	825	832	843	rBV	850433	1361684	19.31%	2.141%
11	8.593	944	953	966	rBV	542120	931356	13.21%	1.465%
12	9.046	1020	1030	1047	rBV	849991	1446004	20.50%	2.274%
13	9.458	1090	1100	1104	rBV6	6706	14179	0.20%	0.022%
14	9.769	1145	1153	1168	rBV	621786	1068593	15.15%	1.680%
15	10.310	1237	1245	1262	rBV	919632	1693973	24.02%	2.664%
16	10.687	1302	1309	1323	rBV	1104309	1944495	27.57%	3.058%
17	10.834	1325	1334	1361	rBV	750133	1479567	20.98%	2.327%
18	12.281	1571	1580	1590	rBV2	17458	39749	0.56%	0.063%
19	13.422	1769	1774	1782	rVB3	9643	18219	0.26%	0.029%
20	13.499	1782	1787	1793	rBV8	4798	11081	0.16%	0.017%
21	13.940	1855	1862	1877	rBV	1898640	2668002	37.83%	4.196%
22	14.222	1902	1910	1935	rBV	2297355	3372562	47.82%	5.304%
23	14.528	1955	1962	1975	rBV	1629603	2430114	34.46%	3.822%
24	14.740	1991	1998	2018	rBV2	60385	207501	2.94%	0.326%
25	14.951	2028	2034	2042	rVB2	7100	16011	0.23%	0.025%
26	15.522	2124	2131	2144	rBV	3252501	4606793	65.32%	7.245%
27	15.640	2145	2151	2165	rVV	826151	1195571	16.95%	1.880%
28	15.769	2168	2173	2178	rVB2	14023	25094	0.36%	0.039%
29	17.287	2424	2431	2440	rBV	2012513	2860266	40.56%	4.498%
30	17.387	2441	2448	2462	rBV	3734449	5402154	76.60%	8.495%
31	18.169	2577	2581	2589	rBV3	52090	86962	1.23%	0.137%
32	19.198	2752	2756	2760	rBV	45468	58783	0.83%	0.092%
33	19.263	2764	2767	2775	rVV	47705	73666	1.04%	0.116%
34	19.398	2787	2790	2795	rBV4	47745	73254	1.04%	0.115%
35	19.622	2822	2828	2839	rBV	4930005	6632069	94.04%	10.429%
36	21.369	3121	3125	3136	rBV	2595180	3307122	46.89%	5.201%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011933.D
Acq On : 05 Oct 2022 16:47
Operator : CG/JU
Sample : N4890-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0E6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37	23.645	3505	3512	3526	rVB2	3527102	7052489	100.00%	11.091%
38	23.804	3533	3539	3549	rVB2	1693125	3430434	48.64%	5.395%




Sum of corrected areas: 63589580

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011933.D
Acq On : 05 Oct 2022 16:47
Operator : CG/JU
Sample : N4890-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0E6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

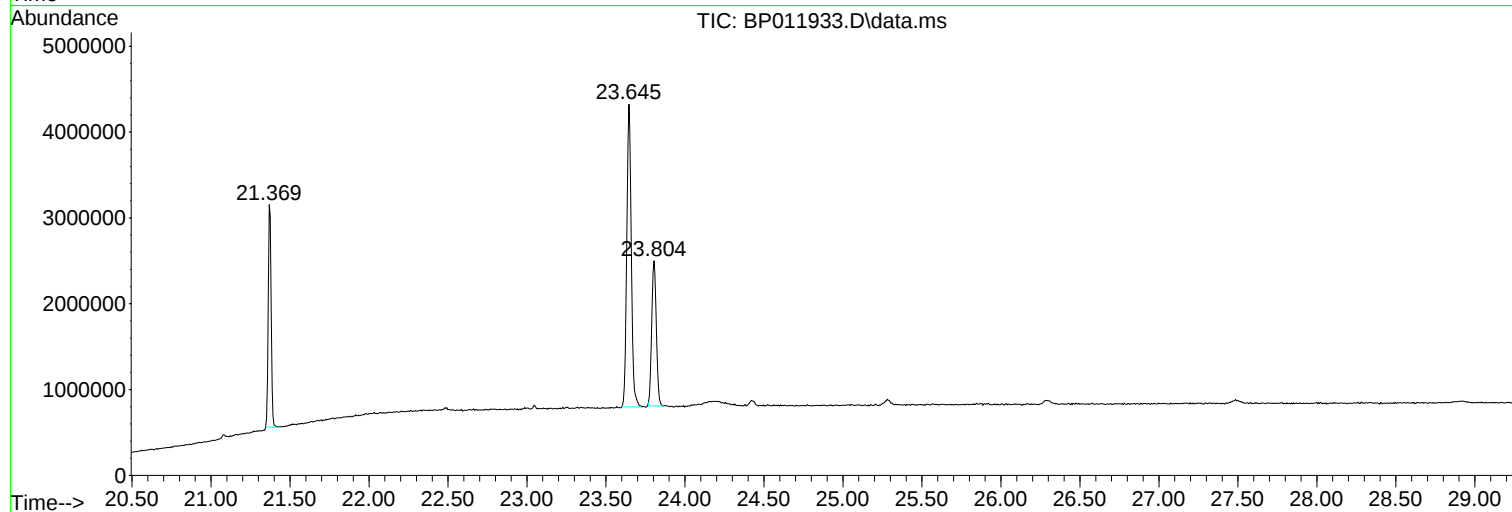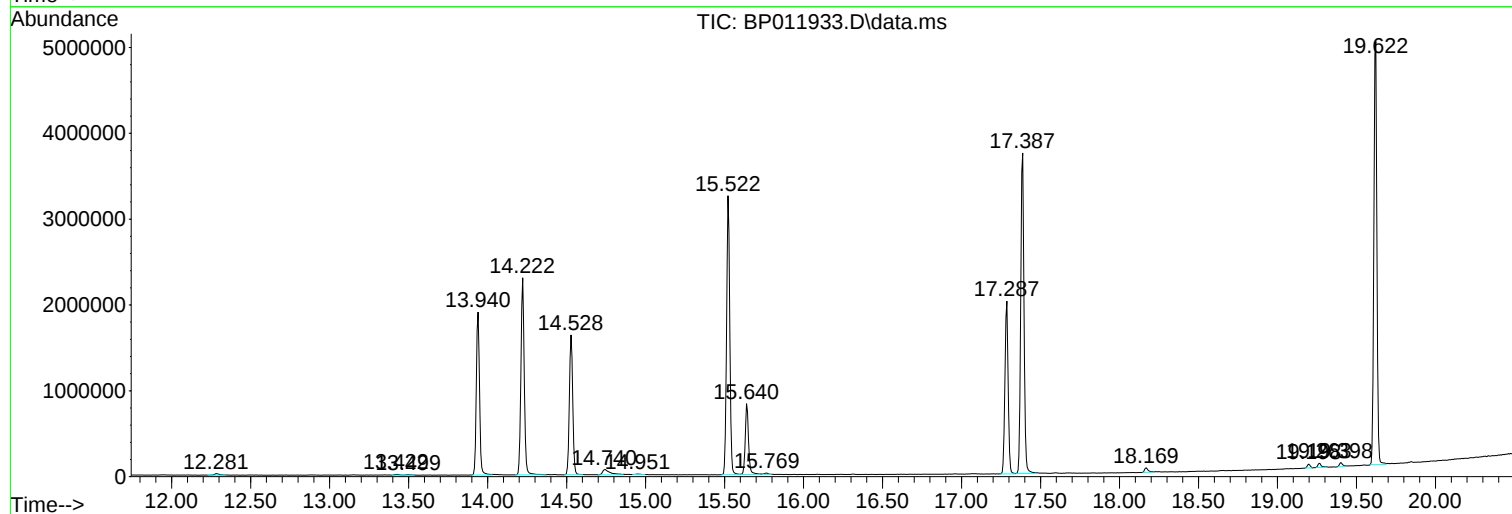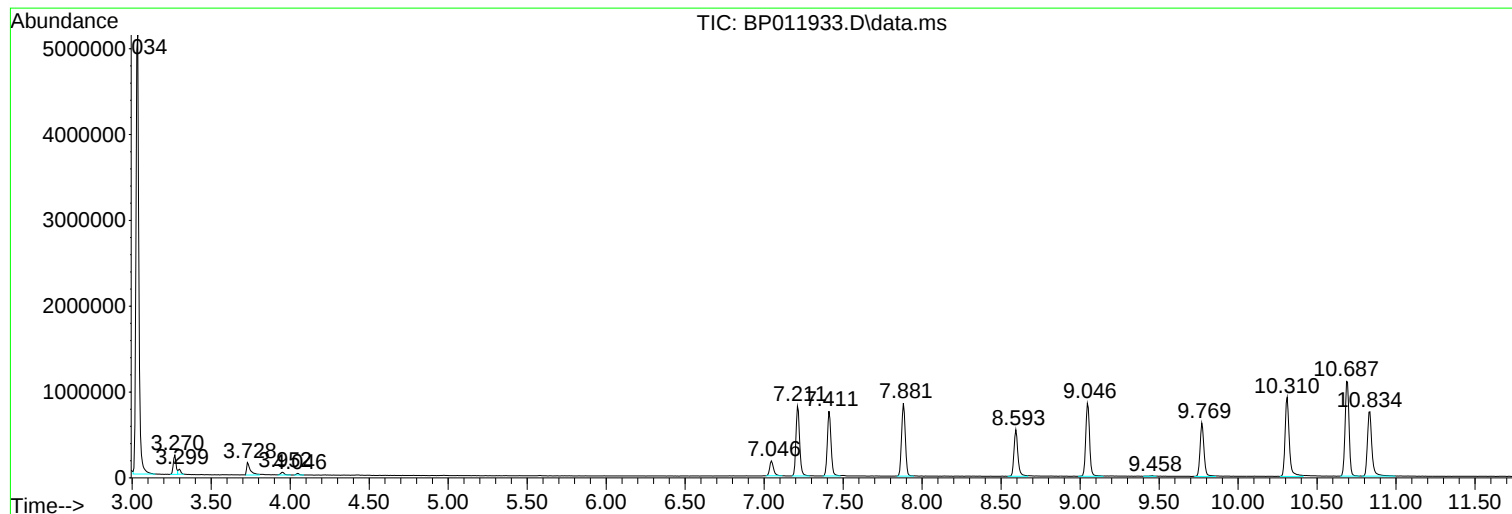

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011933.D
Acq On : 05 Oct 2022 16:47
Operator : CG/JU
Sample : N4890-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0E6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	96.50 ng/ul	6570380	1,4-Dichlorobenzene-d4	7.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43		
4	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		
5	N-Ethylformamide	73	C3H7NO	000627-45-2	9		

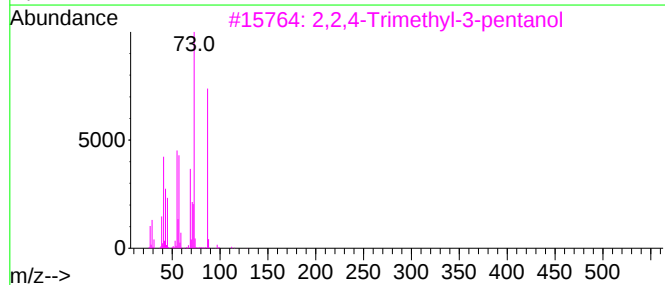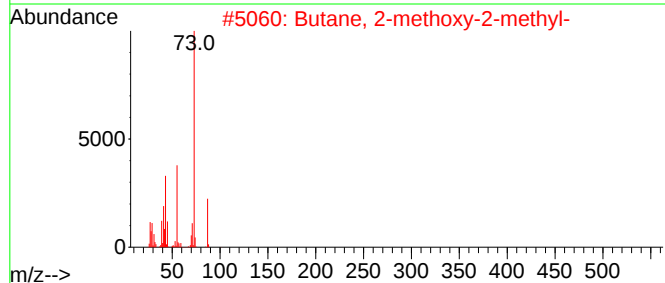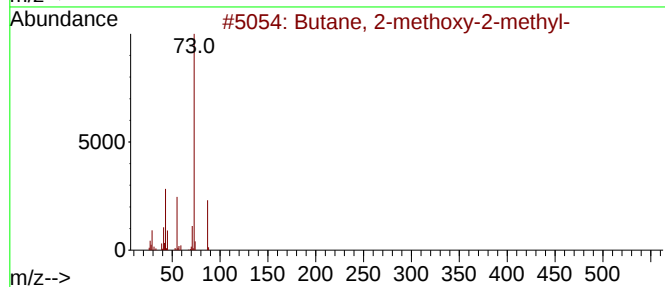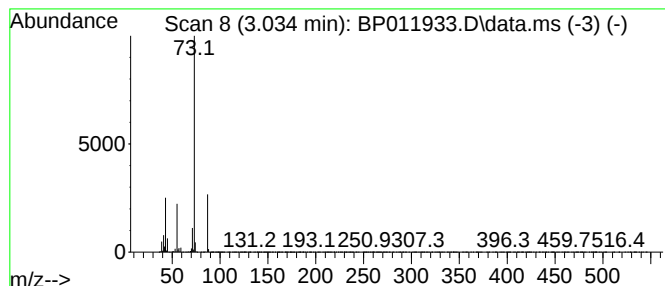

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011933.D
Acq On : 05 Oct 2022 16:47
Operator : CG/JU
Sample : N4890-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY0E6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	96.5	ng/ul	6570380	1	7.881	1361680	20.0