

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011951.D
 Acq On : 06 Oct 2022 03:39
 Operator : CG/JU
 Sample : N4847-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8R4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	27	rVB	5061355	6530304	93.71%	10.209%
2	3.299	49	53	58	rBV	51717	62210	0.89%	0.097%
3	3.728	124	126	142	rBV	175265	295558	4.24%	0.462%
4	3.946	159	163	168	rVB	29335	41318	0.59%	0.065%
5	4.046	176	180	185	rVB	13009	17679	0.25%	0.028%
6	4.416	240	243	248	rVB6	6554	9517	0.14%	0.015%
7	4.993	333	341	345	rVB4	5967	13253	0.19%	0.021%
8	7.040	681	689	704	rBV	207792	410060	5.88%	0.641%
9	7.210	711	718	732	rBV	787572	1282804	18.41%	2.005%
10	7.410	745	752	763	rBV	752911	1230601	17.66%	1.924%
11	7.881	824	832	843	rBV	657767	1083327	15.55%	1.694%
12	7.957	843	845	854	rVB8	5301	10840	0.16%	0.017%
13	8.134	869	875	889	rBV	33370	70960	1.02%	0.111%
14	8.587	945	952	969	rBV	607613	1060379	15.22%	1.658%
15	9.046	1023	1030	1041	rBV	864344	1456999	20.91%	2.278%
16	9.204	1054	1057	1062	rBV7	6688	10606	0.15%	0.017%
17	9.616	1119	1127	1136	rBV	46912	88113	1.26%	0.138%
18	9.769	1146	1153	1169	rBV	546323	913148	13.10%	1.428%
19	10.304	1237	1244	1270	rBV	986403	1821909	26.14%	2.848%
20	10.687	1300	1309	1320	rBV	952480	1626273	23.34%	2.542%
21	10.828	1326	1333	1351	rBV	983874	1824600	26.18%	2.853%
22	12.228	1559	1571	1575	rBV4	9405	21352	0.31%	0.033%
23	12.281	1575	1580	1589	rVB	19136	37645	0.54%	0.059%
24	13.140	1722	1726	1733	rVB9	3797	9726	0.14%	0.015%
25	13.422	1768	1774	1781	rBV	26800	43825	0.63%	0.069%
26	13.492	1781	1786	1795	rVB7	4371	8373	0.12%	0.013%
27	13.934	1853	1861	1875	rBV	2093515	3071849	44.08%	4.802%
28	14.169	1894	1901	1904	rBV	174606	266516	3.82%	0.417%
29	14.216	1904	1909	1929	rVB	2483440	3912222	56.14%	6.116%
30	14.528	1955	1962	1970	rBV	1531015	2253526	32.34%	3.523%
31	14.745	1993	1999	2015	rBV	53089	178284	2.56%	0.279%
32	14.957	2028	2035	2042	rBV	11616	24069	0.35%	0.038%
33	15.522	2122	2131	2145	rBV	3587171	5214989	74.83%	8.153%
34	15.639	2145	2151	2166	rVV	365259	576901	8.28%	0.902%
35	15.763	2168	2172	2178	rVB2	15738	27096	0.39%	0.042%
36	16.304	2261	2264	2272	rVB10	4130	8852	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011951.D
Acq On : 06 Oct 2022 03:39
Operator : CG/JU
Sample : N4847-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8R4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37	17.281	2424	2430	2440	rBV	1914777	2700931	38.76%	4.223%
38	17.381	2441	2447	2461	rVV	4140860	5876025	84.32%	9.186%
39	19.192	2751	2755	2760	rBV2	49344	70394	1.01%	0.110%
40	19.263	2763	2767	2773	rBV2	52698	78330	1.12%	0.122%
41	19.616	2821	2827	2838	rBV	5311735	6915062	99.23%	10.811%
42	21.369	3120	3125	3135	rBV	2247872	2968240	42.59%	4.640%
43	23.639	3504	3511	3527	rVB2	3469885	6968886	100.00%	10.895%
44	23.798	3532	3538	3548	rVB2	1392607	2871040	41.20%	4.488%




Sum of corrected areas: 63964591

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011951.D
Acq On : 06 Oct 2022 03:39
Operator : CG/JU
Sample : N4847-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8R4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

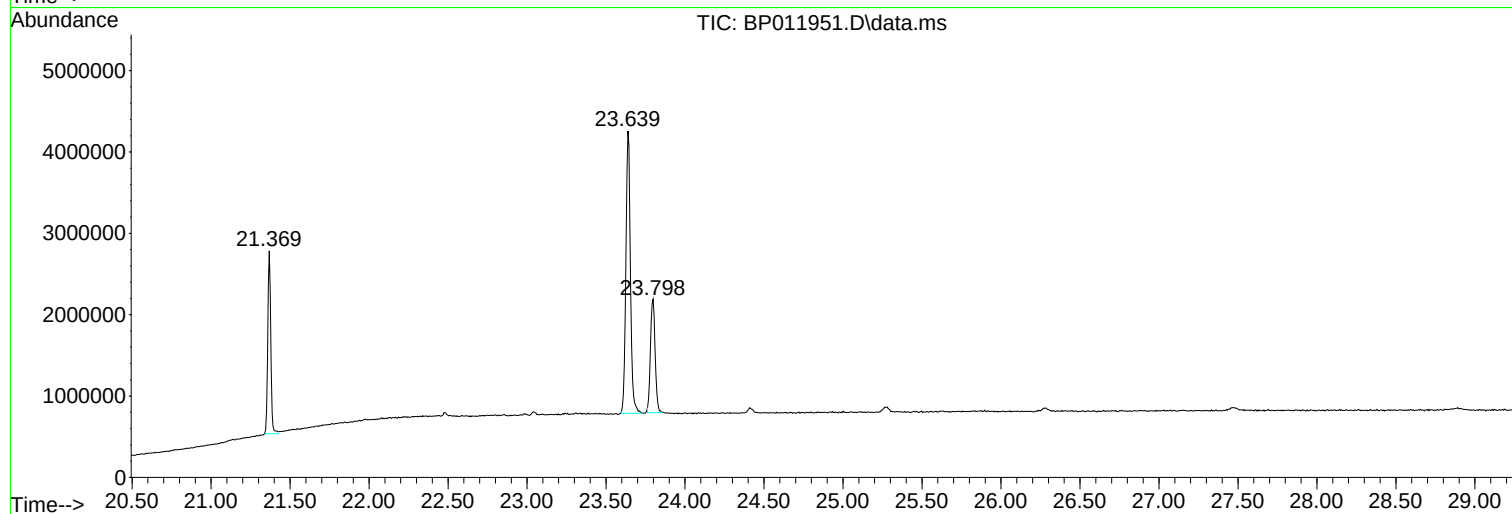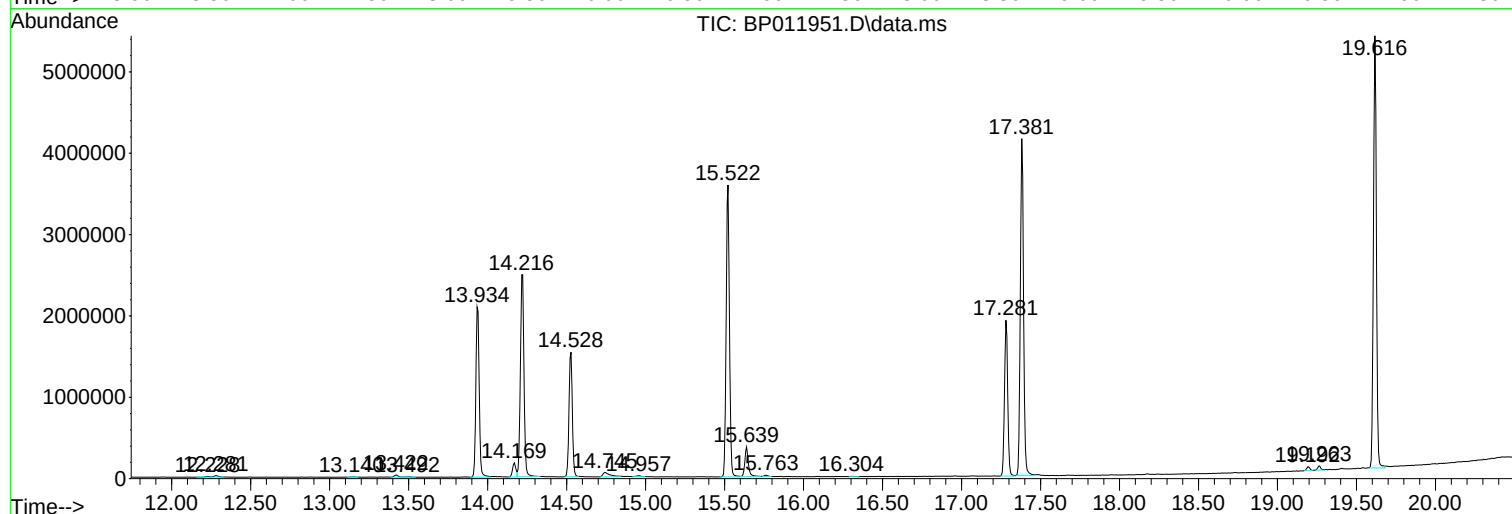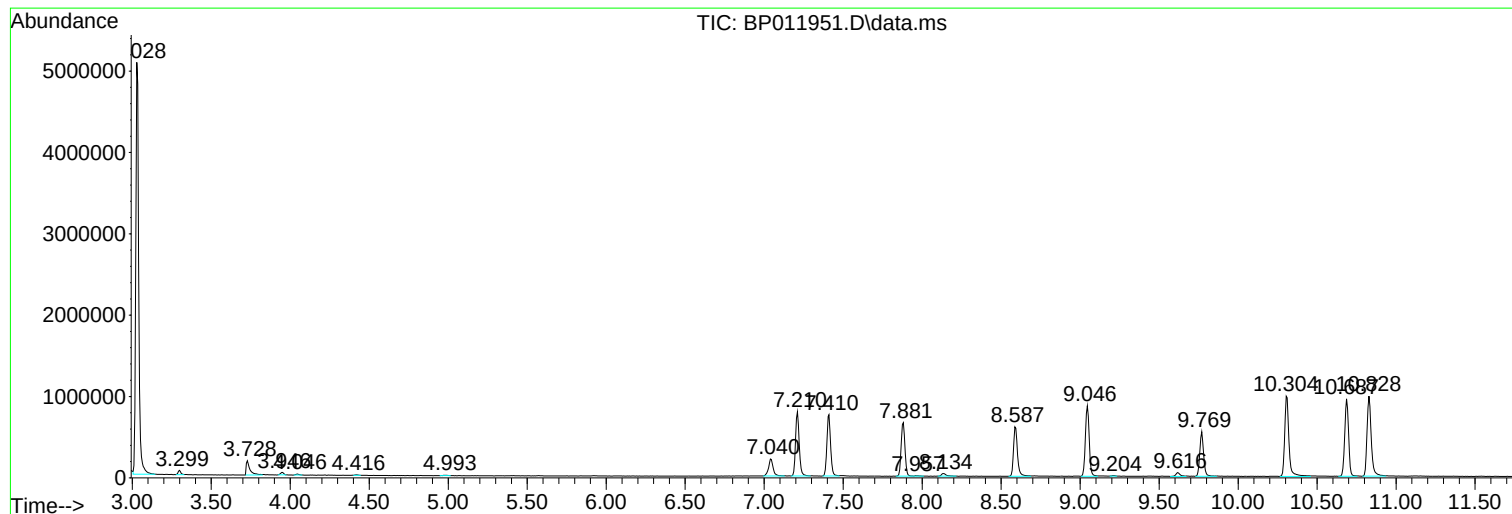

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011951.D
Acq On : 06 Oct 2022 03:39
Operator : CG/JU
Sample : N4847-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8R4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	120.56 ng/ul	6530300	1,4-Dichlorobenzene-d4	7.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17		
5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		

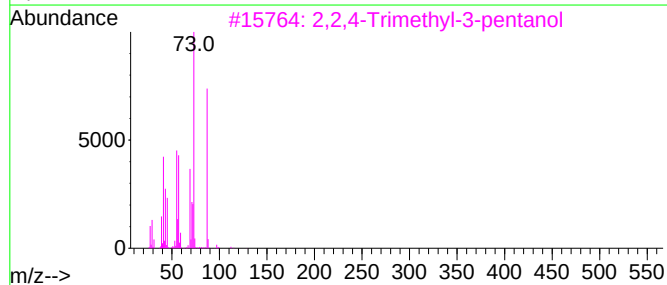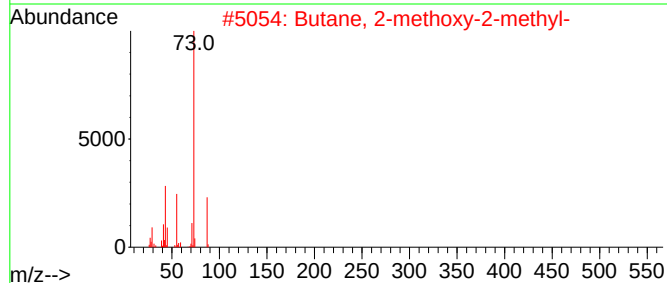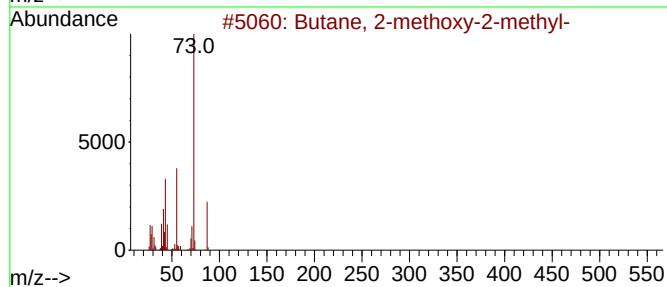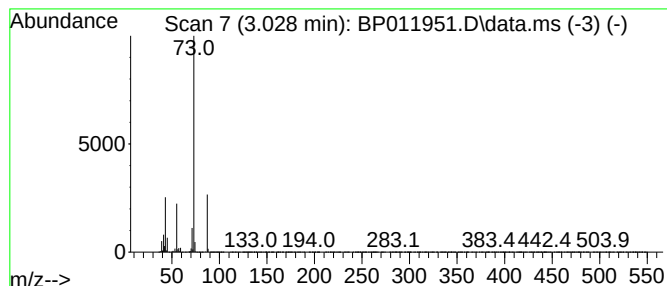

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011951.D
Acq On : 06 Oct 2022 03:39
Operator : CG/JU
Sample : N4847-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8R4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	120.6	ng/ul	6530300	1	7.881	1083330	20.0