

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011952.D
 Acq On : 06 Oct 2022 04:14
 Operator : CG/JU
 Sample : N4847-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8S5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	30	rVB	4692099	6140372	100.00%	10.495%
2	3.299	49	53	62	rVB	46064	61149	1.00%	0.105%
3	3.734	125	127	141	rBV	64038	114348	1.86%	0.195%
4	3.952	158	164	170	rBV	29227	47929	0.78%	0.082%
5	4.046	176	180	187	rBV	22786	30460	0.50%	0.052%
6	4.410	239	242	247	rVB4	9839	13619	0.22%	0.023%
7	7.045	681	690	701	rBV	157566	288282	4.69%	0.493%
8	7.210	711	718	735	rBV	630548	1033205	16.83%	1.766%
9	7.410	744	752	764	rBV	593348	973807	15.86%	1.664%
10	7.487	764	765	772	rVB7	5153	8099	0.13%	0.014%
11	7.881	825	832	843	rBV	888225	1456334	23.72%	2.489%
12	8.134	869	875	884	rBV2	28880	57611	0.94%	0.098%
13	8.587	946	952	970	rBV	441761	802046	13.06%	1.371%
14	8.981	1015	1019	1022	rBV6	3768	6228	0.10%	0.011%
15	9.045	1022	1030	1044	rVV	678586	1137913	18.53%	1.945%
16	9.210	1050	1058	1065	rBV2	18076	33402	0.54%	0.057%
17	9.616	1121	1127	1136	rBV	38746	73294	1.19%	0.125%
18	9.769	1146	1153	1163	rBV	379705	648477	10.56%	1.108%
19	10.310	1237	1245	1273	rBV	721845	1391192	22.66%	2.378%
20	10.686	1301	1309	1326	rBV	1295734	2163911	35.24%	3.698%
21	10.828	1326	1333	1354	rBV	759546	1442700	23.50%	2.466%
22	11.533	1443	1453	1457	rBV	3154	6958	0.11%	0.012%
23	12.280	1573	1580	1587	rBV	13369	26455	0.43%	0.045%
24	13.422	1768	1774	1779	rBV6	5642	9961	0.16%	0.017%
25	13.933	1854	1861	1891	rBV	1580441	2393922	38.99%	4.091%
26	14.222	1902	1910	1925	rBV	1860405	2895990	47.16%	4.950%
27	14.527	1955	1962	1978	rBV	1981785	2934203	47.79%	5.015%
28	14.745	1993	1999	2013	rBV3	34018	123564	2.01%	0.211%
29	15.521	2123	2131	2144	rBV	2683325	3986648	64.93%	6.814%
30	15.639	2145	2151	2166	rVV	388314	593678	9.67%	1.015%
31	15.763	2168	2172	2177	rVB2	11908	19553	0.32%	0.033%
32	16.310	2261	2265	2270	rVB8	3976	6807	0.11%	0.012%
33	16.957	2371	2375	2380	rBV8	3685	6231	0.10%	0.011%
34	17.280	2421	2430	2441	rBV	2365946	3486862	56.79%	5.959%
35	17.380	2441	2447	2464	rVV	3334668	4819322	78.49%	8.237%
36	17.951	2540	2544	2549	rBV5	18869	25196	0.41%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011952.D
 Acq On : 06 Oct 2022 04:14
 Operator : CG/JU
 Sample : N4847-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8S5

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	18.168	2577	2581	2588	rBV9	17296	38250	0.62%	0.065%
38	19.198	2752	2756	2762	rBV4	35691	52058	0.85%	0.089%
39	19.262	2763	2767	2773	rBV	43917	71026	1.16%	0.121%
40	19.615	2821	2827	2839	rBV	4355758	5688720	92.64%	9.723%
41	21.368	3120	3125	3134	rBV	3021459	3872128	63.06%	6.618%
42	23.639	3505	3511	3527	rVB2	2838785	5633959	91.75%	9.629%
43	23.798	3532	3538	3552	rVB2	1891608	3893879	63.41%	6.655%




Sum of corrected areas: 58509748

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011952.D
Acq On : 06 Oct 2022 04:14
Operator : CG/JU
Sample : N4847-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8S5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

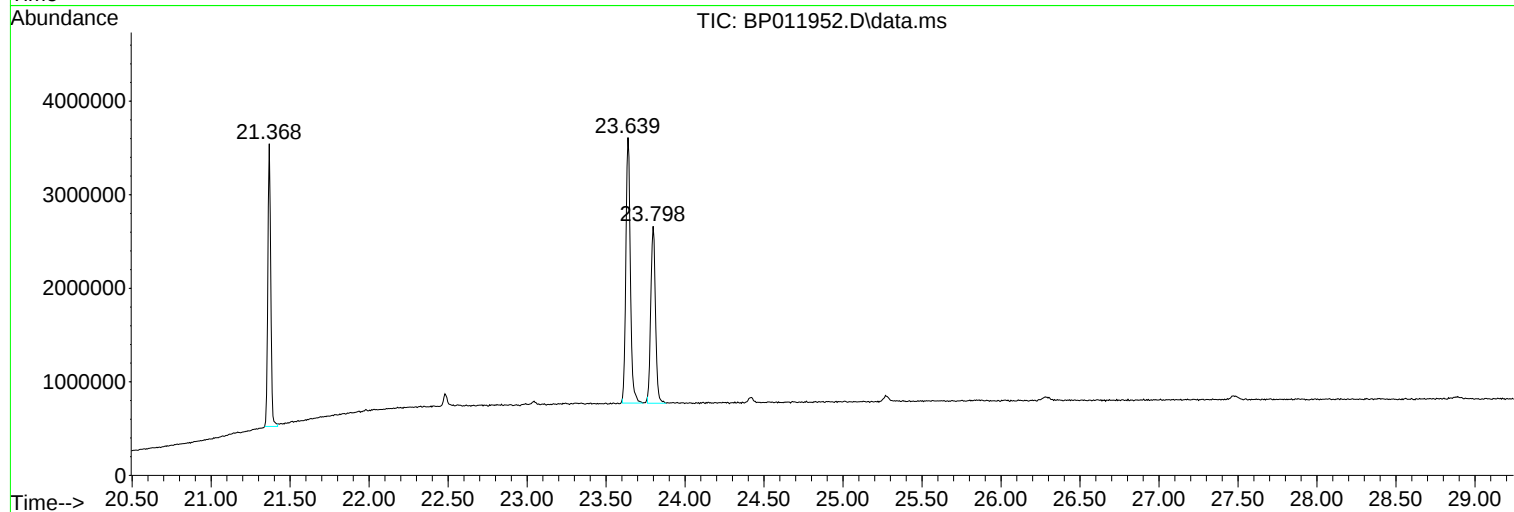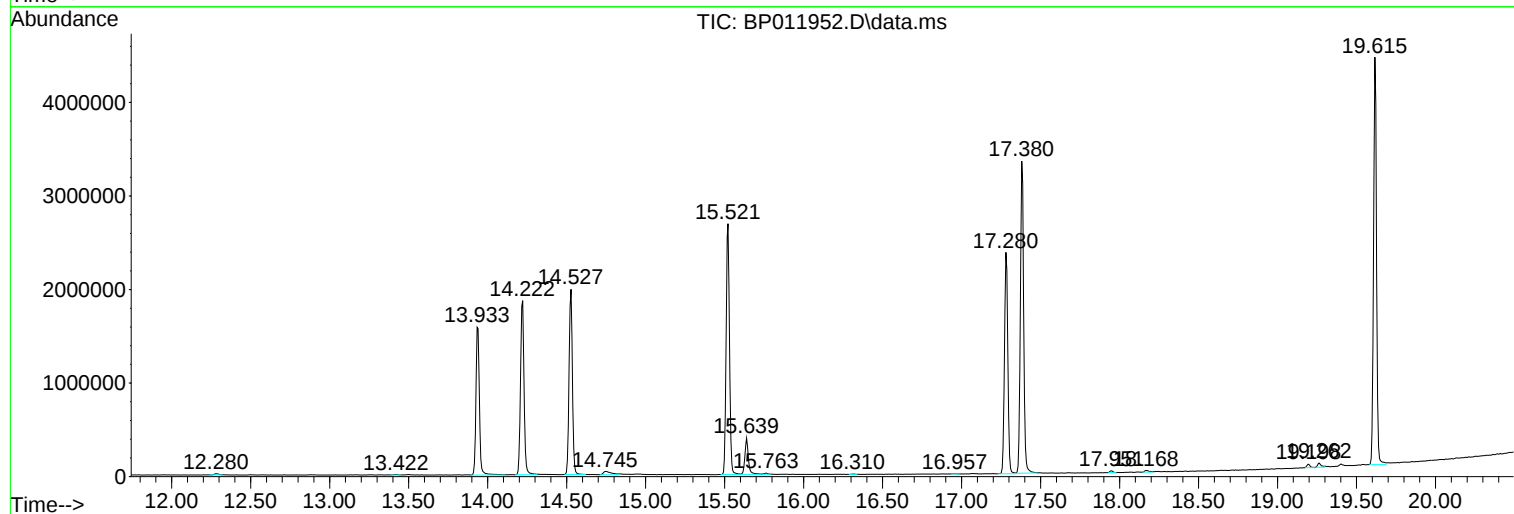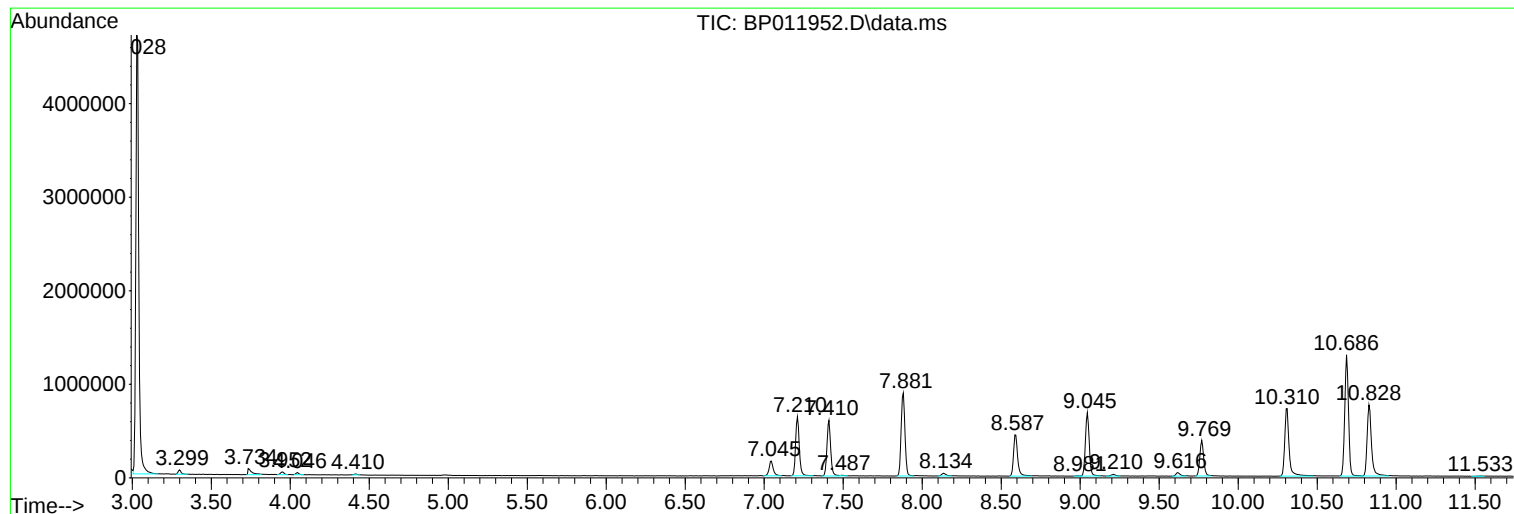

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011952.D
Acq On : 06 Oct 2022 04:14
Operator : CG/JU
Sample : N4847-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8S5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	84.33 ng/ul	6140370	1,4-Dichlorobenzene-d4	7.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

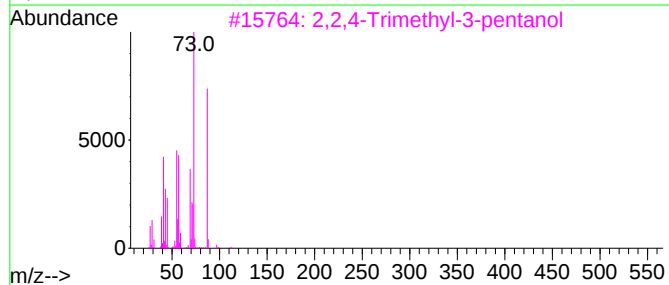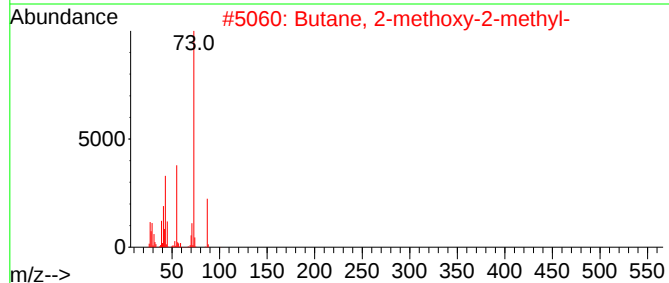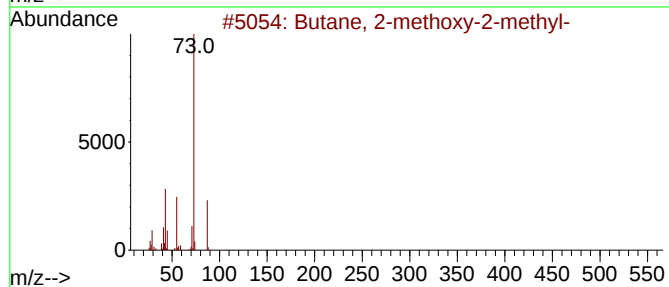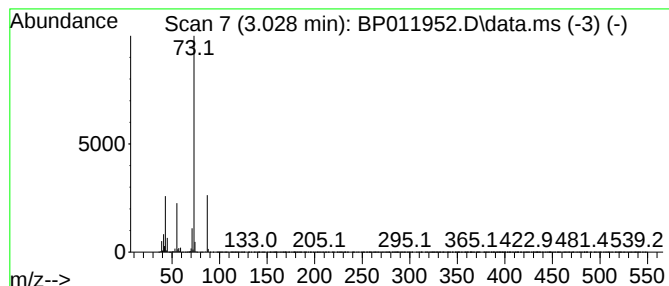

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011952.D
Acq On : 06 Oct 2022 04:14
Operator : CG/JU
Sample : N4847-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8S5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	84.3	ng/ul	6140370	1	7.881	1456330	20.0