

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011964.D
 Acq On : 06 Oct 2022 11:37
 Operator : CG/JU
 Sample : N4956-12
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8W3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	30	rVB	5115960	6739704	86.76%	9.045%
2	3.299	49	53	58	rBV	53366	65537	0.84%	0.088%
3	3.728	123	126	141	rBV	130355	211172	2.72%	0.283%
4	3.952	159	164	170	rVB	32797	52150	0.67%	0.070%
5	4.046	176	180	187	rBV	21258	31364	0.40%	0.042%
6	4.611	272	276	279	rVB4	8335	11078	0.14%	0.015%
7	4.969	334	337	341	rVB4	5528	8271	0.11%	0.011%
8	7.040	684	689	703	rVB	200361	362026	4.66%	0.486%
9	7.211	711	718	732	rBV	842298	1374949	17.70%	1.845%
10	7.405	745	751	763	rBV	762066	1274050	16.40%	1.710%
11	7.875	823	831	841	rBV	943759	1559912	20.08%	2.093%
12	8.587	946	952	965	rBV	622579	1057931	13.62%	1.420%
13	9.046	1021	1030	1041	rBV	937306	1608729	20.71%	2.159%
14	9.452	1092	1099	1103	rBV2	10096	16239	0.21%	0.022%
15	9.769	1143	1153	1169	rBV	694160	1217585	15.67%	1.634%
16	10.304	1236	1244	1263	rBV	1102791	2017079	25.96%	2.707%
17	10.687	1301	1309	1323	rBV	1364024	2350105	30.25%	3.154%
18	10.828	1325	1333	1355	rVV	767868	1471809	18.95%	1.975%
19	10.981	1357	1359	1367	rVB8	8127	12053	0.16%	0.016%
20	11.352	1420	1422	1433	rVB9	3756	8778	0.11%	0.012%
21	12.275	1572	1579	1585	rBV3	21611	41238	0.53%	0.055%
22	13.146	1721	1727	1733	rVB6	4740	9410	0.12%	0.013%
23	13.346	1757	1761	1764	rBV5	6509	8413	0.11%	0.011%
24	13.422	1768	1774	1778	rVB6	9688	14866	0.19%	0.020%
25	13.498	1782	1787	1793	rBV8	5278	10616	0.14%	0.014%
26	13.934	1854	1861	1877	rBV	2437335	3474410	44.72%	4.663%
27	14.216	1899	1909	1929	rBV	2803819	4253809	54.76%	5.709%
28	14.522	1954	1961	1972	rBV	2144807	3182693	40.97%	4.271%
29	14.734	1991	1997	2011	rBV	108221	274175	3.53%	0.368%
30	14.887	2019	2023	2027	rBV7	5925	9881	0.13%	0.013%
31	14.945	2029	2033	2042	rVB9	12339	27621	0.36%	0.037%
32	15.522	2121	2131	2144	rBV	3693689	5678988	73.10%	7.621%
33	15.640	2144	2151	2165	rVV	1004477	1468268	18.90%	1.970%
34	15.763	2168	2172	2177	rVB3	28839	45151	0.58%	0.061%
35	16.234	2250	2252	2257	rVB6	6824	8865	0.11%	0.012%
36	16.681	2324	2328	2334	rBV9	5602	14289	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011964.D
 Acq On : 06 Oct 2022 11:37
 Operator : CG/JU
 Sample : N4956-12
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8W3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	17.039	2386	2389	2391	rBV4	7719	9783	0.13%	0.013%
38	17.281	2424	2430	2440	rBV	2681094	3786977	48.75%	5.082%
39	17.381	2441	2447	2463	rVB	4441082	6284069	80.89%	8.433%
40	18.163	2576	2580	2590	rBV2	122689	188960	2.43%	0.254%
41	19.192	2752	2755	2761	rVB2	53770	78104	1.01%	0.105%
42	19.263	2763	2767	2773	rBV	67690	113219	1.46%	0.152%
43	19.398	2786	2790	2794	rBV2	86115	113696	1.46%	0.153%
44	19.616	2821	2827	2839	rBV	5867200	7594973	97.77%	10.193%
45	21.075	3073	3075	3083	rBV5	98356	138332	1.78%	0.186%
46	21.369	3120	3125	3133	rBV	3320264	4237068	54.54%	5.686%
47	23.639	3504	3511	3524	rVB2	3912321	7768569	100.00%	10.426%
48	23.798	3532	3538	3550	rVB2	2054830	4226538	54.41%	5.672%




Sum of corrected areas: 74513502

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011964.D
Acq On : 06 Oct 2022 11:37
Operator : CG/JU
Sample : N4956-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8W3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

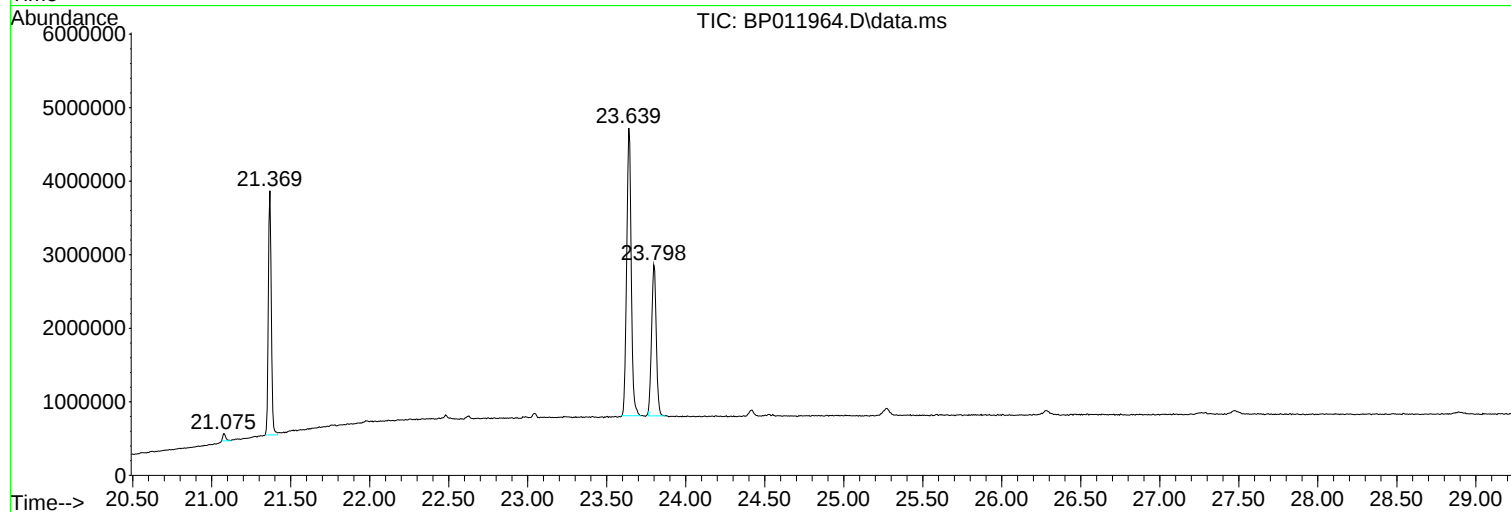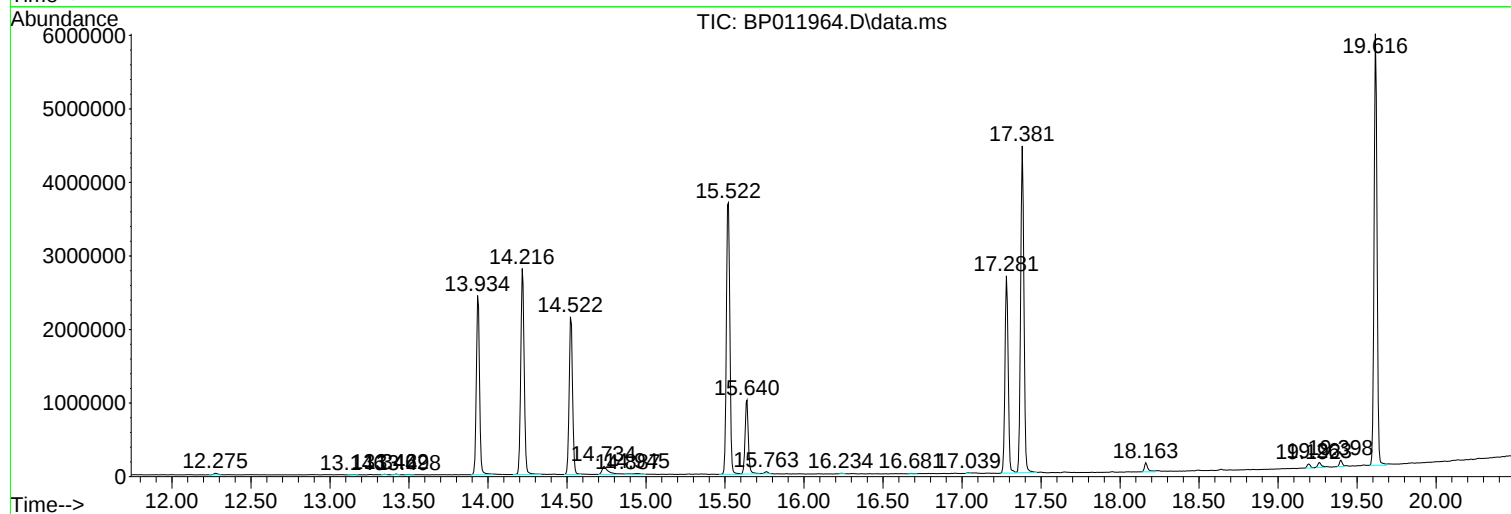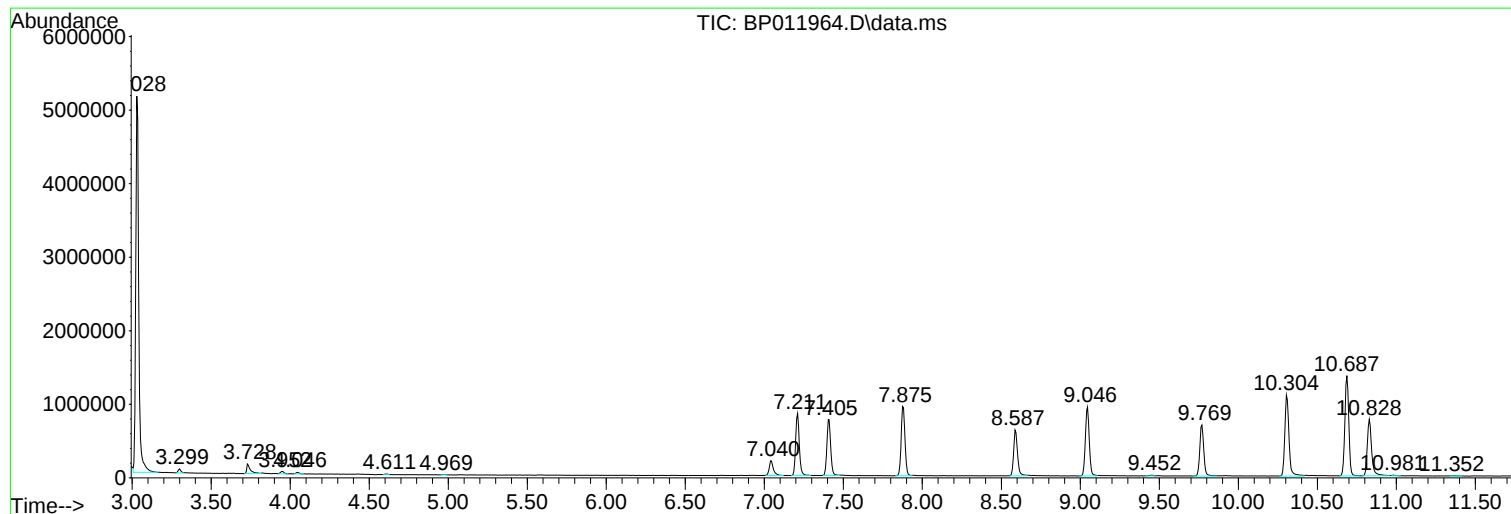

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011964.D
Acq On : 06 Oct 2022 11:37
Operator : CG/JU
Sample : N4956-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8W3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	86.41 ng/ul	6739700	1,4-Dichlorobenzene-d4	7.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17		
5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		

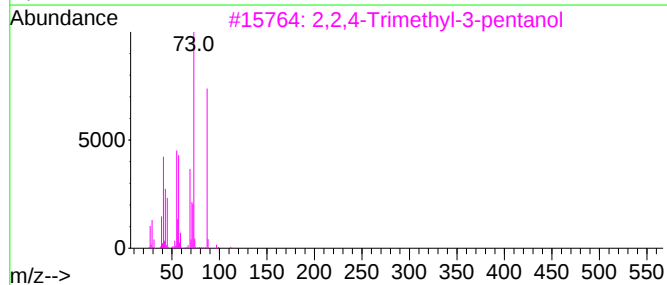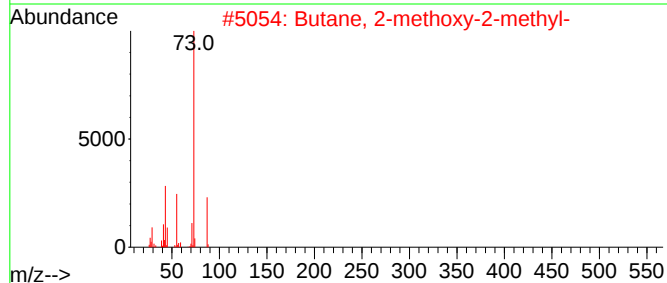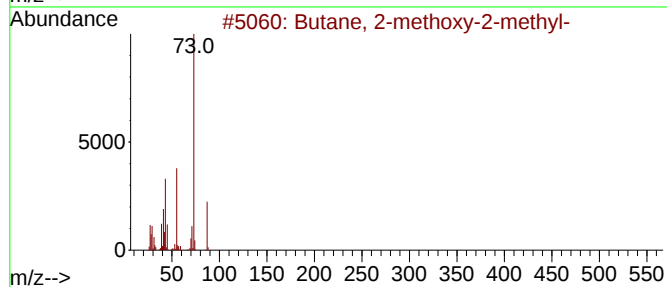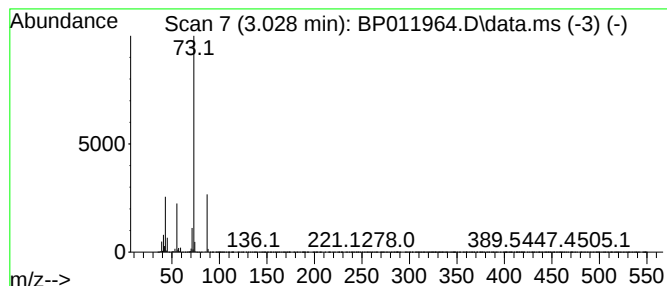

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011964.D
Acq On : 06 Oct 2022 11:37
Operator : CG/JU
Sample : N4956-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8W3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	86.4	ng/u1	6739700	1	7.881	1559910	20.0