

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011973.D
 Acq On : 06 Oct 2022 16:49
 Operator : CG/JU
 Sample : PB148077BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK077

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011973.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	18	rVB	190205	237056	4.58%	0.461%
2	3.299	49	53	59	rVB	60699	74168	1.43%	0.144%
3	3.722	122	125	150	rBV	623066	958646	18.51%	1.866%
4	4.046	177	180	185	rVB	17358	23346	0.45%	0.045%
5	7.045	683	690	704	rBV	779403	1268734	24.50%	2.470%
6	7.210	711	718	730	rBV	689885	1115917	21.55%	2.172%
7	7.410	745	752	763	rBV	833718	1352536	26.12%	2.633%
8	7.881	825	832	846	rVB	765579	1237074	23.89%	2.408%
9	8.592	945	953	967	rBV	966376	1624485	31.37%	3.162%
10	9.045	1022	1030	1045	rBV	739589	1249145	24.12%	2.431%
11	9.769	1143	1153	1165	rBV	584447	981338	18.95%	1.910%
12	10.310	1237	1245	1266	rBV	872798	1611935	31.13%	3.138%
13	10.686	1301	1309	1324	rVB	1039513	1776327	34.30%	3.458%
14	10.828	1326	1333	1356	rBV	815120	1595386	30.81%	3.105%
15	12.281	1575	1580	1588	rBV3	13514	31033	0.60%	0.060%
16	13.422	1766	1774	1779	rBV3	20163	32423	0.63%	0.063%
17	13.498	1782	1787	1793	rVB9	3532	6170	0.12%	0.012%
18	13.939	1855	1862	1876	rBV	1475039	2189933	42.29%	4.263%
19	14.222	1902	1910	1923	rBV	1843177	2874884	55.52%	5.596%
20	14.527	1953	1962	1973	rBV	1506374	2255605	43.56%	4.390%
21	14.633	1978	1980	1988	rVB8	3514	6831	0.13%	0.013%
22	14.733	1991	1997	2022	rBV	461795	1044626	20.17%	2.033%
23	15.522	2124	2131	2145	rBV	2504597	3643598	70.36%	7.092%
24	15.639	2145	2151	2168	rVV	633996	914859	17.67%	1.781%
25	15.763	2168	2172	2176	rVB3	12173	19397	0.37%	0.038%
26	16.310	2259	2265	2269	rBV9	4026	7304	0.14%	0.014%
27	17.068	2390	2394	2398	rBV5	3695	6360	0.12%	0.012%
28	17.280	2424	2430	2441	rBV	1831519	2657846	51.33%	5.173%
29	17.380	2441	2447	2462	rVV2	2767730	4079356	78.78%	7.940%
30	19.192	2752	2755	2760	rBV4	33240	45671	0.88%	0.089%
31	19.262	2764	2767	2771	rVB2	32362	43270	0.84%	0.084%
32	19.615	2822	2827	2839	rBV	3708979	4907029	94.76%	9.551%
33	21.368	3120	3125	3136	rBV	2464873	3122883	60.31%	6.078%
34	23.639	3504	3511	3523	rBV2	2554568	5178198	100.00%	10.079%
35	23.798	3532	3538	3549	rVB2	1563718	3202568	61.85%	6.234%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011973.D
Acq On : 06 Oct 2022 16:49
Operator : CG/JU
Sample : PB148077BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK077

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION




Sum of corrected areas: 51375937

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011973.D
Acq On : 06 Oct 2022 16:49
Operator : CG/JU
Sample : PB148077BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK077

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

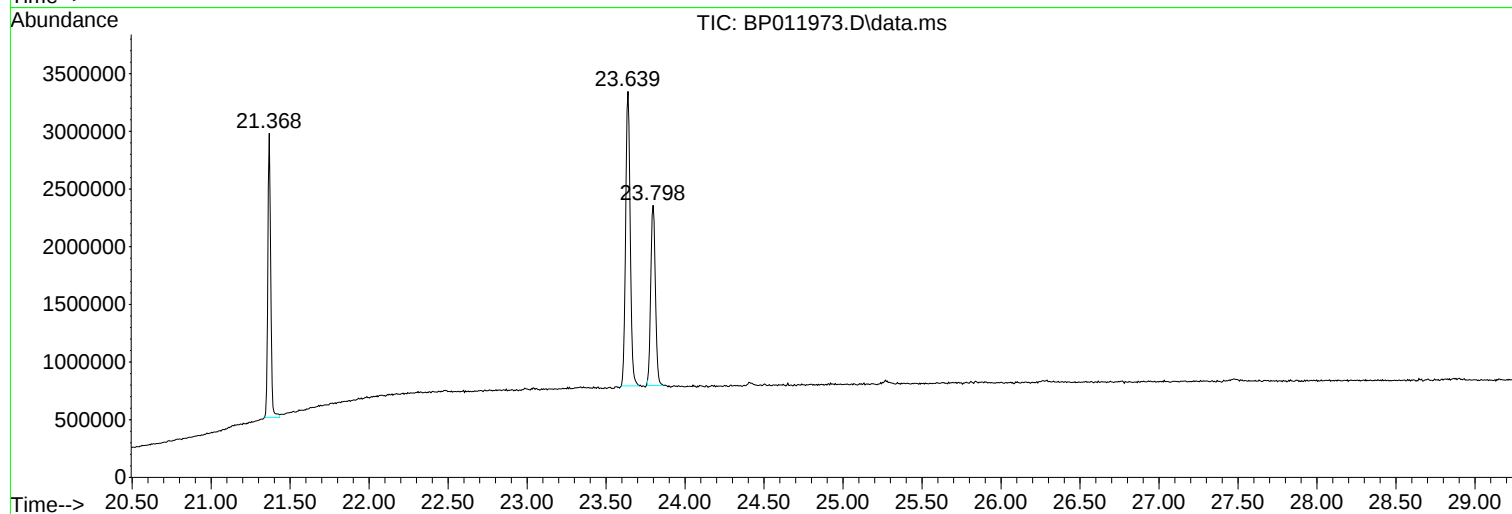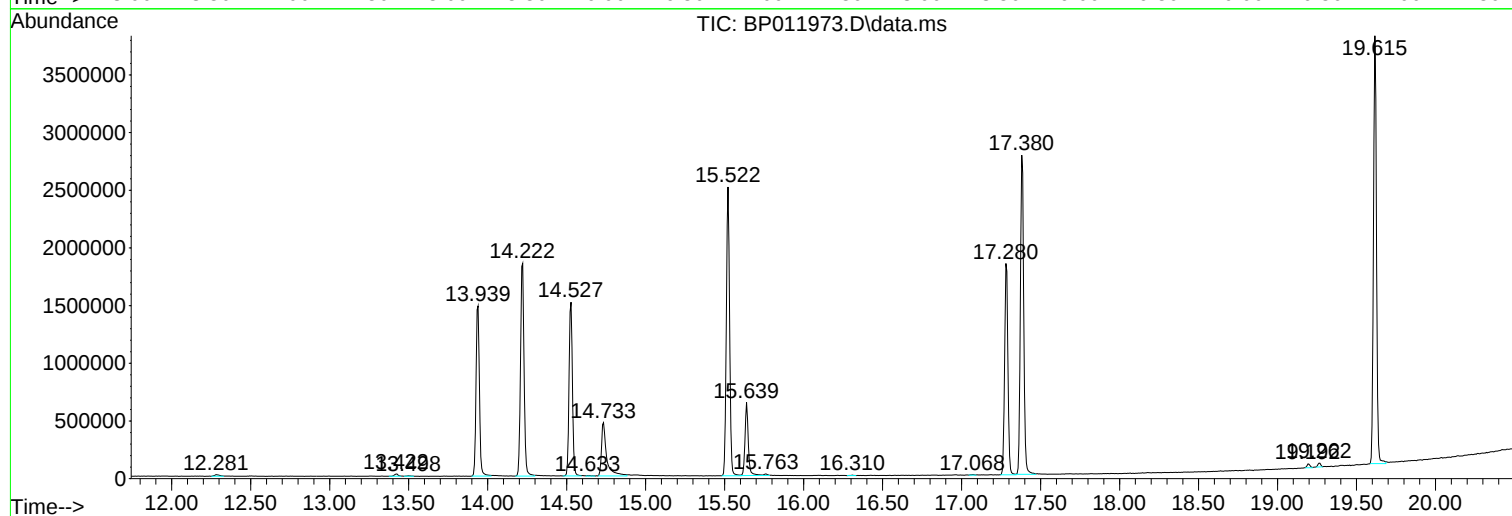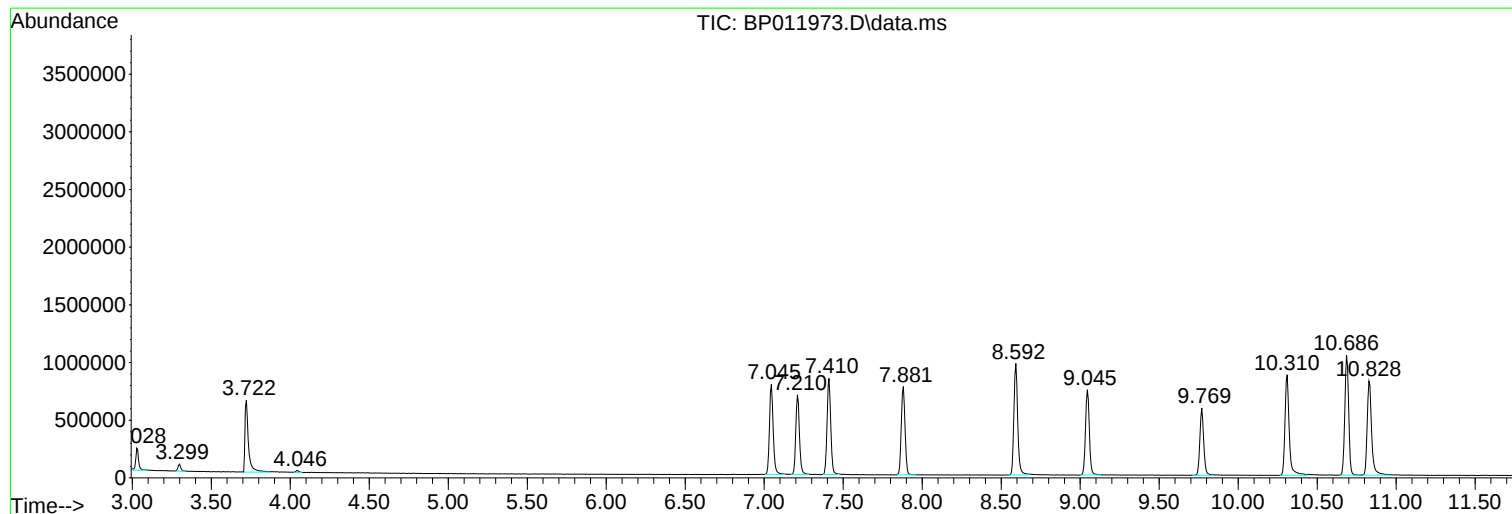

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011973.D
Acq On : 06 Oct 2022 16:49
Operator : CG/JU
Sample : PB148077BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK077










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	3.83 ng/ul	237056	1,4-Dichlorobenzene-d4	7.881

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	90
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

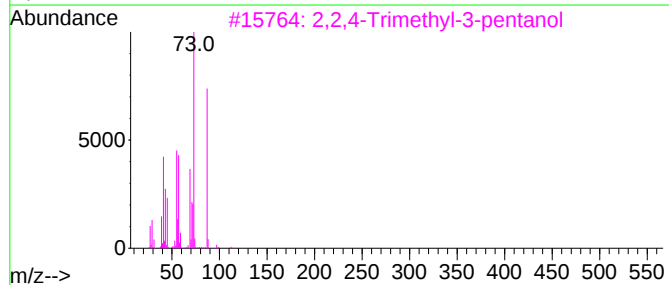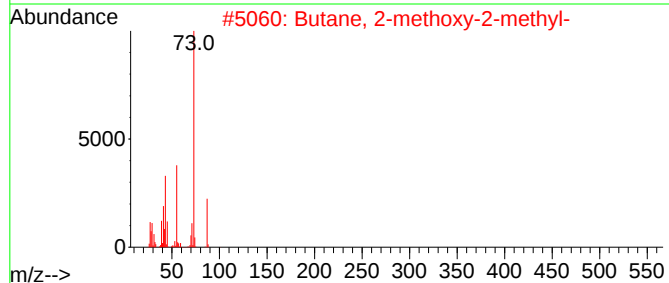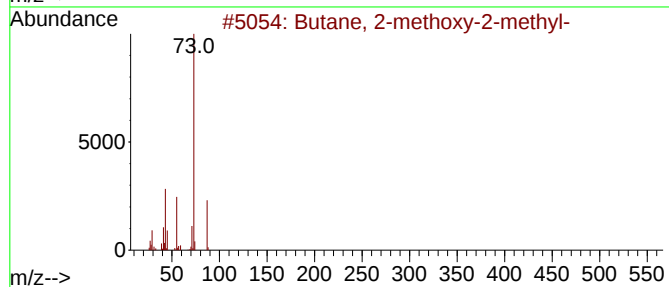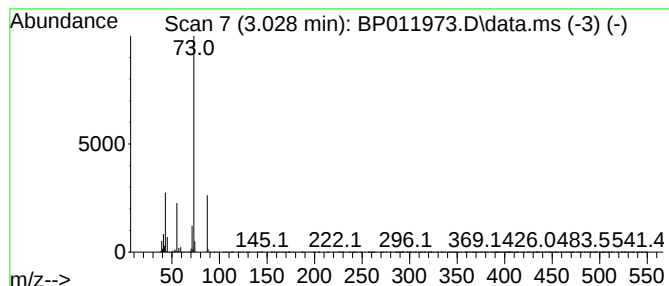

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011973.D
Acq On : 06 Oct 2022 16:49
Operator : CG/JU
Sample : PB148077BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK077

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	3.8	ng/u1	237056	1	7.881	1237070	20.0