

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011977.D
 Acq On : 06 Oct 2022 19:09
 Operator : CG/JU
 Sample : N4923-14
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10013

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.029	3	7	34	rVB	4909435	6549214	85.96%	9.686%
2	3.299	49	53	58	rBV	48477	63414	0.83%	0.094%
3	3.740	126	128	141	rBV	90728	192304	2.52%	0.284%
4	3.946	159	163	168	rVB	27863	43833	0.58%	0.065%
5	4.046	177	180	184	rVB	14766	18161	0.24%	0.027%
6	7.046	684	690	702	rVB	159407	301014	3.95%	0.445%
7	7.211	711	718	733	rVB	728095	1179540	15.48%	1.745%
8	7.411	744	752	763	rBV	647470	1079270	14.17%	1.596%
9	7.875	824	831	841	rBV	873627	1424447	18.70%	2.107%
10	8.593	946	953	970	rBV	478029	865166	11.35%	1.280%
11	9.046	1022	1030	1042	rBV	788257	1320546	17.33%	1.953%
12	9.452	1094	1099	1107	rVB5	5968	13431	0.18%	0.020%
13	9.769	1145	1153	1168	rBV	562013	984303	12.92%	1.456%
14	10.305	1237	1244	1264	rBV	836315	1596667	20.96%	2.362%
15	10.481	1269	1274	1289	rVB5	14277	48528	0.64%	0.072%
16	10.687	1301	1309	1322	rVB	1238044	2091284	27.45%	3.093%
17	10.828	1326	1333	1359	rBV	713321	1444495	18.96%	2.136%
18	12.275	1574	1579	1589	rVB	18414	36592	0.48%	0.054%
19	12.557	1622	1627	1634	rVB10	7057	13905	0.18%	0.021%
20	13.422	1769	1774	1781	rVB2	14118	24746	0.32%	0.037%
21	13.493	1783	1786	1790	rBV5	5361	7735	0.10%	0.011%
22	13.934	1855	1861	1877	rBV	1999651	2859825	37.53%	4.230%
23	14.216	1902	1909	1926	rBV	2267201	3351428	43.99%	4.957%
24	14.528	1954	1962	1975	rBV	1762893	2774183	36.41%	4.103%
25	14.740	1992	1998	2011	rBV2	74472	214360	2.81%	0.317%
26	14.946	2030	2033	2041	rVB9	11262	22794	0.30%	0.034%
27	15.522	2122	2131	2144	rBV	3138560	4763793	62.52%	7.046%
28	15.640	2144	2151	2167	rVV	885621	1297986	17.04%	1.920%
29	15.763	2168	2172	2183	rVB3	16779	34283	0.45%	0.051%
30	16.240	2249	2253	2261	rVB10	6727	14269	0.19%	0.021%
31	17.045	2385	2390	2391	rBV5	9161	12661	0.17%	0.019%
32	17.281	2424	2430	2441	rBV	2474634	3415947	44.83%	5.052%
33	17.381	2441	2447	2472	rVB	4074430	5798134	76.10%	8.576%
34	17.945	2541	2543	2550	rVB7	8406	12139	0.16%	0.018%
35	18.163	2575	2580	2589	rBV	139929	229065	3.01%	0.339%
36	19.192	2751	2755	2762	rBV	54722	76991	1.01%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011977.D
Acq On : 06 Oct 2022 19:09
Operator : CG/JU
Sample : N4923-14
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10013

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37	19.263	2763	2767	2769	rBV	59041	76133	1.00%	0.113%
38	19.398	2786	2790	2800	rBV2	101322	181741	2.39%	0.269%
39	19.616	2821	2827	2839	rBV	5574747	7163478	94.02%	10.595%
40	21.075	3072	3075	3081	rBV3	130172	184627	2.42%	0.273%
41	21.369	3120	3125	3135	rBV	3073112	4046213	53.11%	5.984%
42	23.639	3504	3511	3524	rVB2	3661363	7619263	100.00%	11.269%
43	23.792	3531	3537	3549	rVB2	2030526	4164004	54.65%	6.159%




Sum of corrected areas: 67611912

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011977.D
Acq On : 06 Oct 2022 19:09
Operator : CG/JU
Sample : N4923-14
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

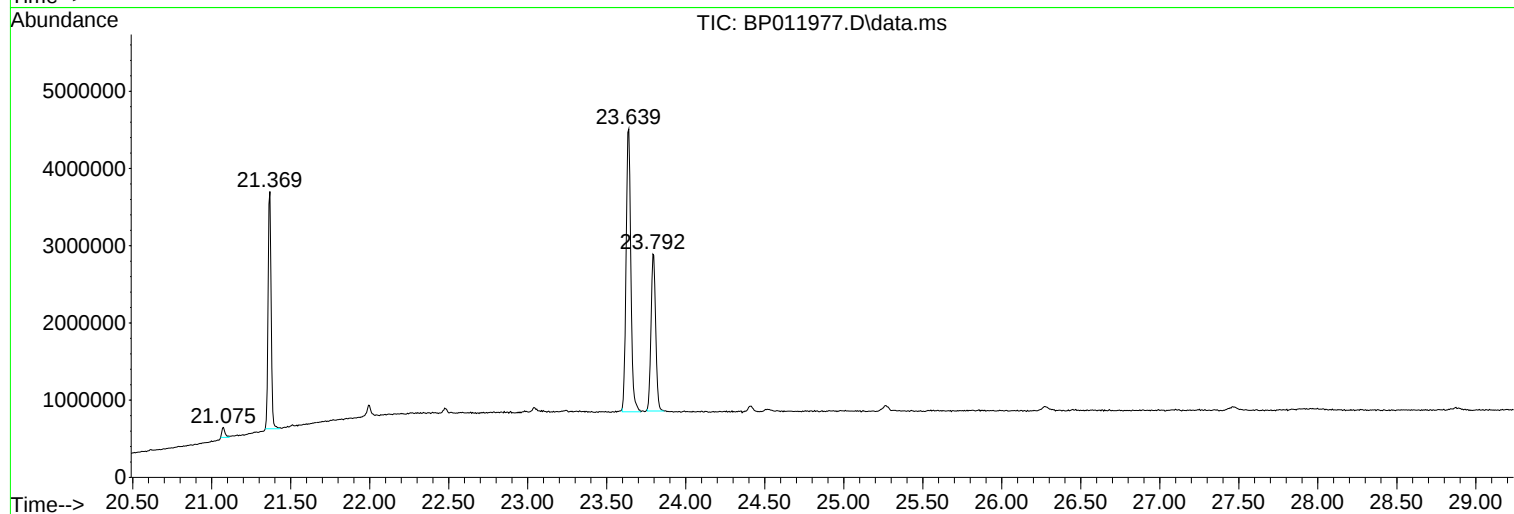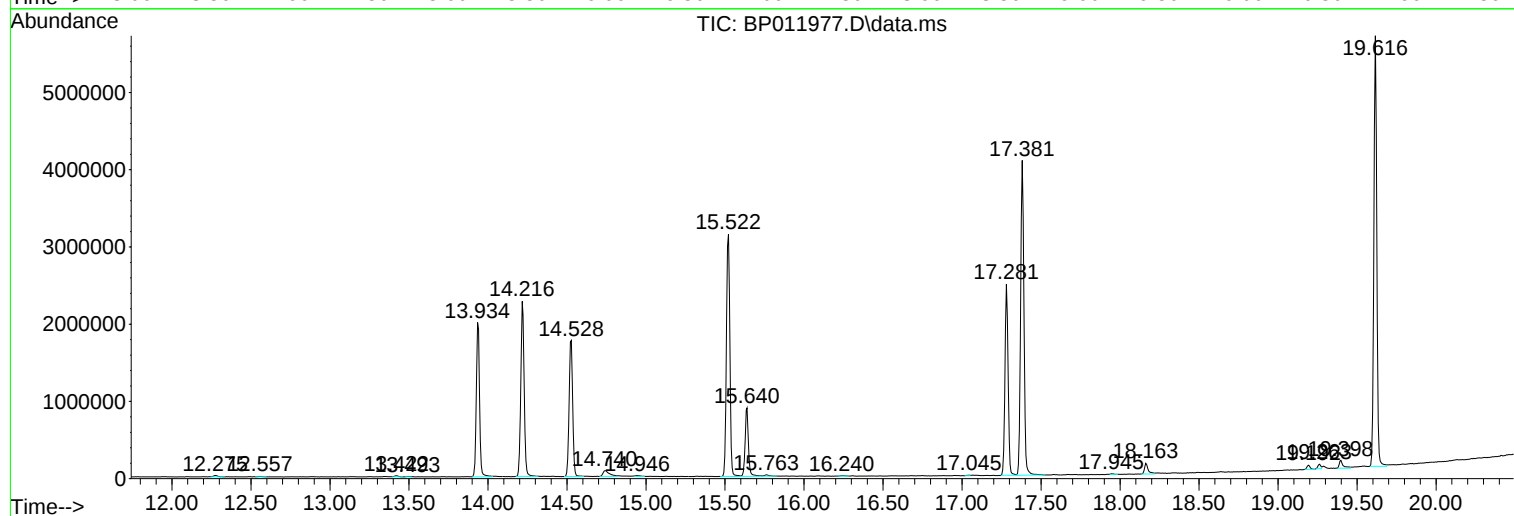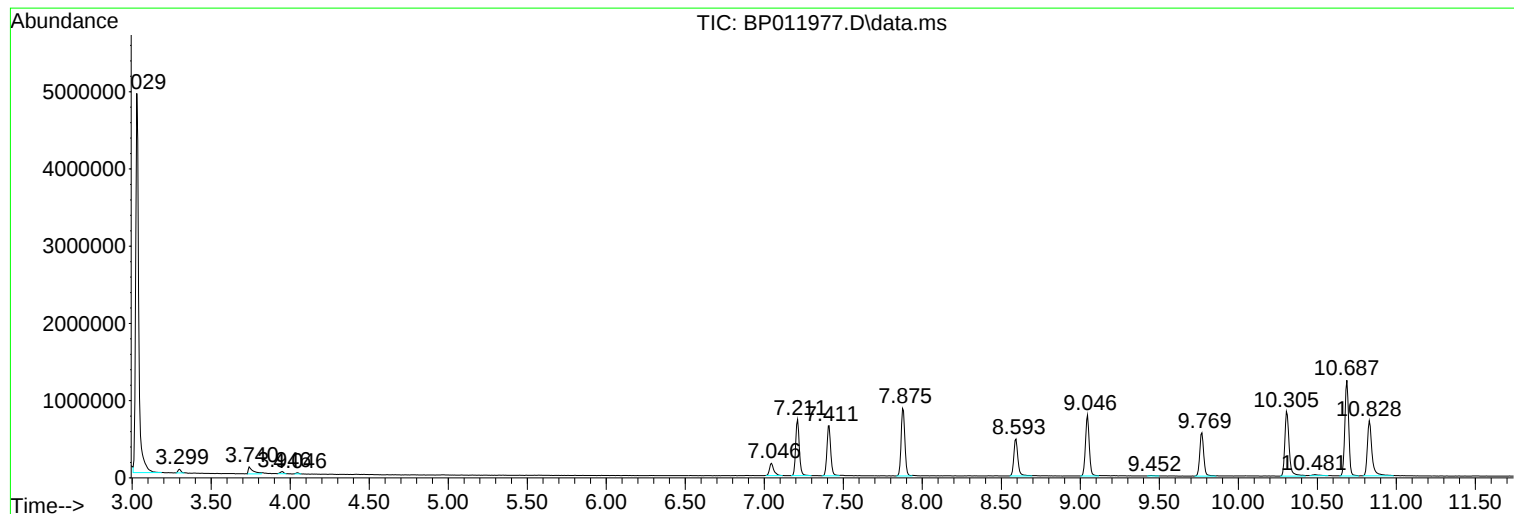

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011977.D
Acq On : 06 Oct 2022 19:09
Operator : CG/JU
Sample : N4923-14
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10013










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.029	91.95 ng/ul	6549210	1,4-Dichlorobenzene-d4	7.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43		
4	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		
5	N-Ethylformamide	73	C3H7NO	000627-45-2	9		

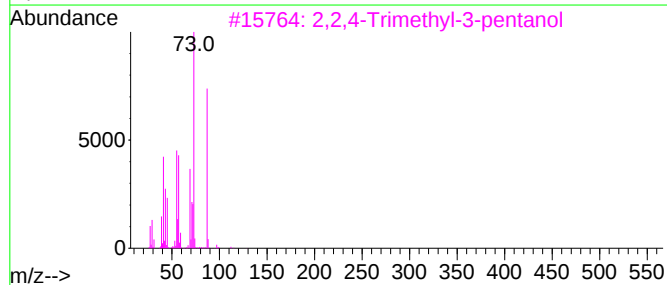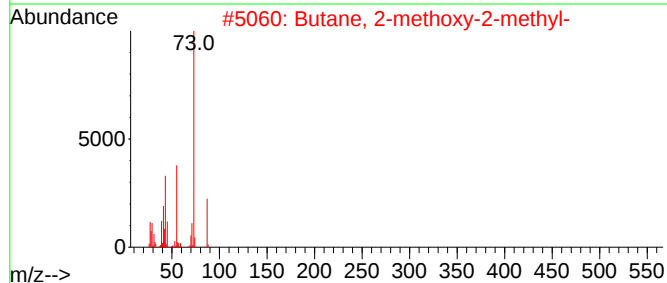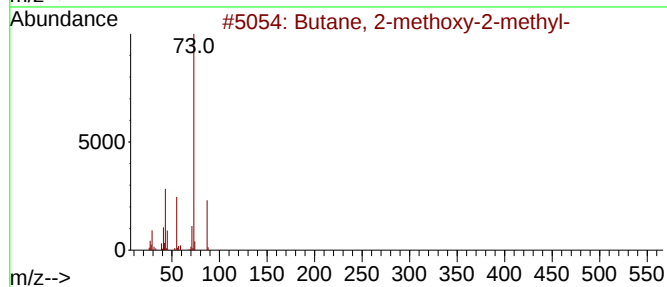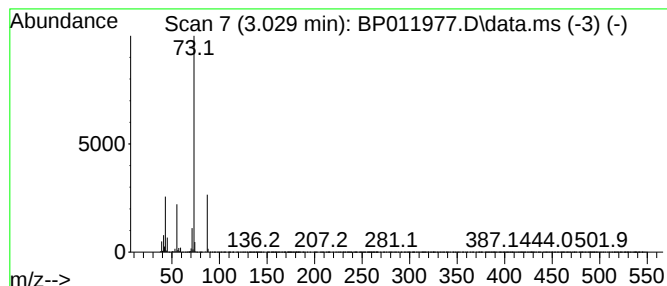

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011977.D
Acq On : 06 Oct 2022 19:09
Operator : CG/JU
Sample : N4923-14
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.029	92.0	ng/ul	6549210	1	7.875	1424450	20.0