

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011978.D
 Acq On : 06 Oct 2022 19:44
 Operator : CG/JU
 Sample : N4923-12
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	29	rVB	4981456	6405572	100.00%	10.619%
2	3.299	49	53	58	rVB	43838	51867	0.81%	0.086%
3	3.734	125	127	140	rBV	95180	181136	2.83%	0.300%
4	3.946	160	163	168	rVB	28885	38187	0.60%	0.063%
5	4.046	177	180	186	rVB	16834	22317	0.35%	0.037%
6	7.046	683	690	700	rBV	147882	272672	4.26%	0.452%
7	7.210	711	718	732	rBV	697687	1145209	17.88%	1.899%
8	7.410	744	752	762	rBV	622403	1045621	16.32%	1.733%
9	7.875	824	831	841	rBV	833275	1353126	21.12%	2.243%
10	8.593	945	953	972	rBV	416117	748841	11.69%	1.241%
11	9.046	1022	1030	1046	rBV	761948	1308440	20.43%	2.169%
12	9.452	1092	1099	1102	rBV5	6516	10790	0.17%	0.018%
13	9.769	1145	1153	1166	rBV	553232	966009	15.08%	1.601%
14	10.304	1237	1244	1266	rBV	798290	1516575	23.68%	2.514%
15	10.687	1300	1309	1324	rVB	1154542	1987513	31.03%	3.295%
16	10.828	1326	1333	1360	rBV	552347	1142369	17.83%	1.894%
17	12.275	1574	1579	1587	rVV	16285	32658	0.51%	0.054%
18	12.557	1621	1627	1634	rBV4	28922	51598	0.81%	0.086%
19	12.716	1649	1654	1657	rBV6	5727	10096	0.16%	0.017%
20	13.322	1752	1757	1758	rBV5	4816	6698	0.10%	0.011%
21	13.345	1758	1761	1767	rVV7	5496	13737	0.21%	0.023%
22	13.416	1769	1773	1780	rVB6	13245	24658	0.38%	0.041%
23	13.934	1853	1861	1875	rBV	1776069	2561423	39.99%	4.246%
24	14.216	1902	1909	1930	rBV	2194485	3173788	49.55%	5.262%
25	14.522	1955	1961	1970	rBV	1691929	2578490	40.25%	4.275%
26	14.581	1970	1971	1976	rVB3	8475	9622	0.15%	0.016%
27	14.745	1993	1999	2013	rBV2	61478	188012	2.94%	0.312%
28	14.839	2013	2015	2021	rVB7	7542	10700	0.17%	0.018%
29	14.928	2026	2030	2033	rBV3	8016	13665	0.21%	0.023%
30	15.516	2123	2130	2144	rBV	2966991	4413781	68.91%	7.317%
31	15.639	2145	2151	2166	rVV	765425	1133123	17.69%	1.878%
32	15.763	2168	2172	2178	rVB2	13781	24053	0.38%	0.040%
33	16.304	2261	2264	2269	rBV6	5175	6980	0.11%	0.012%
34	16.822	2349	2352	2358	rBV8	4697	8380	0.13%	0.014%
35	17.281	2423	2430	2440	rBV	2142456	3085226	48.16%	5.115%
36	17.381	2440	2447	2464	rVV2	3373728	4873249	76.08%	8.079%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011978.D
 Acq On : 06 Oct 2022 19:44
 Operator : CG/JU
 Sample : N4923-12
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	18.163	2575	2580	2589	rBV3	79619	139994	2.19%	0.232%
38	18.639	2658	2661	2667	rBV5	17742	26055	0.41%	0.043%
39	19.192	2752	2755	2761	rVB2	42238	54415	0.85%	0.090%
40	19.263	2763	2767	2771	rBV	51240	76682	1.20%	0.127%
41	19.398	2787	2790	2797	rBV5	39646	57969	0.90%	0.096%
42	19.616	2821	2827	2835	rBV	4591650	5986378	93.46%	9.924%
43	21.074	3072	3075	3079	rBV4	95733	138572	2.16%	0.230%
44	21.369	3120	3125	3134	rBV	2644285	3513492	54.85%	5.825%
45	23.639	3504	3511	3523	rVB2	3215979	6332147	98.85%	10.497%
46	23.798	3531	3538	3548	rVB	1754639	3579080	55.87%	5.933%




Sum of corrected areas: 60320965

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011978.D
Acq On : 06 Oct 2022 19:44
Operator : CG/JU
Sample : N4923-12
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

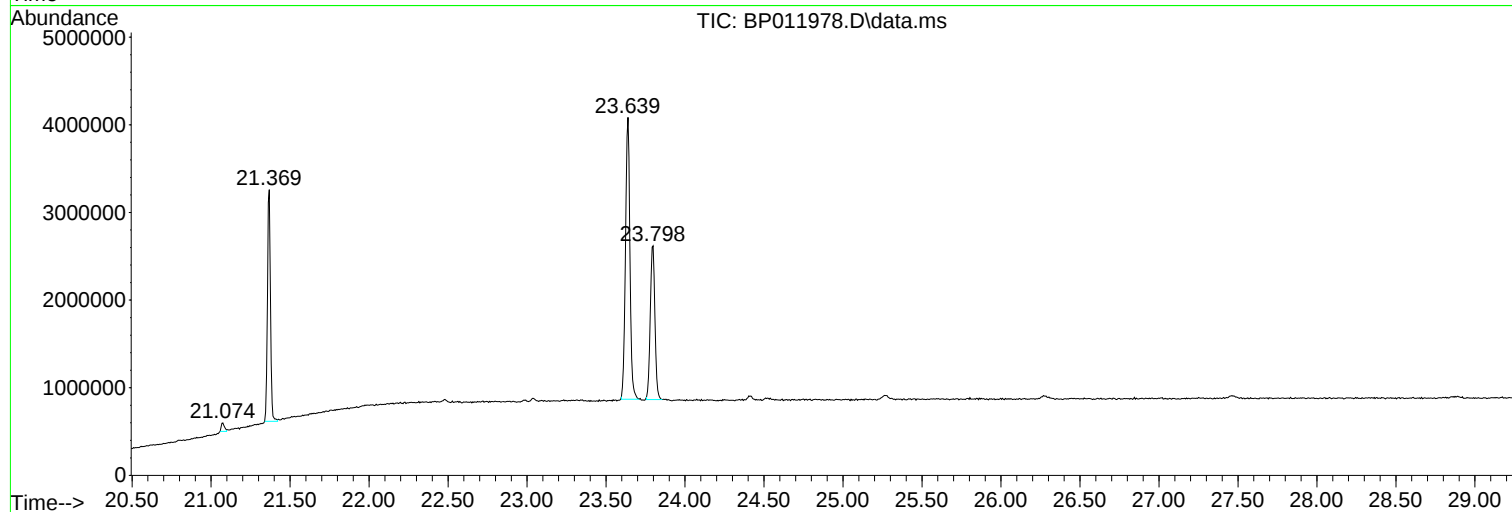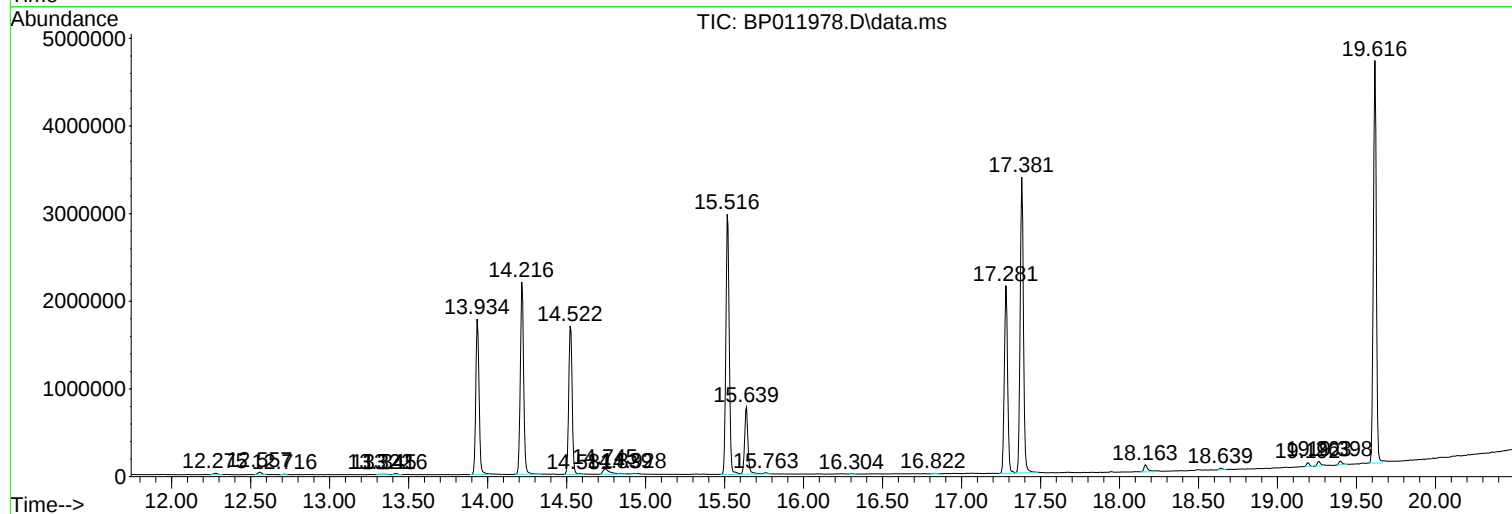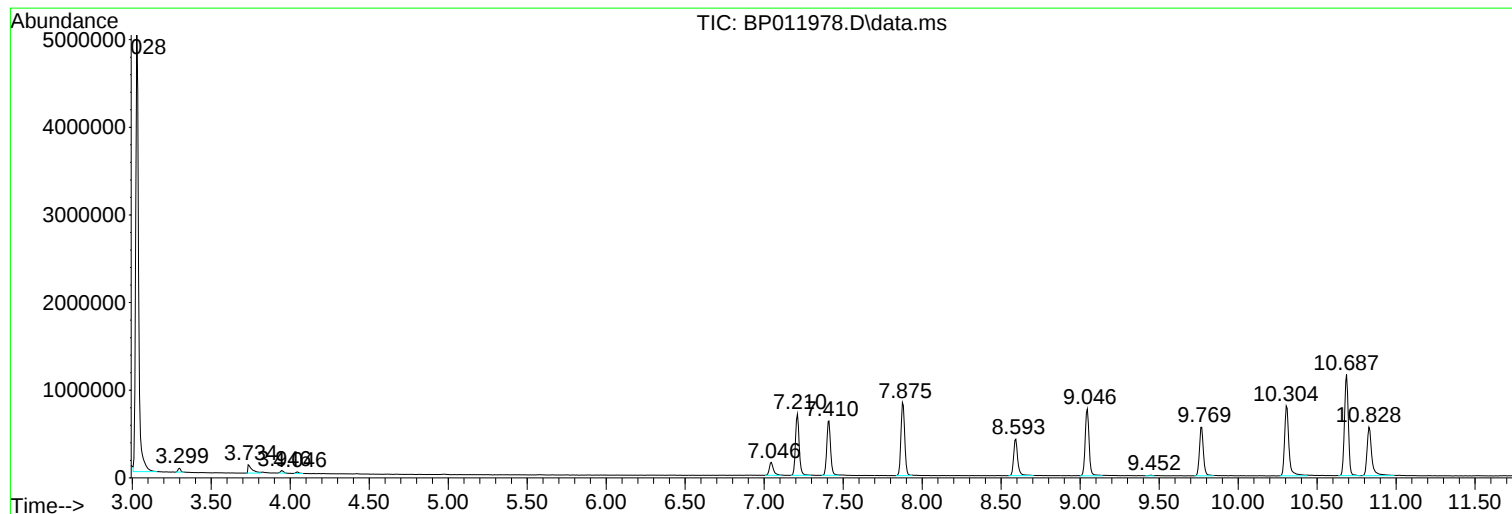

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011978.D
Acq On : 06 Oct 2022 19:44
Operator : CG/JU
Sample : N4923-12
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10041










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	94.68 ng/ul	6405570	1,4-Dichlorobenzene-d4	7.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43		
4	N-Ethylformamide	73	C3H7NO	000627-45-2	9		
5	Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9		

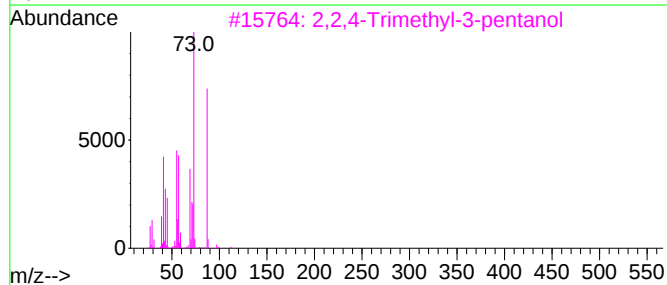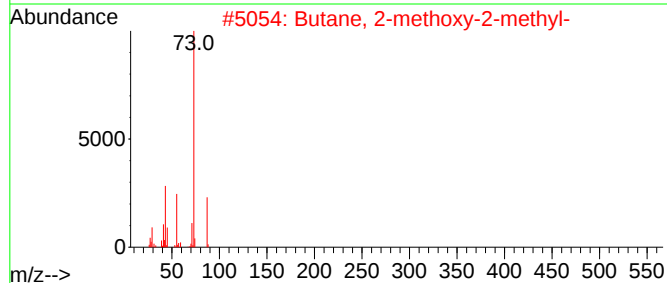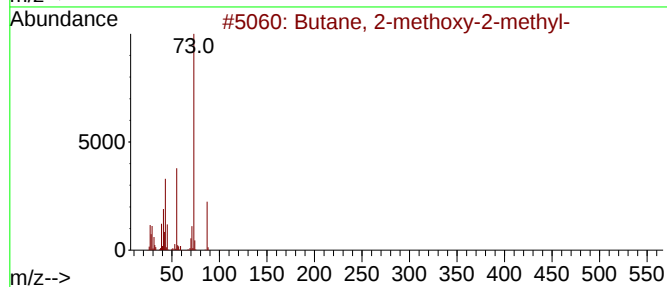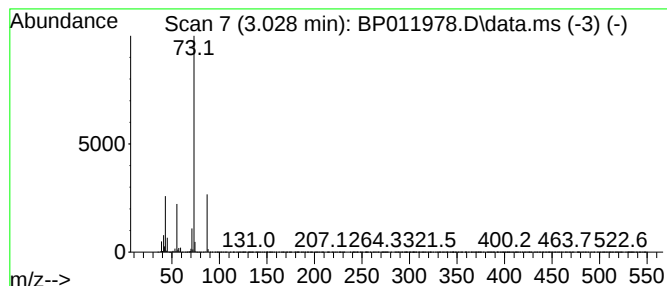

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011978.D
Acq On : 06 Oct 2022 19:44
Operator : CG/JU
Sample : N4923-12
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	94.7	ng/ul	6405570	1	7.875	1353130	20.0