

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011985.D
 Acq On : 06 Oct 2022 23:45
 Operator : CG/JU
 Sample : PB147981BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK981

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	7	10	16	rVB	159543	190449	5.54%	0.924%
2	3.122	20	23	26	rVV	42177	48591	1.41%	0.236%
3	3.152	26	28	30	rVV2	21977	21479	0.63%	0.104%
4	3.175	30	32	35	rVV	28399	33573	0.98%	0.163%
5	3.217	35	39	49	rVB	2050502	2144793	62.41%	10.407%
6	3.558	93	97	104	rVB	63790	78591	2.29%	0.381%
7	4.040	175	179	184	rBV	25099	34248	1.00%	0.166%
8	4.234	210	212	216	rBV3	5068	6113	0.18%	0.030%
9	4.981	337	339	345	rVB4	5805	5794	0.17%	0.028%
10	7.875	824	831	846	rBV	1258841	2083752	60.64%	10.111%
11	8.281	898	900	907	rVB8	2080	3912	0.11%	0.019%
12	8.716	970	974	981	rBV8	1785	3630	0.11%	0.018%
13	10.681	1297	1308	1327	rBV	1566208	2855951	83.11%	13.857%
14	13.251	1739	1745	1751	rBV8	3572	8182	0.24%	0.040%
15	14.522	1954	1961	1977	rBV	2311186	3422248	99.59%	16.605%
16	15.098	2055	2059	2062	rBV6	2049	3853	0.11%	0.019%
17	17.281	2423	2430	2451	rBV	2222532	3436486	100.00%	16.674%
18	21.363	3120	3124	3134	rBV	2282708	3023990	88.00%	14.673%
19	23.792	3531	3537	3549	rVB2	1584916	3203813	93.23%	15.545%




Sum of corrected areas: 20609448

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011985.D
Acq On : 06 Oct 2022 23:45
Operator : CG/JU
Sample : PB147981BL
Misc : GCMS CONFIRMATION
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

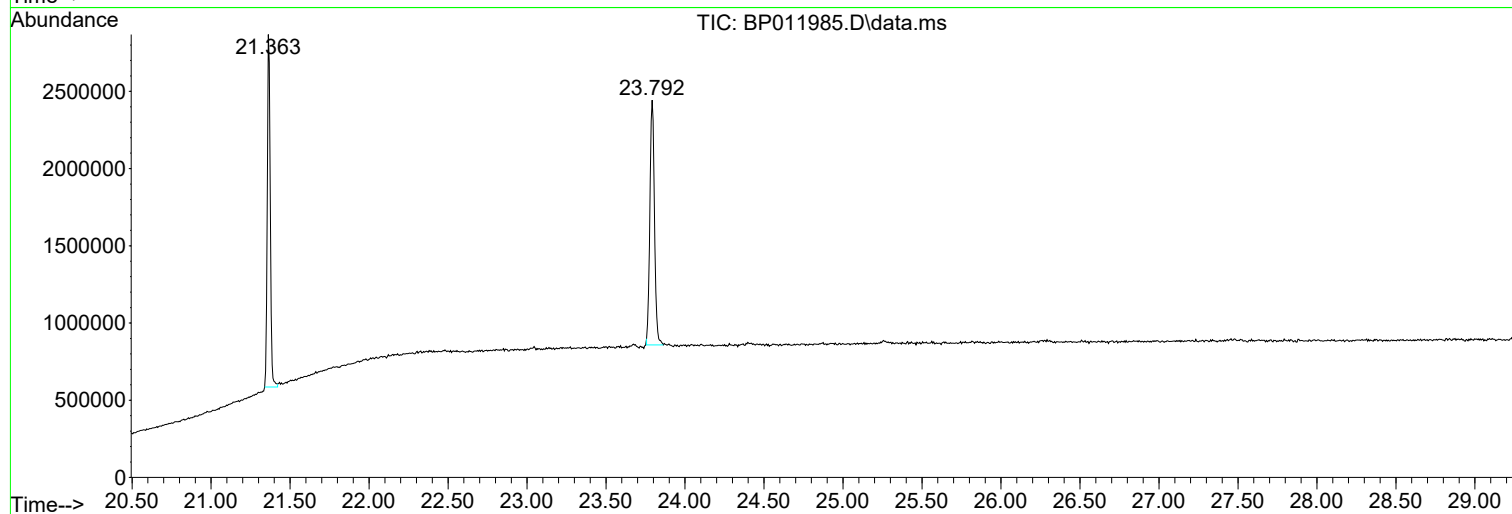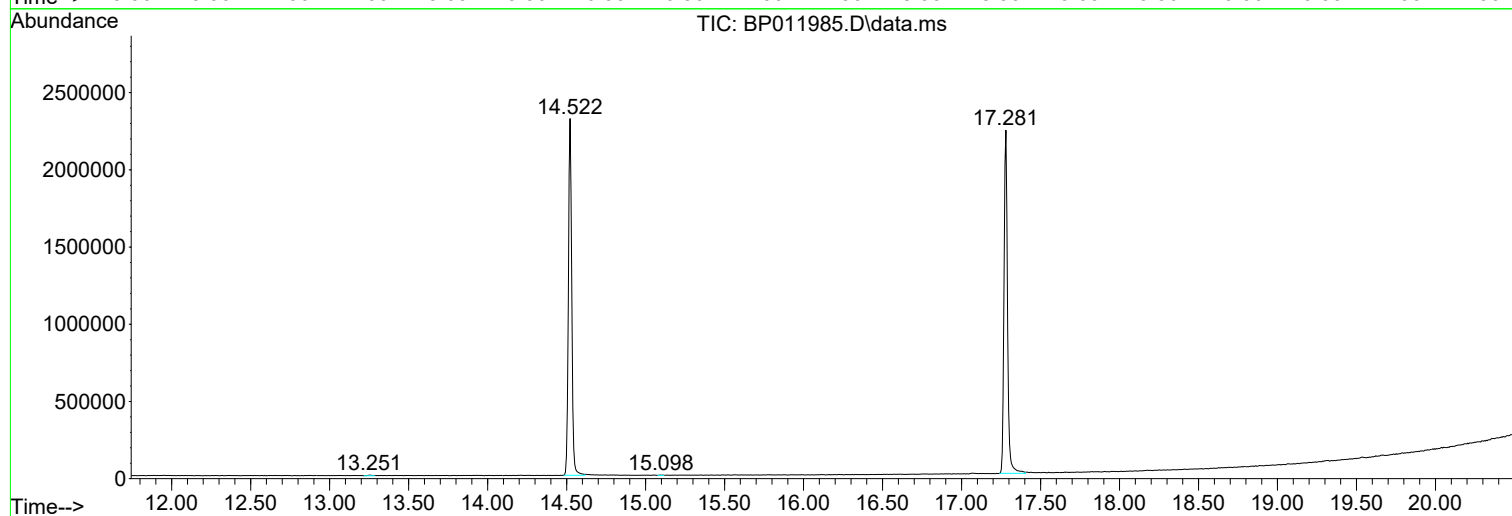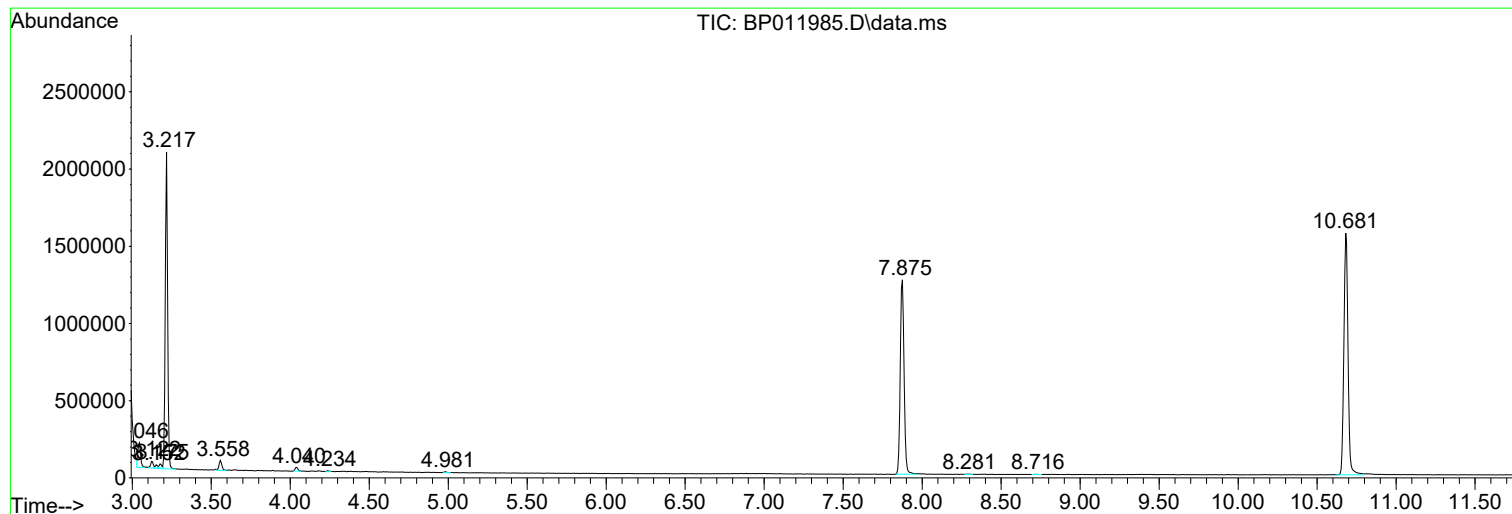

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011985.D
Acq On : 06 Oct 2022 23:45
Operator : CG/JU
Sample : PB147981BL
Misc : GCMS CONFIRMATION
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK981










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.217	20.59 ng/ul	2144790	1,4-Dichlorobenzene-d4	7.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	95
2			Heptane	100	C7H16	000142-82-5	91
3			Heptane	100	C7H16	000142-82-5	91
4			Heptane	100	C7H16	000142-82-5	68
5			Pentane, 2-methyl-	86	C6H14	000107-83-5	53

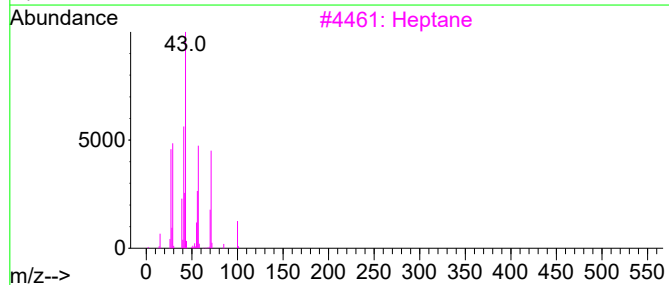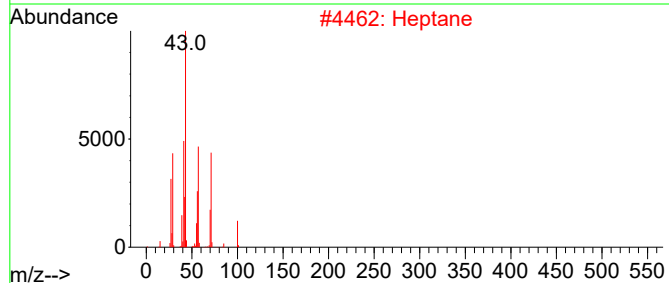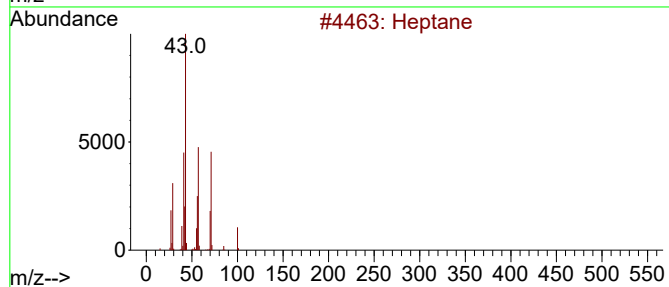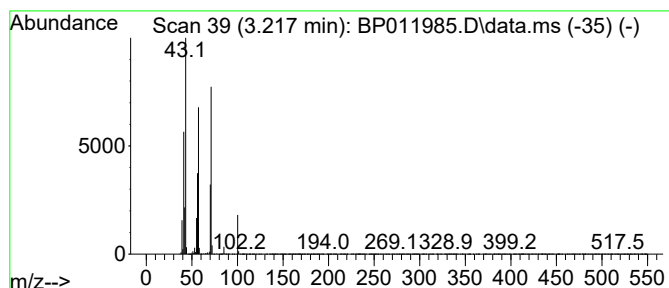

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011985.D
Acq On : 06 Oct 2022 23:45
Operator : CG/JU
Sample : PB147981BL
Misc : GCMS CONFIRMATION
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.217	20.6	ng/ul	2144790	1	7.875	2083750	20.0