

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011987.D
 Acq On : 07 Oct 2022 00:54
 Operator : CG/JU
 Sample : N4806-08
 Misc : GCMS CONFIRMATION
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0B07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	7	10	18	rVB	273183	329155	7.42%	1.201%
2	3.128	21	24	27	rVV	85936	95690	2.16%	0.349%
3	3.158	27	29	31	rVV	44154	44234	1.00%	0.161%
4	3.181	31	33	35	rVV2	59461	59573	1.34%	0.217%
5	3.222	35	40	51	rVB	3967139	4434869	100.00%	16.184%
6	3.528	89	92	94	rBV3	15084	18464	0.42%	0.067%
7	3.564	94	98	103	rVB	135404	166295	3.75%	0.607%
8	4.040	175	179	186	rVB	28481	41517	0.94%	0.152%
9	5.175	367	372	377	rBV4	5967	11336	0.26%	0.041%
10	6.358	569	573	578	rVB5	5502	9595	0.22%	0.035%
11	6.511	594	599	608	rBV3	16192	29420	0.66%	0.107%
12	6.952	672	674	681	rBV6	3386	6276	0.14%	0.023%
13	7.763	807	812	815	rBV6	4611	7507	0.17%	0.027%
14	7.875	823	831	846	rBV	1224399	2043432	46.08%	7.457%
15	10.463	1265	1271	1275	rVB9	4300	8821	0.20%	0.032%
16	10.634	1293	1300	1301	rBV7	5873	10003	0.23%	0.037%
17	10.681	1301	1308	1326	rVV	1610705	2806683	63.29%	10.242%
18	10.934	1346	1351	1355	rBV7	5066	8166	0.18%	0.030%
19	11.081	1374	1376	1382	rVB7	4561	7796	0.18%	0.028%
20	11.146	1382	1387	1389	rBV6	5145	8250	0.19%	0.030%
21	11.704	1478	1482	1488	rBV9	2363	4446	0.10%	0.016%
22	12.357	1588	1593	1600	rBV4	6153	12669	0.29%	0.046%
23	12.575	1622	1630	1634	rBV3	6046	12774	0.29%	0.047%
24	13.251	1741	1745	1750	rBV5	3328	4540	0.10%	0.017%
25	13.340	1750	1760	1770	rVV5	6775	18641	0.42%	0.068%
26	13.557	1793	1797	1799	rBV5	3628	6257	0.14%	0.023%
27	13.581	1799	1801	1807	rVB6	3811	6484	0.15%	0.024%
28	13.840	1839	1845	1852	rBV3	11462	23142	0.52%	0.084%
29	13.893	1852	1854	1858	rVV5	4589	5747	0.13%	0.021%
30	14.075	1882	1885	1889	rBV4	5124	7309	0.16%	0.027%
31	14.245	1909	1914	1921	rBV3	14537	28147	0.63%	0.103%
32	14.304	1921	1924	1927	rBV5	5413	5601	0.13%	0.020%
33	14.351	1928	1932	1936	rVB6	4837	7249	0.16%	0.026%
34	14.416	1939	1943	1946	rBV5	6671	8914	0.20%	0.033%
35	14.522	1950	1961	1970	rBV	2260402	3383897	76.30%	12.349%
36	14.840	2012	2015	2020	rBV6	5819	9436	0.21%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011987.D
 Acq On : 07 Oct 2022 00:54
 Operator : CG/JU
 Sample : N4806-08
 Misc : GCMS CONFIRMATION
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0B07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	14.922	2025	2029	2035	rVB2	11969	20219	0.46%	0.074%
38	15.140	2063	2066	2069	rBV3	7116	10222	0.23%	0.037%
39	15.310	2090	2095	2101	rBV7	10573	19178	0.43%	0.070%
40	15.575	2135	2140	2145	rBV2	32529	56295	1.27%	0.205%
41	15.781	2172	2175	2180	rBV4	16088	21290	0.48%	0.078%
42	15.869	2187	2190	2195	rVB	12985	20107	0.45%	0.073%
43	16.810	2347	2350	2353	rBV4	23689	25475	0.57%	0.093%
44	17.281	2424	2430	2434	rBV	2214751	3347990	75.49%	12.218%
45	17.322	2434	2437	2447	rVB	416736	620510	13.99%	2.264%
46	17.992	2547	2551	2557	rBV2	65954	92603	2.09%	0.338%
47	18.069	2560	2564	2572	rVB	130425	174922	3.94%	0.638%
48	18.145	2574	2577	2581	rVV	68753	106293	2.40%	0.388%
49	18.192	2582	2585	2591	rVB	85675	133559	3.01%	0.487%
50	18.333	2604	2609	2613	rBV2	139745	216127	4.87%	0.789%
51	18.392	2616	2619	2622	rVV	118291	154094	3.47%	0.562%
52	18.433	2622	2626	2632	rVB	199626	260396	5.87%	0.950%
53	19.286	2766	2771	2778	rBV	725360	971934	21.92%	3.547%
54	19.610	2823	2826	2828	rBV2	74959	102903	2.32%	0.376%
55	19.639	2828	2831	2838	rVB	293004	394690	8.90%	1.440%
56	20.116	2909	2912	2918	rVB2	200552	290642	6.55%	1.061%
57	20.222	2927	2930	2934	rBV	74532	97084	2.19%	0.354%
58	20.380	2955	2957	2961	rVB	110182	119735	2.70%	0.437%
59	21.363	3119	3124	3129	rBV	2408427	3448475	77.76%	12.584%
60	23.792	3531	3537	3547	rVB2	1472936	3005696	67.77%	10.969%




Sum of corrected areas: 27402774

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011987.D
Acq On : 07 Oct 2022 00:54
Operator : CG/JU
Sample : N4806-08
Misc : GCMS CONFIRMATION
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0B07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

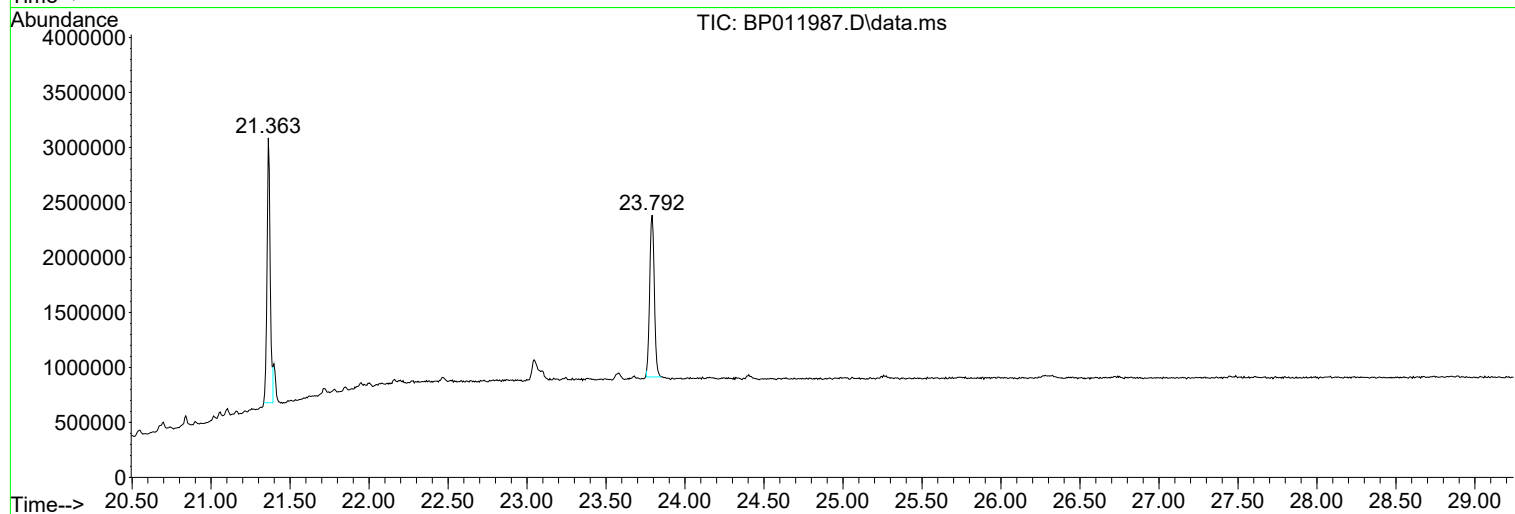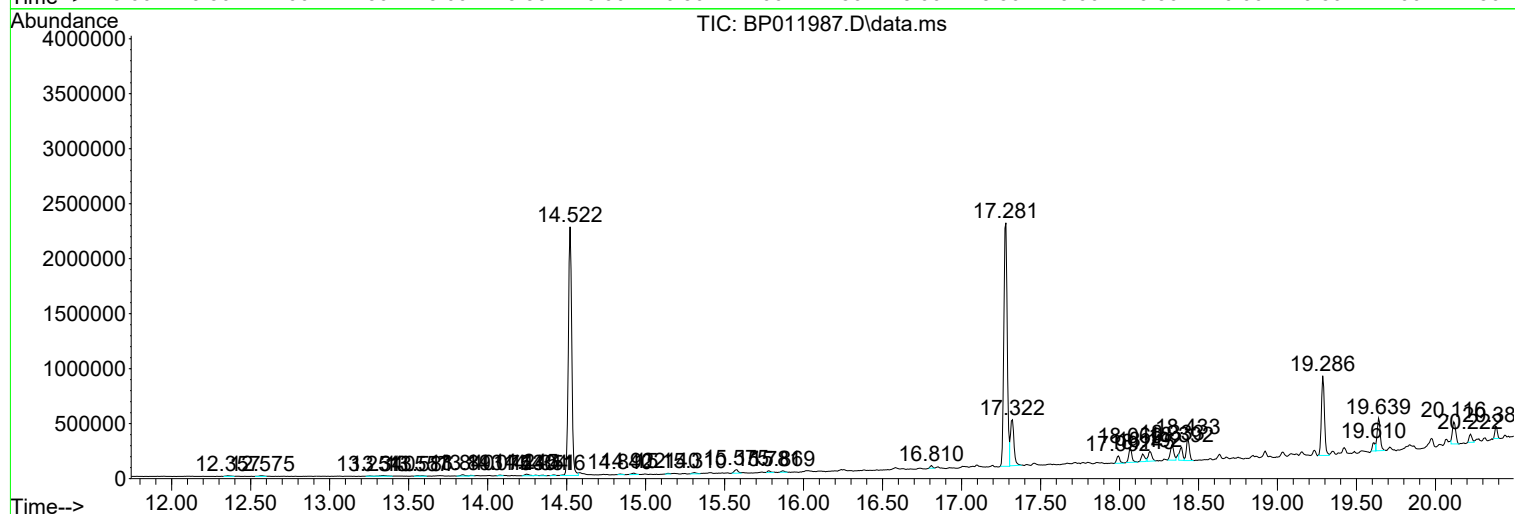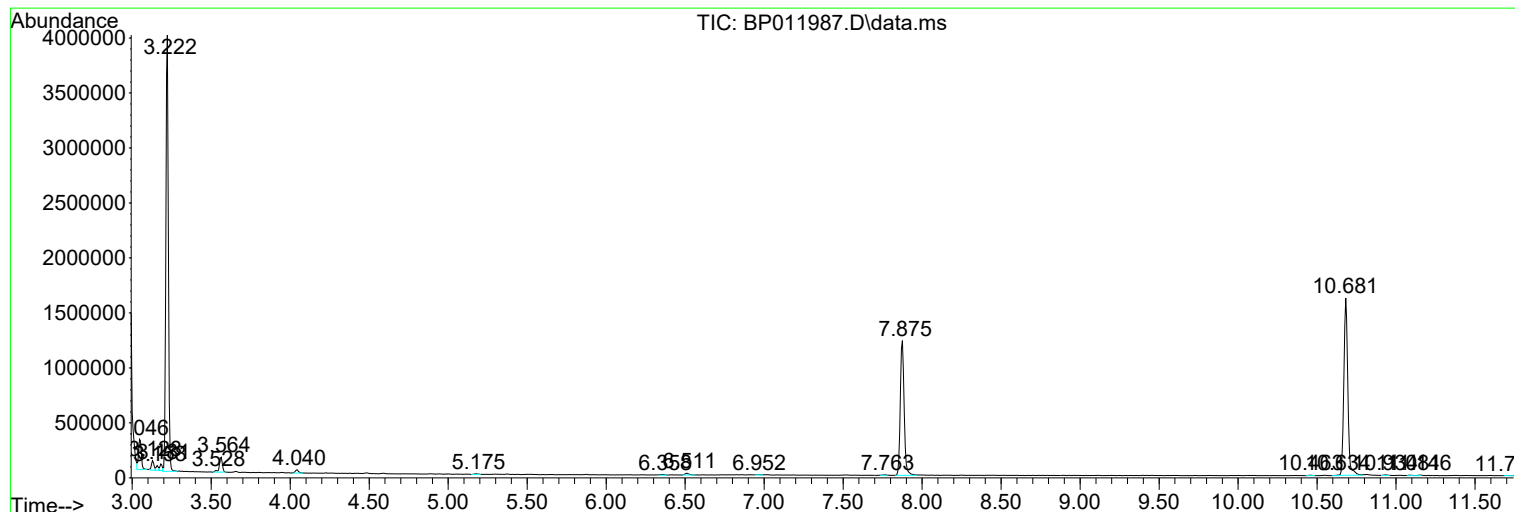

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011987.D
Acq On : 07 Oct 2022 00:54
Operator : CG/JU
Sample : N4806-08
Misc : GCMS CONFIRMATION
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0B07










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.046 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.046	3.22 ng/ul	329155	1,4-Dichlorobenzene-d4	7.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentane, 1,1-dimethyl-	98	C7H14	001638-26-2	83
2			Cyclopentane, 1,1-dimethyl-	98	C7H14	001638-26-2	74
3			3-Undecene, 8-methyl-	168	C12H24	1000061-84-4	53
4			4-Nonene, 5-methyl-	140	C10H20	015918-07-7	50
5			1-Hexene, 3-methyl-	98	C7H14	003404-61-3	47

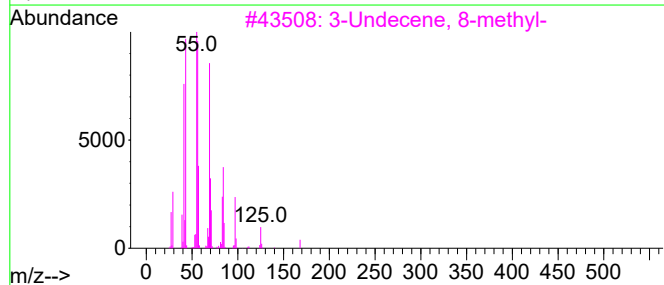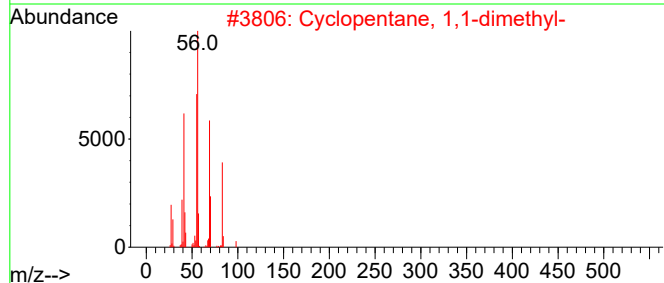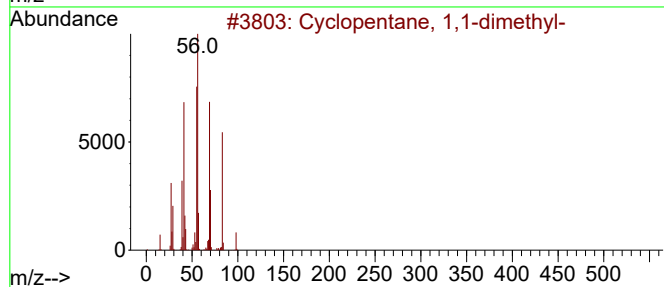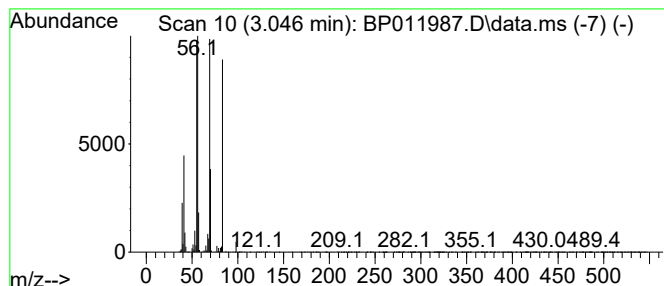

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011987.D
Acq On : 07 Oct 2022 00:54
Operator : CG/JU
Sample : N4806-08
Misc : GCMS CONFIRMATION
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0B07










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.222	43.41 ng/ul	4434870	1,4-Dichlorobenzene-d4	7.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	94
2			Heptane	100	C7H16	000142-82-5	91
3			Heptane	100	C7H16	000142-82-5	91
4			Heptane	100	C7H16	000142-82-5	91
5			Hexane, 3-methyl-	100	C7H16	000589-34-4	47

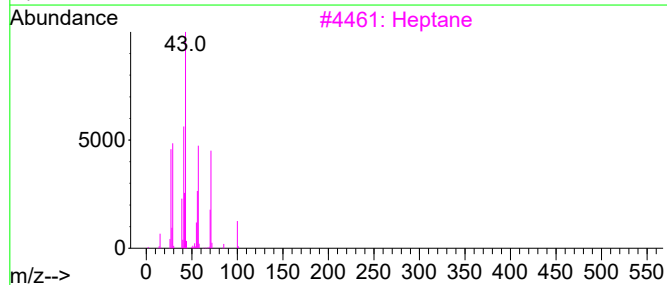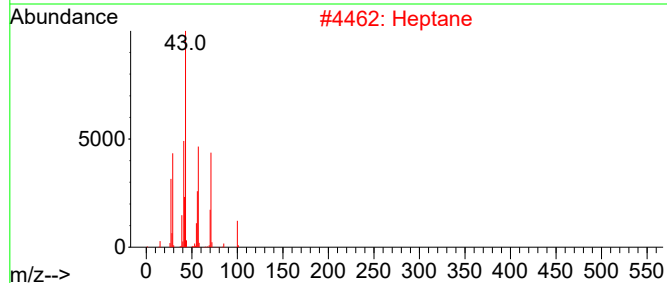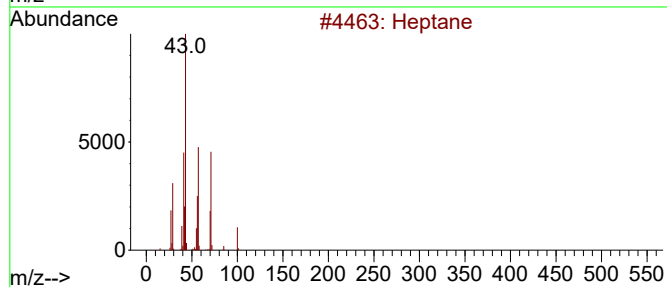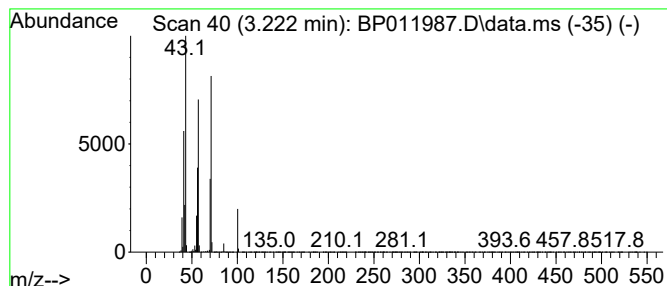

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011987.D
Acq On : 07 Oct 2022 00:54
Operator : CG/JU
Sample : N4806-08
Misc : GCMS CONFIRMATION
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0B07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.046	3.2	ng/u1	329155	1	7.875	2043430	20.0
(DEL) Alkane: S...	3.222	43.4	ng/u1	4434870	1	7.875	2043430	20.0