

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
 Data File : BP011990.D
 Acq On : 07 Oct 2022 03:11
 Operator : CG/JU
 Sample : PB148079BL
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK079

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	21	rVB	181814	244261	3.68%	0.375%
2	3.293	49	52	61	rVB	76199	104420	1.57%	0.160%
3	3.717	122	124	141	rBV	844070	1277761	19.27%	1.961%
4	4.046	176	180	184	rVB	12821	16931	0.26%	0.026%
5	7.040	682	689	702	rBV	1018652	1697859	25.60%	2.606%
6	7.205	711	717	729	rBV	916871	1458548	21.99%	2.239%
7	7.405	742	751	765	rBV	1085537	1775999	26.78%	2.726%
8	7.875	823	831	843	rBV	714489	1162071	17.52%	1.784%
9	8.587	944	952	968	rBV	1306281	2193002	33.06%	3.366%
10	9.040	1022	1029	1043	rBV	1000478	1669229	25.17%	2.562%
11	9.763	1143	1152	1170	rBV	774251	1306481	19.70%	2.006%
12	10.299	1236	1243	1265	rBV	1177527	2199184	33.16%	3.376%
13	10.681	1301	1308	1320	rBV	1026825	1741198	26.25%	2.673%
14	10.822	1324	1332	1360	rBV	1251196	2301897	34.71%	3.534%
15	12.275	1572	1579	1587	rBV2	19999	44207	0.67%	0.068%
16	13.416	1768	1773	1780	rBV4	20043	32578	0.49%	0.050%
17	13.493	1780	1786	1791	rBV6	3646	7321	0.11%	0.011%
18	13.934	1851	1861	1875	rBV	2184320	3193782	48.15%	4.903%
19	14.210	1901	1908	1924	rBV	2643825	4082012	61.55%	6.266%
20	14.522	1954	1961	1972	rBV	1565056	2376834	35.84%	3.649%
21	14.722	1989	1995	2022	rBV	777993	1533974	23.13%	2.355%
22	15.516	2123	2130	2143	rBV	3623831	5268855	79.44%	8.088%
23	15.634	2144	2150	2160	rVV	878041	1239248	18.68%	1.902%
24	15.757	2167	2171	2179	rVB3	16271	28498	0.43%	0.044%
25	16.304	2261	2264	2270	rVB8	4388	8014	0.12%	0.012%
26	16.951	2371	2374	2379	rBV6	4559	7515	0.11%	0.012%
27	17.057	2390	2392	2398	rVB7	4329	7519	0.11%	0.012%
28	17.275	2423	2429	2440	rBV	1915086	2859075	43.11%	4.389%
29	17.375	2440	2446	2466	rVV	3954516	5796241	87.39%	8.898%
30	19.192	2751	2755	2759	rBV2	43367	58244	0.88%	0.089%
31	19.257	2763	2766	2770	rVV	45089	56039	0.84%	0.086%
32	19.610	2821	2826	2835	rBV	4923953	6618393	99.79%	10.160%
33	21.363	3119	3124	3135	rBV	2421046	3151733	47.52%	4.838%
34	23.633	3503	3510	3527	rVB2	3208801	6632401	100.00%	10.181%
35	23.792	3531	3537	3546	rVB	1539211	2992359	45.12%	4.593%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011990.D
Acq On : 07 Oct 2022 03:11
Operator : CG/JU
Sample : PB148079BL
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK079

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION




Sum of corrected areas: 65143683

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011990.D
Acq On : 07 Oct 2022 03:11
Operator : CG/JU
Sample : PB148079BL
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK079

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

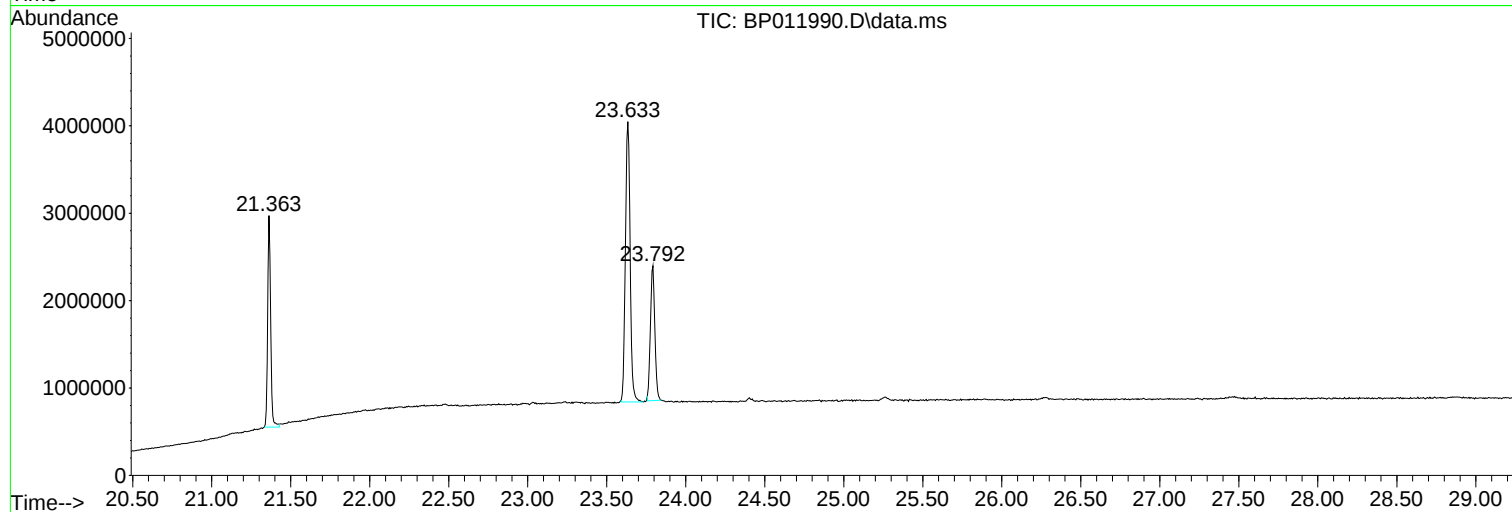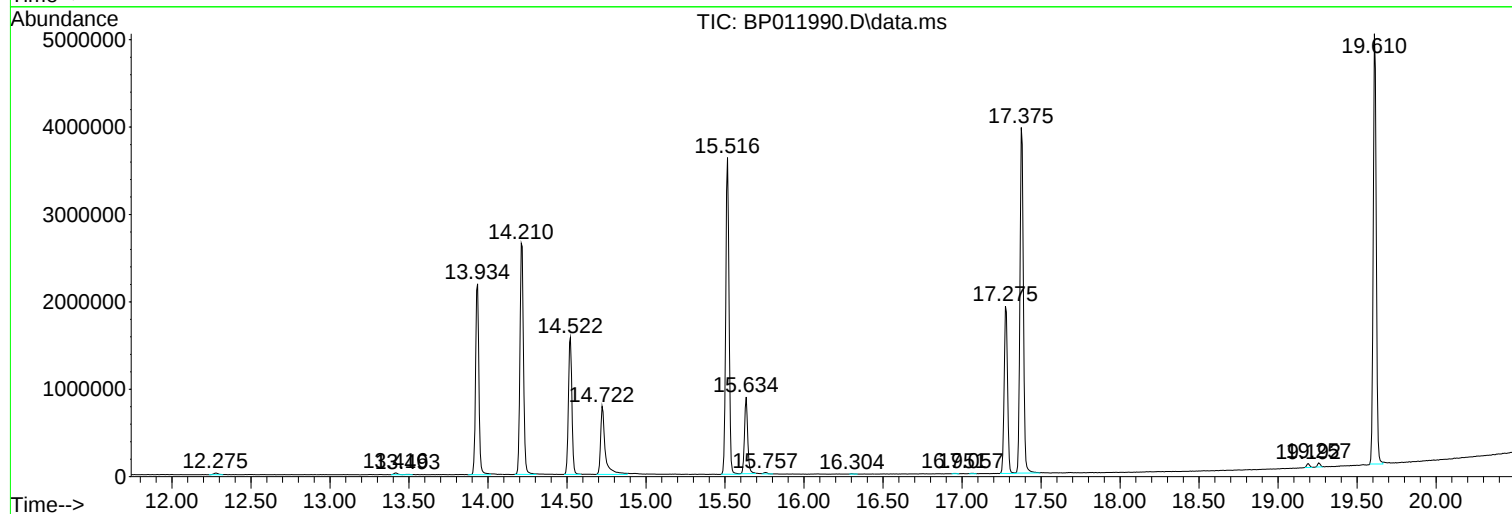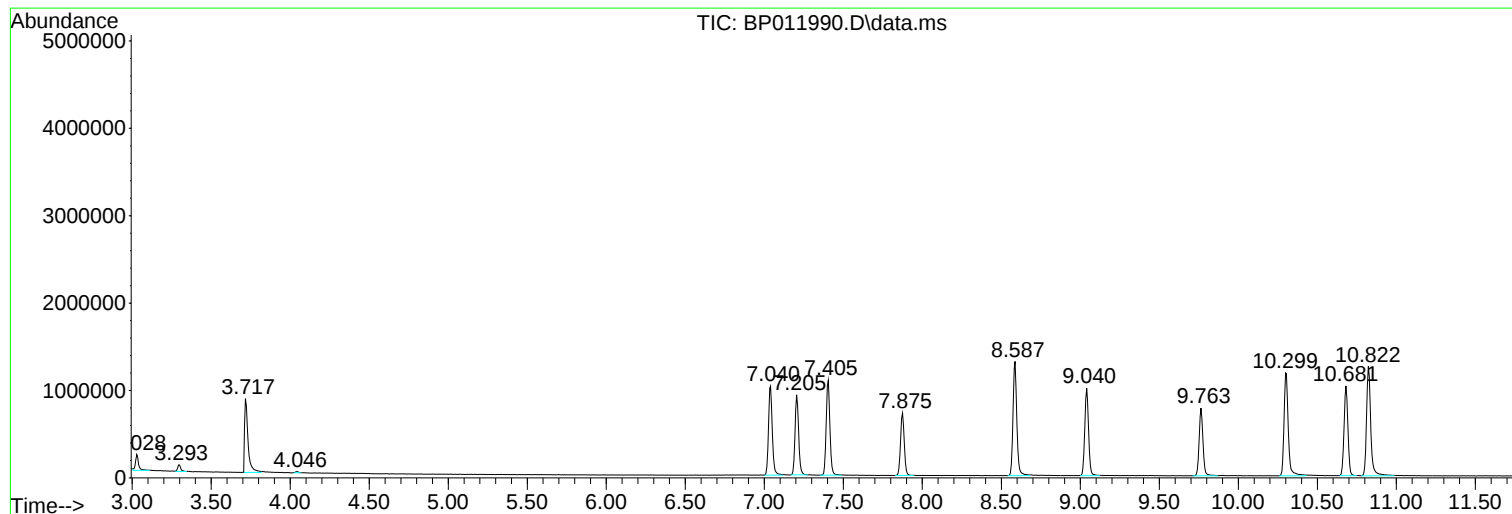

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011990.D
Acq On : 07 Oct 2022 03:11
Operator : CG/JU
Sample : PB148079BL
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK079










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	4.20 ng/ul	244261	1,4-Dichlorobenzene-d4	7.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12		
5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		

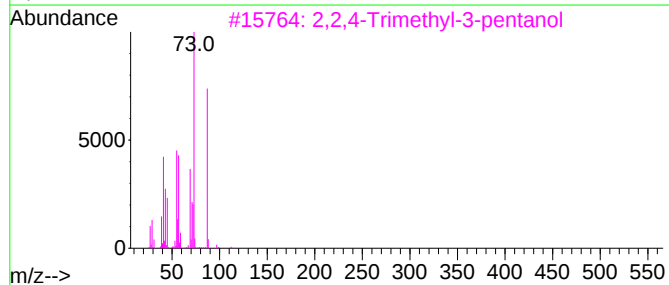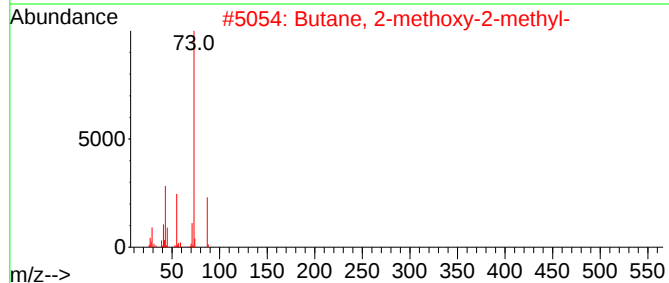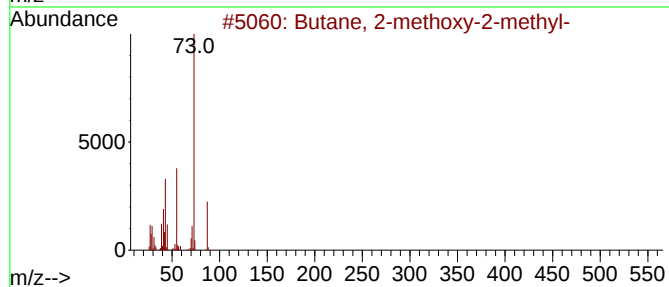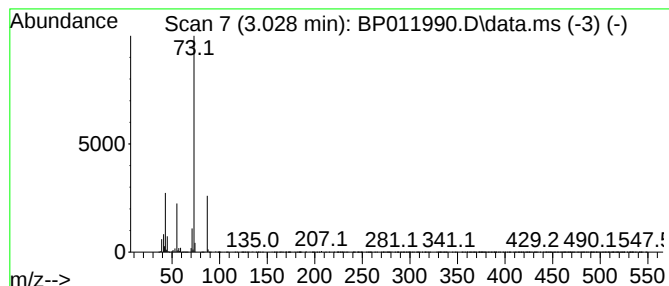

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100522\
Data File : BP011990.D
Acq On : 07 Oct 2022 03:11
Operator : CG/JU
Sample : PB148079BL
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK079

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	4.2	ng/u1	244261	1	7.875	1162070	20.0