
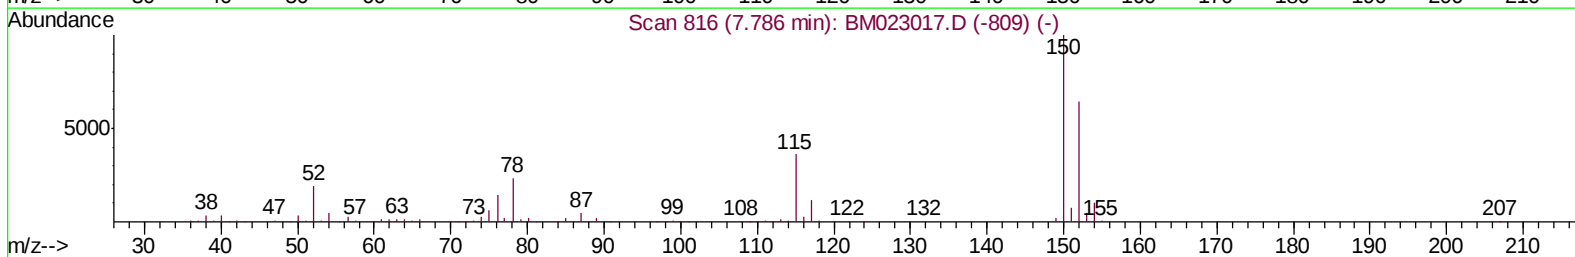
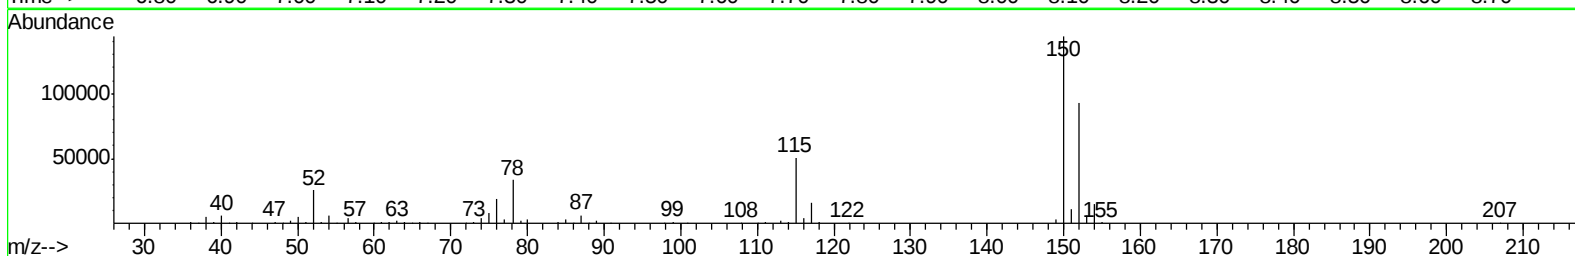


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100719\
Data File : BM023033.D
Acq On : 07 Oct 2019 15:43
Operator : JU
Sample : K5056-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB23

Quant Time: Oct 07 16:49:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 07 01:10:23 2019
Response via : Initial Calibration

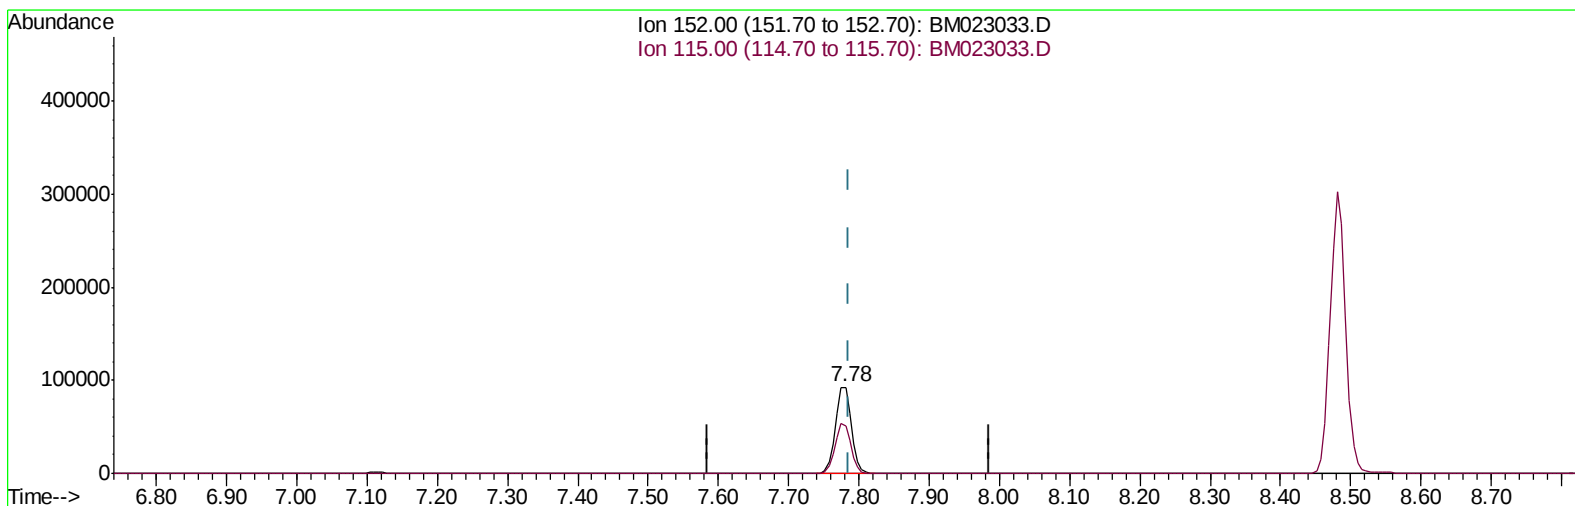

TIC: BM023033.D

(1) 1,4-Dichlorobenzene-d4 (I)

7.781min (-0.006) 20.00ng/ul




response 145820

Ion	Exp%	Act%
152.00	100	100
115.00	55.90	54.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100719\
Data File : BM023035.D
Acq On : 07 Oct 2019 16:55
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB23

Quant Time: Oct 07 17:54:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 07 16:37:53 2019
Response via : Initial Calibration

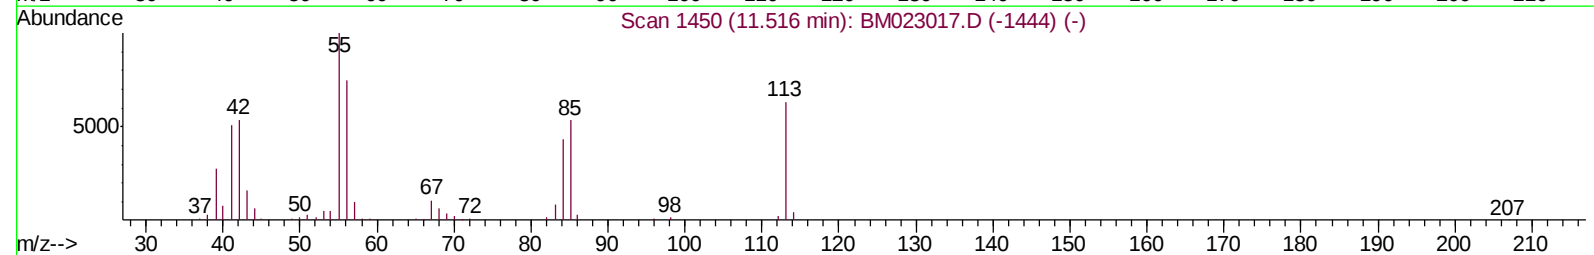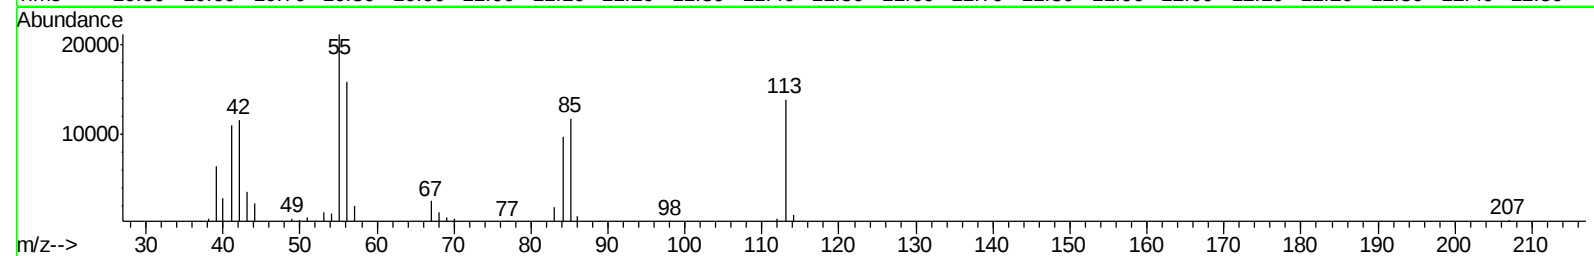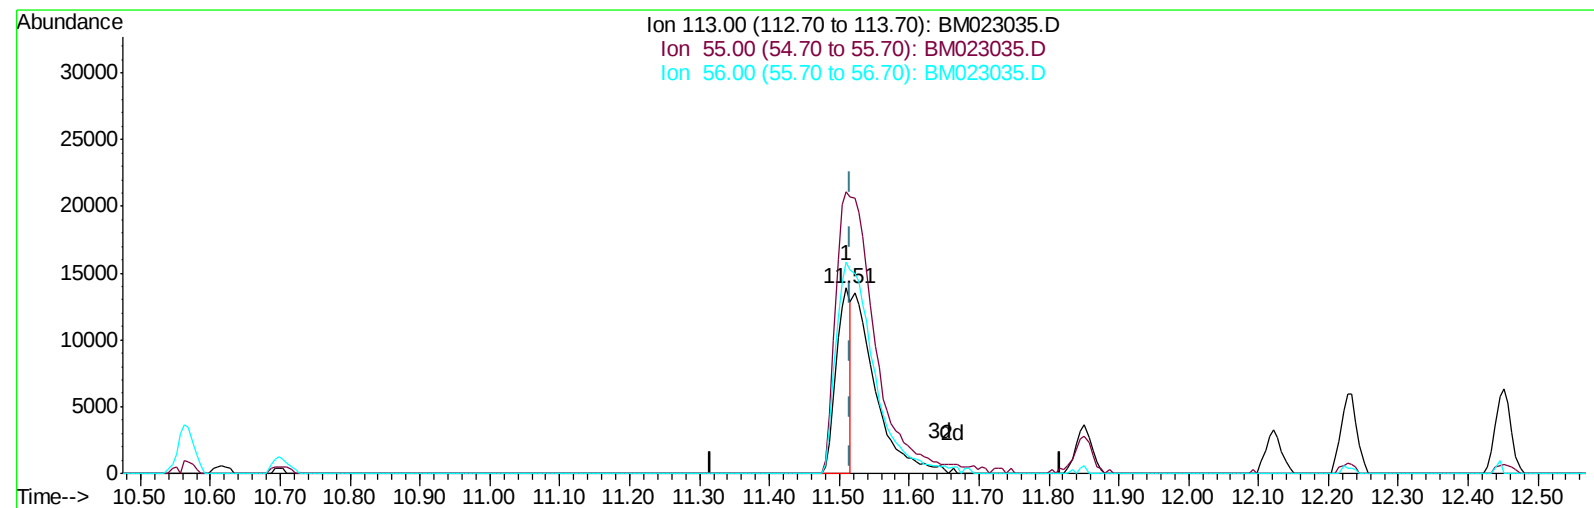

TIC: BM023035.D

(32) Caprolactam

11.510min (-0.006) 6.56ng/ul

response 20404

Ion	Exp%	Act%
113.00	100	100
55.00	150.70	152.17
56.00	114.30	114.03
0.00	0.00	0.00