
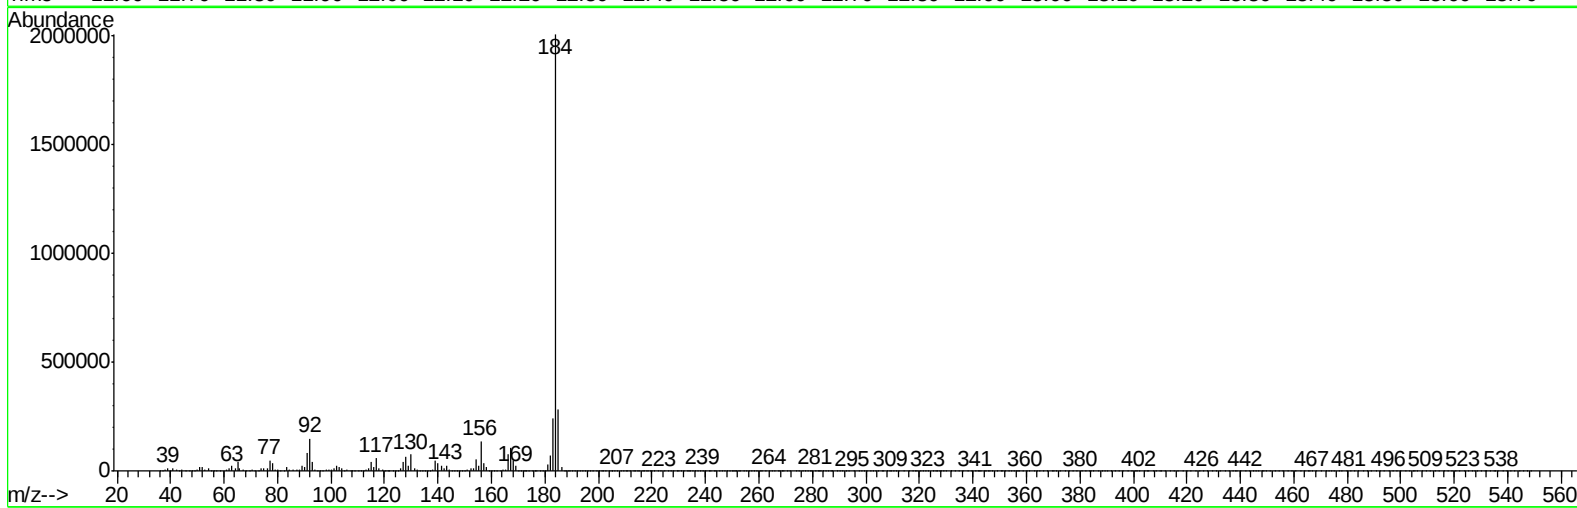


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100719\
 Data File : BP000535.D
 Acq On : 07 Oct 2019 10:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 07:36:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 01 18:03:42 2019
 Response via : Initial Calibration

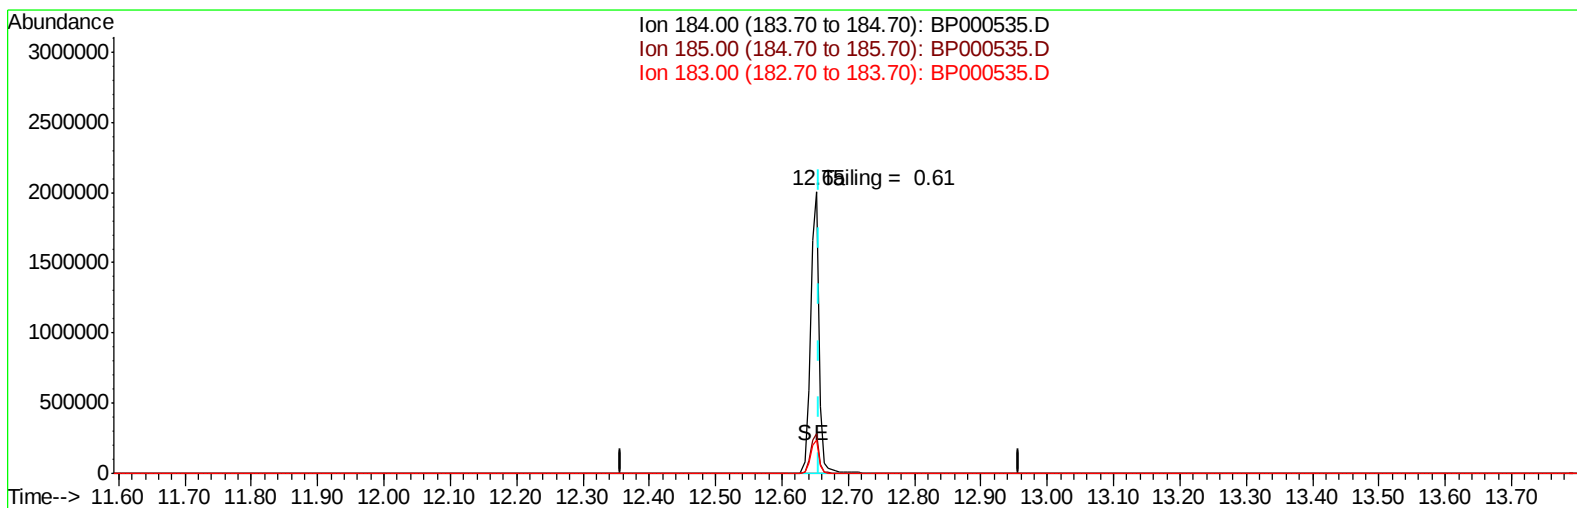

TIC: BP000535.D

(77) Benzidine



12.651min (-0.006) 129945.20ng

response 1787375

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	14.04
183.00	12.10	12.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100719\
 Data File : BP000535.D
 Acq On : 07 Oct 2019 10:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 07:36:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 01 18:03:42 2019
 Response via : Initial Calibration

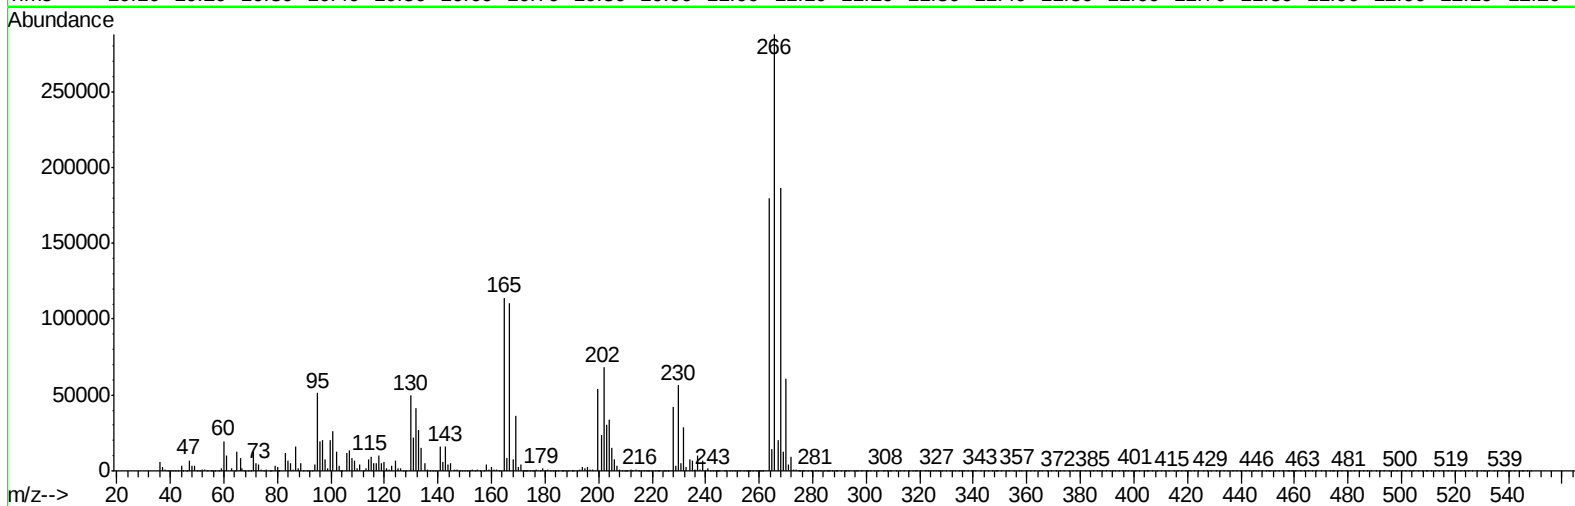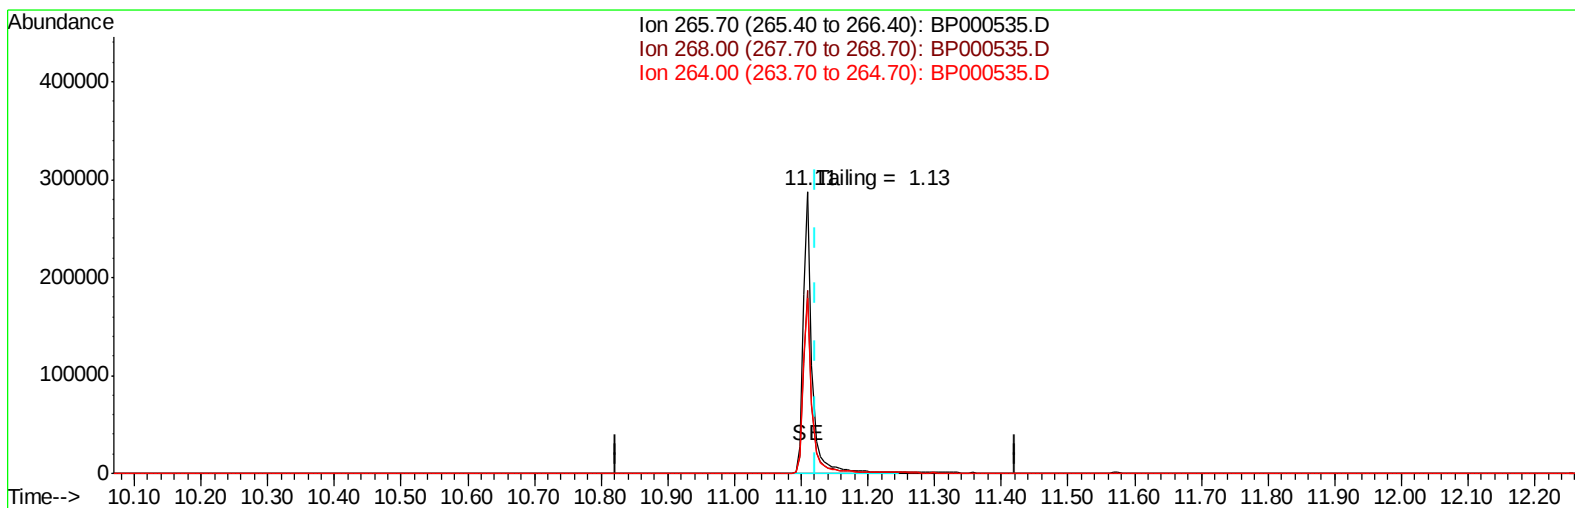

TIC: BP000535.D

(70) Pentachlorophenol (C)

11.110min (-0.012) 141164.85ng

response 259649

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	64.79
264.00	61.20	62.43
0.00	0.00	0.00