


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100719\
 Data File : BP000535.D
 Acq On : 07 Oct 2019 10:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 01 18:03:42 2019

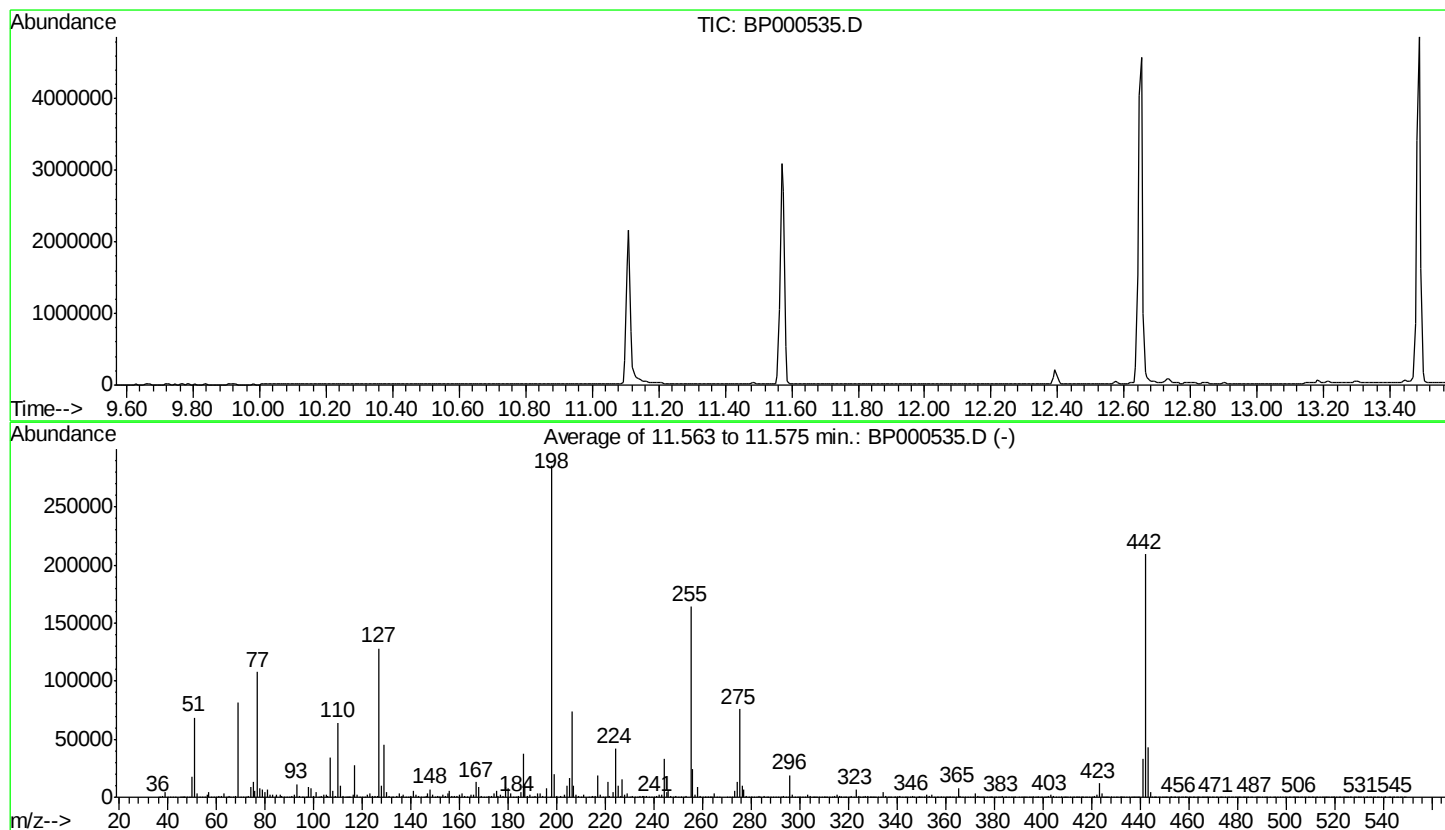

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	68625	PASS
68	69	0.00	2	1.9	1533	PASS
69	198	0.00	100	28.4	81120	PASS
70	69	0.00	2	0.6	501	PASS
127	198	10	80	44.8	127999	PASS
197	198	0.00	2	0.1	282	PASS
198	198	100	100	100.0	285686	PASS
199	198	5	9	6.9	19849	PASS
275	198	10	60	26.6	75912	PASS
365	198	1	100	2.9	8271	PASS
441	198	0.01	100	11.7	33357	PASS
442	198	50	100	73.2	209100	PASS
443	442	15	24	20.6	43055	PASS