

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100725\
 Data File : BP025949.D
 Acq On : 07 Oct 2025 19:21
 Operator : RC/JU
 Sample : Q3294-01 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HD-02-10062025

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.008	8	12	23	rVB	171755	226534	8.18%	1.190%
2	5.384	410	416	434	rBV	146205	308379	11.13%	1.620%
3	6.972	677	686	699	rBV2	73919	243249	8.78%	1.278%
4	7.737	808	816	830	rBV	693353	1262934	45.60%	6.633%
5	8.896	1005	1013	1030	rBV	63111	189249	6.83%	0.994%
6	10.496	1278	1285	1311	rBV	810749	1692830	61.12%	8.891%
7	12.966	1698	1705	1718	rBV	236217	450193	16.25%	2.365%
8	13.672	1819	1825	1830	rBV3	16218	32043	1.16%	0.168%
9	14.078	1888	1894	1898	rBV	35146	61544	2.22%	0.323%
10	14.348	1933	1940	1947	rBV	1217501	1975386	71.32%	10.375%
11	14.407	1948	1950	1962	rVB2	47704	86338	3.12%	0.453%
12	14.766	2006	2011	2016	rBV6	16737	33776	1.22%	0.177%
13	15.419	2117	2122	2131	rVB2	37797	77487	2.80%	0.407%
14	15.731	2169	2175	2191	rVB2	29882	92875	3.35%	0.488%
15	15.878	2195	2200	2208	rBV2	127020	248614	8.98%	1.306%
16	16.084	2231	2235	2237	rBV2	28958	39609	1.43%	0.208%
17	16.895	2370	2373	2377	rVV	20775	28605	1.03%	0.150%
18	16.954	2380	2383	2395	rVB3	41159	81991	2.96%	0.431%
19	17.142	2409	2415	2420	rBV2	1207120	1981696	71.55%	10.408%
20	17.189	2420	2423	2434	rVV	434862	722869	26.10%	3.797%
21	17.289	2435	2440	2446	rVB	85597	143500	5.18%	0.754%
22	17.584	2485	2490	2499	rBV2	25003	64601	2.33%	0.339%
23	17.660	2499	2503	2506	rBV	26256	37607	1.36%	0.198%
24	18.054	2566	2570	2571	rBV	79238	91500	3.30%	0.481%
25	18.189	2590	2593	2598	rVB	29911	37694	1.36%	0.198%
26	18.254	2598	2604	2608	rBV3	111479	206294	7.45%	1.083%
27	18.289	2608	2610	2621	rVB	62101	96768	3.49%	0.508%
28	18.378	2622	2625	2628	rBV	41502	46289	1.67%	0.243%
29	18.572	2654	2658	2663	rBV	38092	58129	2.10%	0.305%
30	18.631	2665	2668	2675	rVB4	34296	55894	2.02%	0.294%
31	19.001	2727	2731	2734	rBV	66270	112449	4.06%	0.591%
32	19.272	2772	2777	2785	rBV	728265	1126182	40.66%	5.915%
33	19.648	2833	2841	2850	rBV	670562	1259861	45.49%	6.617%
34	19.860	2872	2877	2882	rBV	438691	610874	22.06%	3.208%
35	20.166	2926	2929	2938	rVB2	134634	220081	7.95%	1.156%
36	20.272	2945	2947	2951	rVB	78007	85048	3.07%	0.447%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100725\
Data File : BP025949.D
Acq On : 07 Oct 2025 19:21
Operator : RC/JU
Sample : Q3294-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-02-10062025

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.583	3163	3170	3175	rBV2	1528061	2769670	100.00%	14.547%
38	24.942	3733	3741	3751	rVB	828515	2180979	78.75%	11.455%




Sum of corrected areas: 19039621

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100725\
Data File : BP025949.D
Acq On : 07 Oct 2025 19:21
Operator : RC/JU
Sample : Q3294-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-02-10062025

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

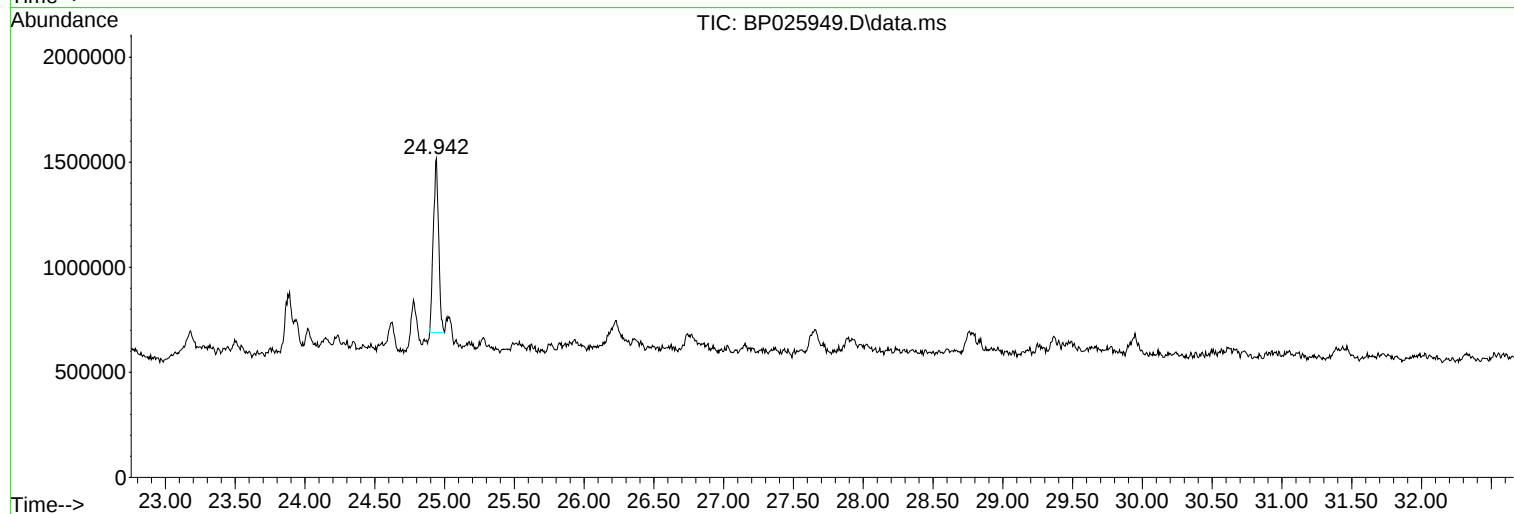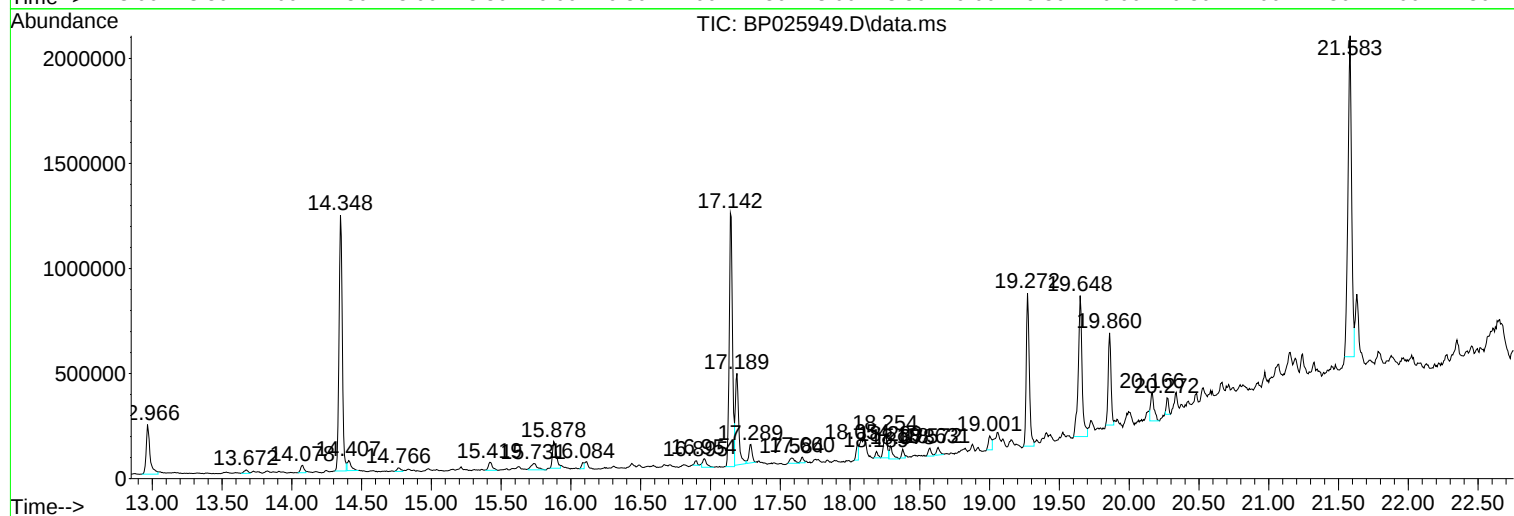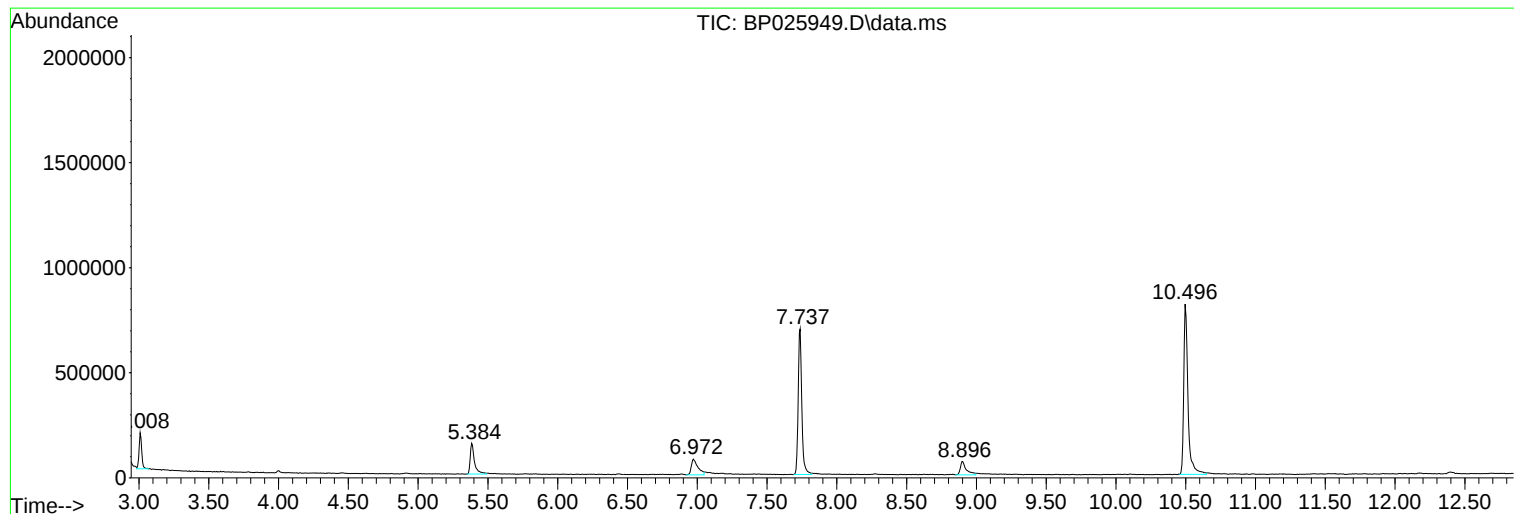

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100725\
Data File : BP025949.D
Acq On : 07 Oct 2025 19:21
Operator : RC/JU
Sample : Q3294-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-02-10062025

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100725\
Data File : BP025949.D
Acq On : 07 Oct 2025 19:21
Operator : RC/JU
Sample : Q3294-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HD-02-10062025

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------