


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100725\
Data File : BP025939.D
Acq On : 07 Oct 2025 10:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 19:16:54 2025

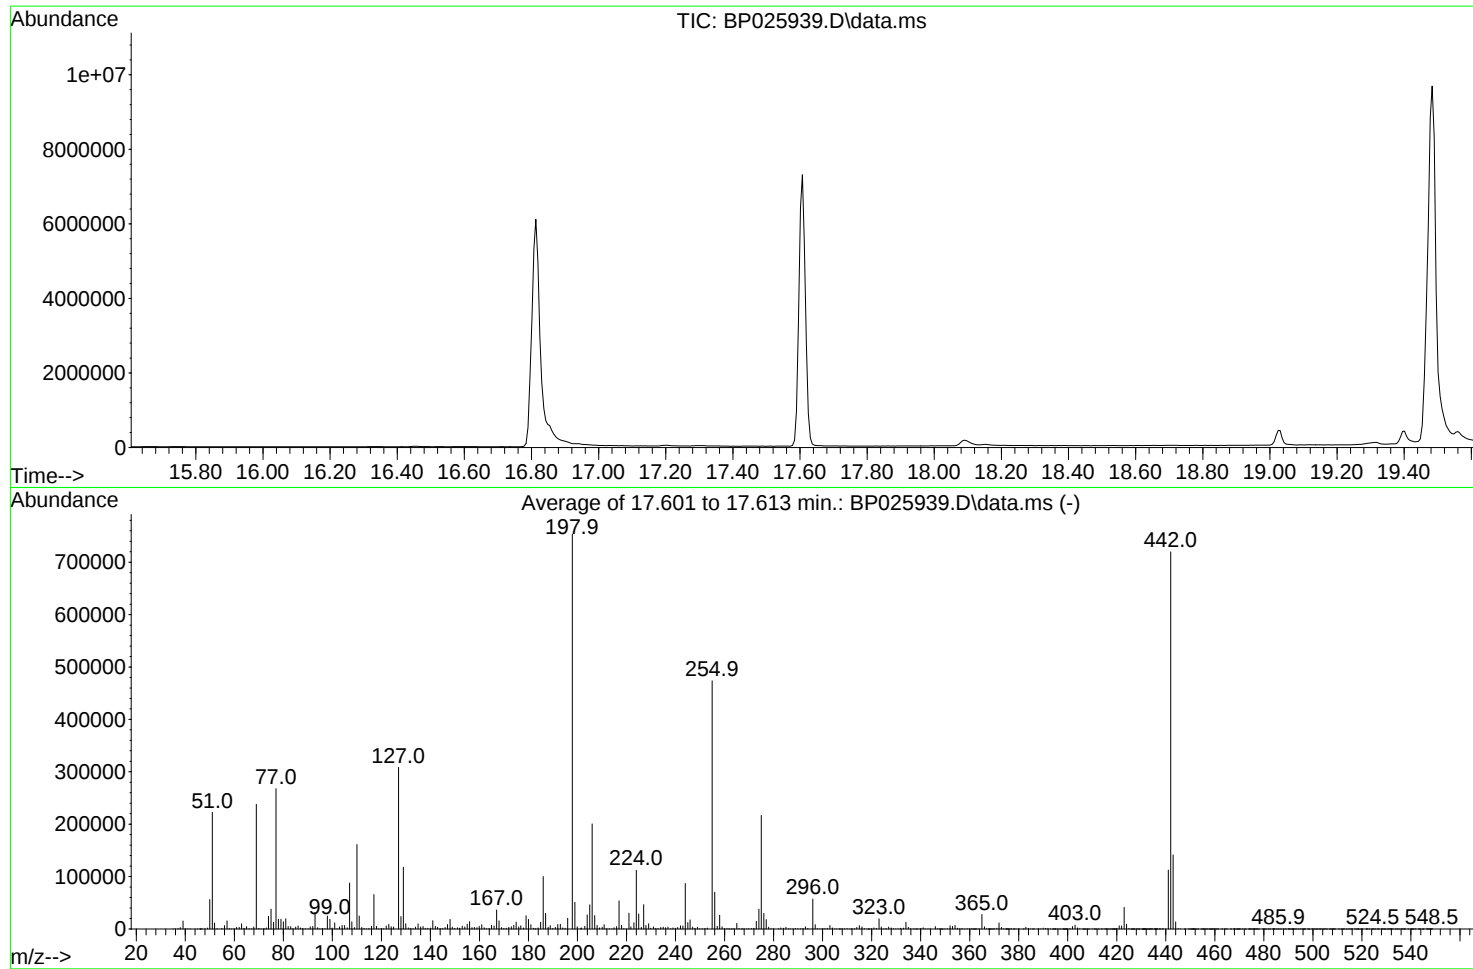




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2482

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	3862	PASS
69	69	100	100	100.0	237768	PASS
70	69	0.00	2	0.5	1144	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	753713	PASS
199	198	5	9	6.7	50777	PASS
365	198	1	100	3.7	27663	PASS
441	443	0.01	150	79.5	112192	PASS
442	442	100	100	100.0	719866	PASS
443	442	15	24	19.6	141192	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100725\
Data File : BP025939.D
Acq On : 07 Oct 2025 10:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 07 17:25:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 19:16:54 2025
Response via : Initial Calibration

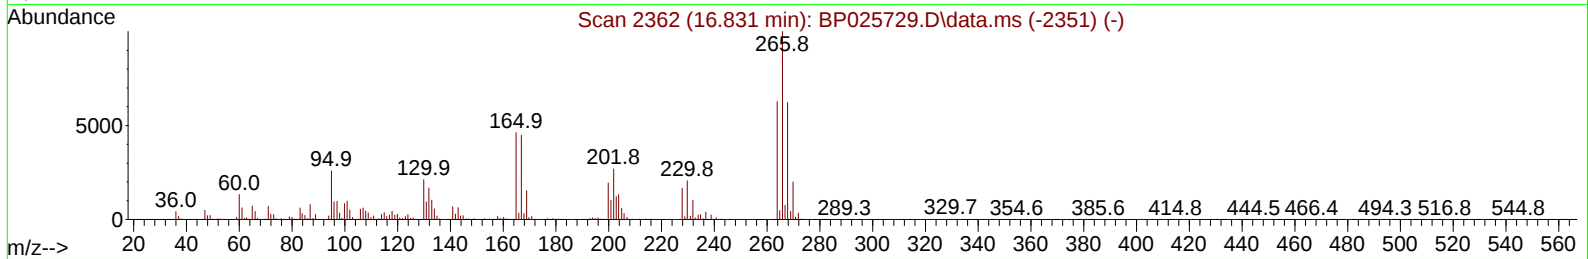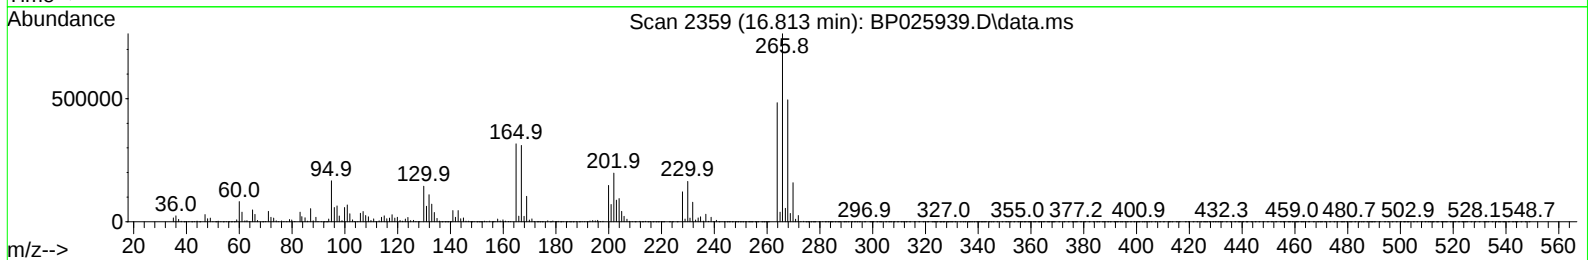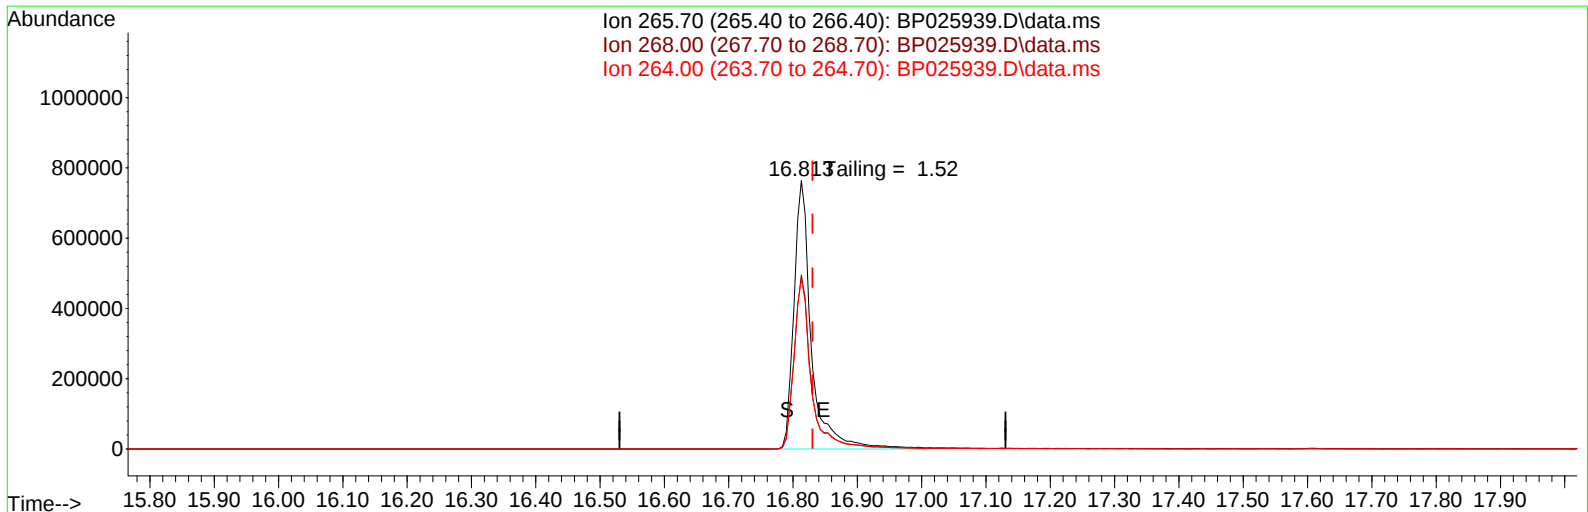

TIC: BP025939.D\data.ms

(70) Pentachlorophenol (C)

16.813min (-0.018) 8520531.03 ng m




response 1446782

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.90
264.00	62.70	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100725\
Data File : BP025939.D
Acq On : 07 Oct 2025 10:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 07 17:25:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 19:16:54 2025
Response via : Initial Calibration

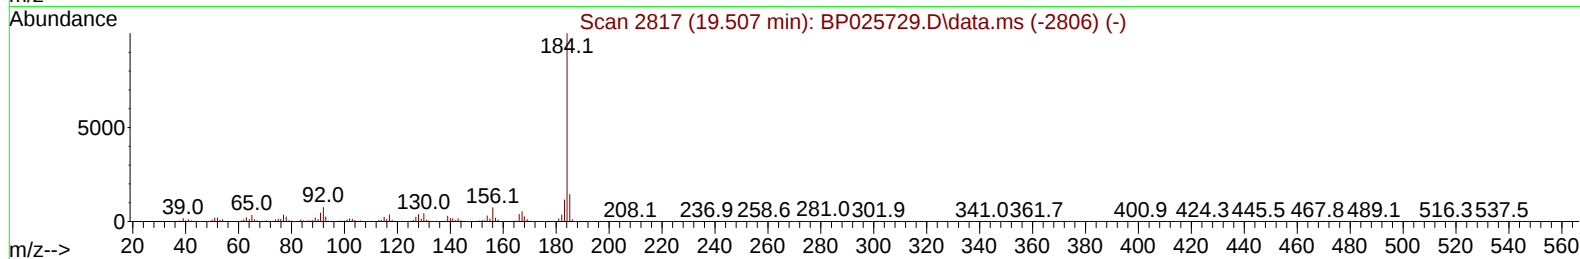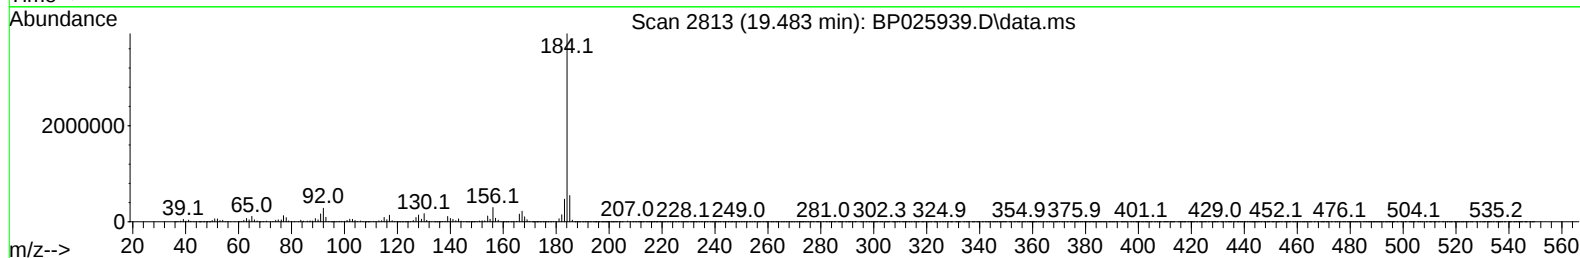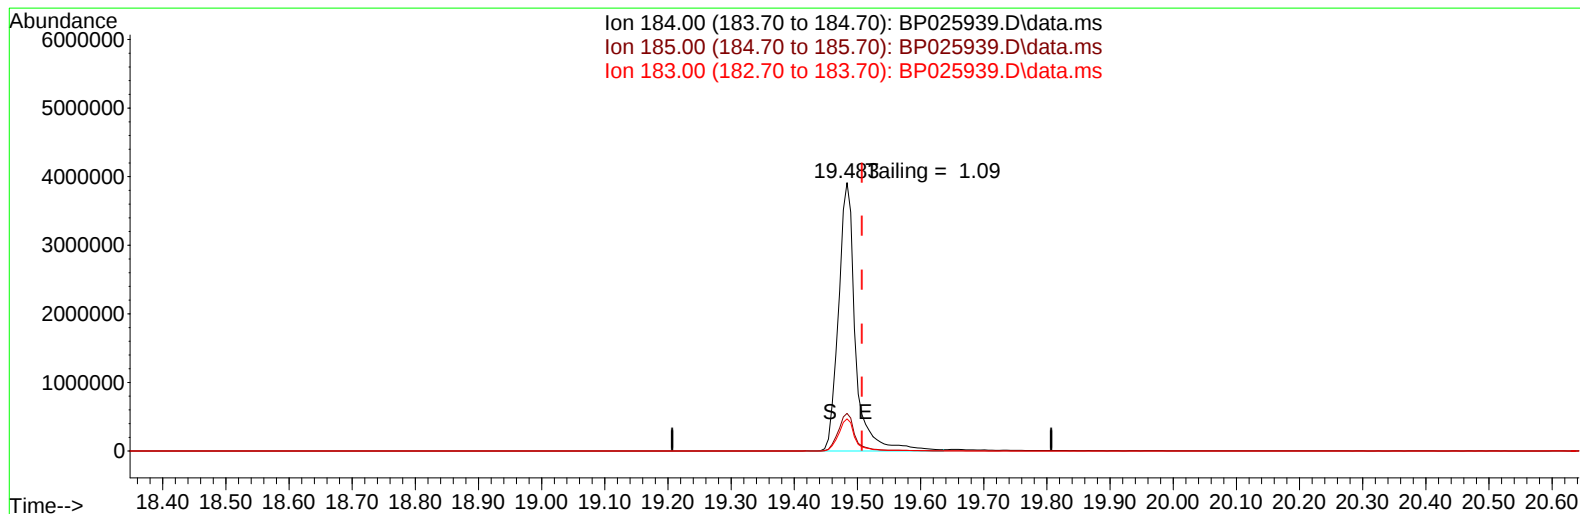

TIC: BP025939.D\data.ms

(77) Benzidine

19.483min (-0.023) 2303072.84 ng

response 7363831

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.00
183.00	11.50	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/7/2025	BNA_P	<u>BP025939.D</u>
Compound Name	Response	Retention Time
DDT	3076420	20.766
DDD	80878	20.307
DDE	1089	19.401
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
81967	3158387	2.60

Instrument :
BNA_P
ClientSampleId :
DFTPP